
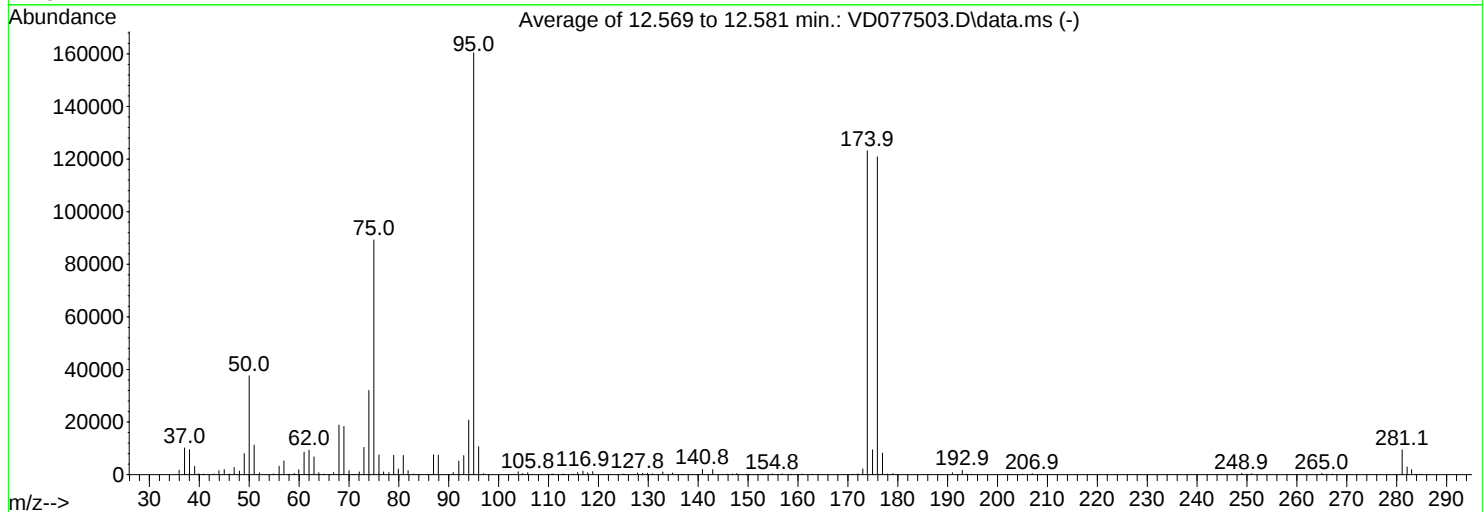


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110623\
 Data File : VD077503.D
 Acq On : 06 Nov 2023 09:14
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D103023S.M
 Title : SW846 8260
 Last Update : Tue Oct 31 04:19:17 2023

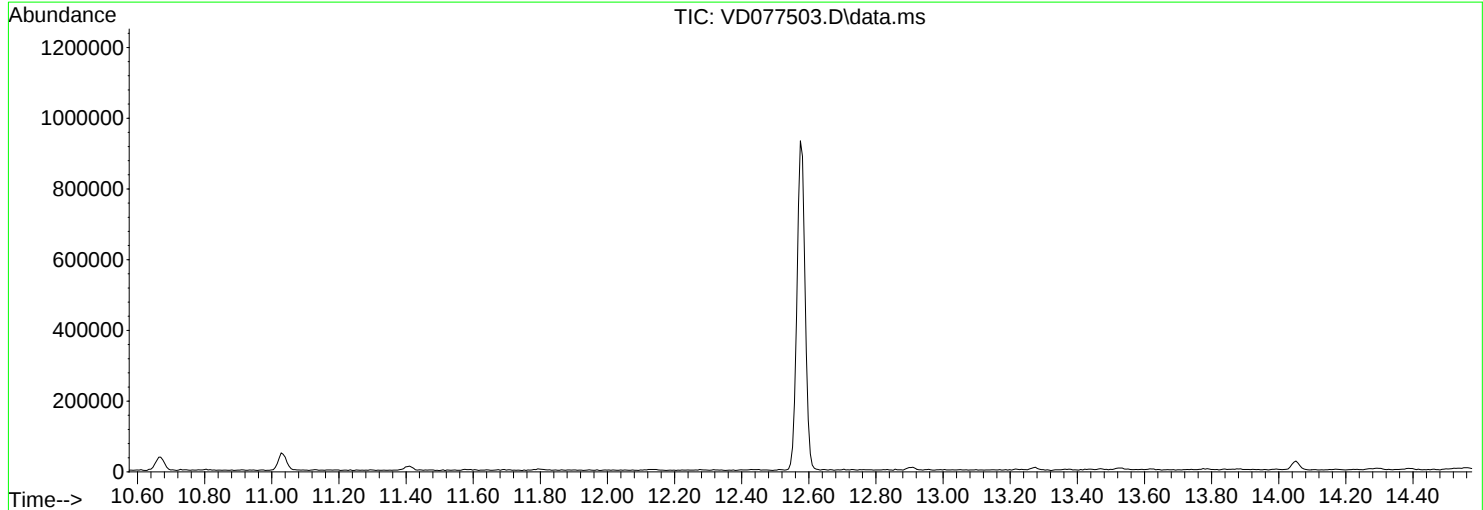

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	37608	PASS
75	95	30	60	55.7	89267	PASS
95	95	100	100	100.0	160405	PASS
96	95	5	9	6.6	10665	PASS
173	174	0.00	2	1.8	2213	PASS
174	95	50	100	76.8	123165	PASS
175	174	5	9	7.7	9457	PASS
176	174	95	101	98.1	120869	PASS
177	176	5	9	6.8	8240	PASS