

Data File : VD064168.D
Acq On : 08 Nov 2019 21:37
Operator : VA/SY
Sample : K5758-01
Misc : 5.09G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CO-1008

Quant Time: Nov 09 01:50:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 08 16:20:44 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	47384	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	73491	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	76347	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	44470	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.34	65	29172	74.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	149.72%	
35) Dibromofluoromethane	7.93	113	20086	47.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.22%	
50) Toluene-d8	10.34	98	88585	55.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.32%	
62) 4-Bromofluorobenzene	12.64	95	39425	71.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	143.08%	

Target Compounds


						Qvalue
2) Dichlorodifluoromethane	2.03	85	736	1.873	ug/l	85
3) Chloromethane	2.21	50	907	2.152	ug/l #	42
5) Bromomethane	2.79	94	538	1.890	ug/l #	19
10) Methyl Iodide	4.31	142	71	2.174	ug/l #	39
13) Acrolein	3.93	56	364	15.808	ug/l #	74
16) Acetone	4.17	43	17523	189.804	ug/l #	82
18) Methyl Acetate	4.73	43	313	1.214	ug/l #	53
20) Methylene Chloride	4.96	84	1262	2.706	ug/l #	78
21) trans-1,2-Dichloroethene	5.47	96	472	1.046	ug/l #	1
25) 2-Butanone	7.23	43	4126	34.593	ug/l	91
29) Tetrahydrofuran	7.58	42	683	9.531	ug/l #	55
31) Cyclohexane	7.99	56	1256	1.642	ug/l #	7
32) 1,1,1-Trichloroethane	7.91	97	753	1.014	ug/l #	24
36) 1,1-Dichloropropene	7.97	75	3672	5.414	ug/l #	53
37) Ethyl Acetate	7.31	43	523	1.829	ug/l #	76
38) Carbon Tetrachloride	7.98	117	4169	5.744	ug/l #	12
41) Methacrylonitrile	7.53	41	280	1.558	ug/l #	29
48) Methyl methacrylate	9.48	41	686	2.381	ug/l #	58
51) 4-Methyl-2-Pentanone	10.23	43	2497	8.838	ug/l #	48
55) 1,1,2-Trichloroethane	10.81	97	957	2.921	ug/l #	37
59) 2-Hexanone	10.99	43	1894	9.423	ug/l	89
75) 1,1,2,2-Tetrachloroethane	12.74	83	891	1.812	ug/l #	89
76) 1,2,3-Trichloropropane	12.64	75	20484	57.187	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.64	75	20484	113.596	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	14.52	75	120	1.365	ug/l #	1
95) Naphthalene	15.41	128	2016	1.280	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VD064168.D
Acq On : 08 Nov 2019 21:37
Operator : VA/SY
Sample : K5758-01
Misc : 5.09G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CO-1008

Quant Time: Nov 09 01:50:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 08 16:20:44 2019
Response via : Initial Calibration

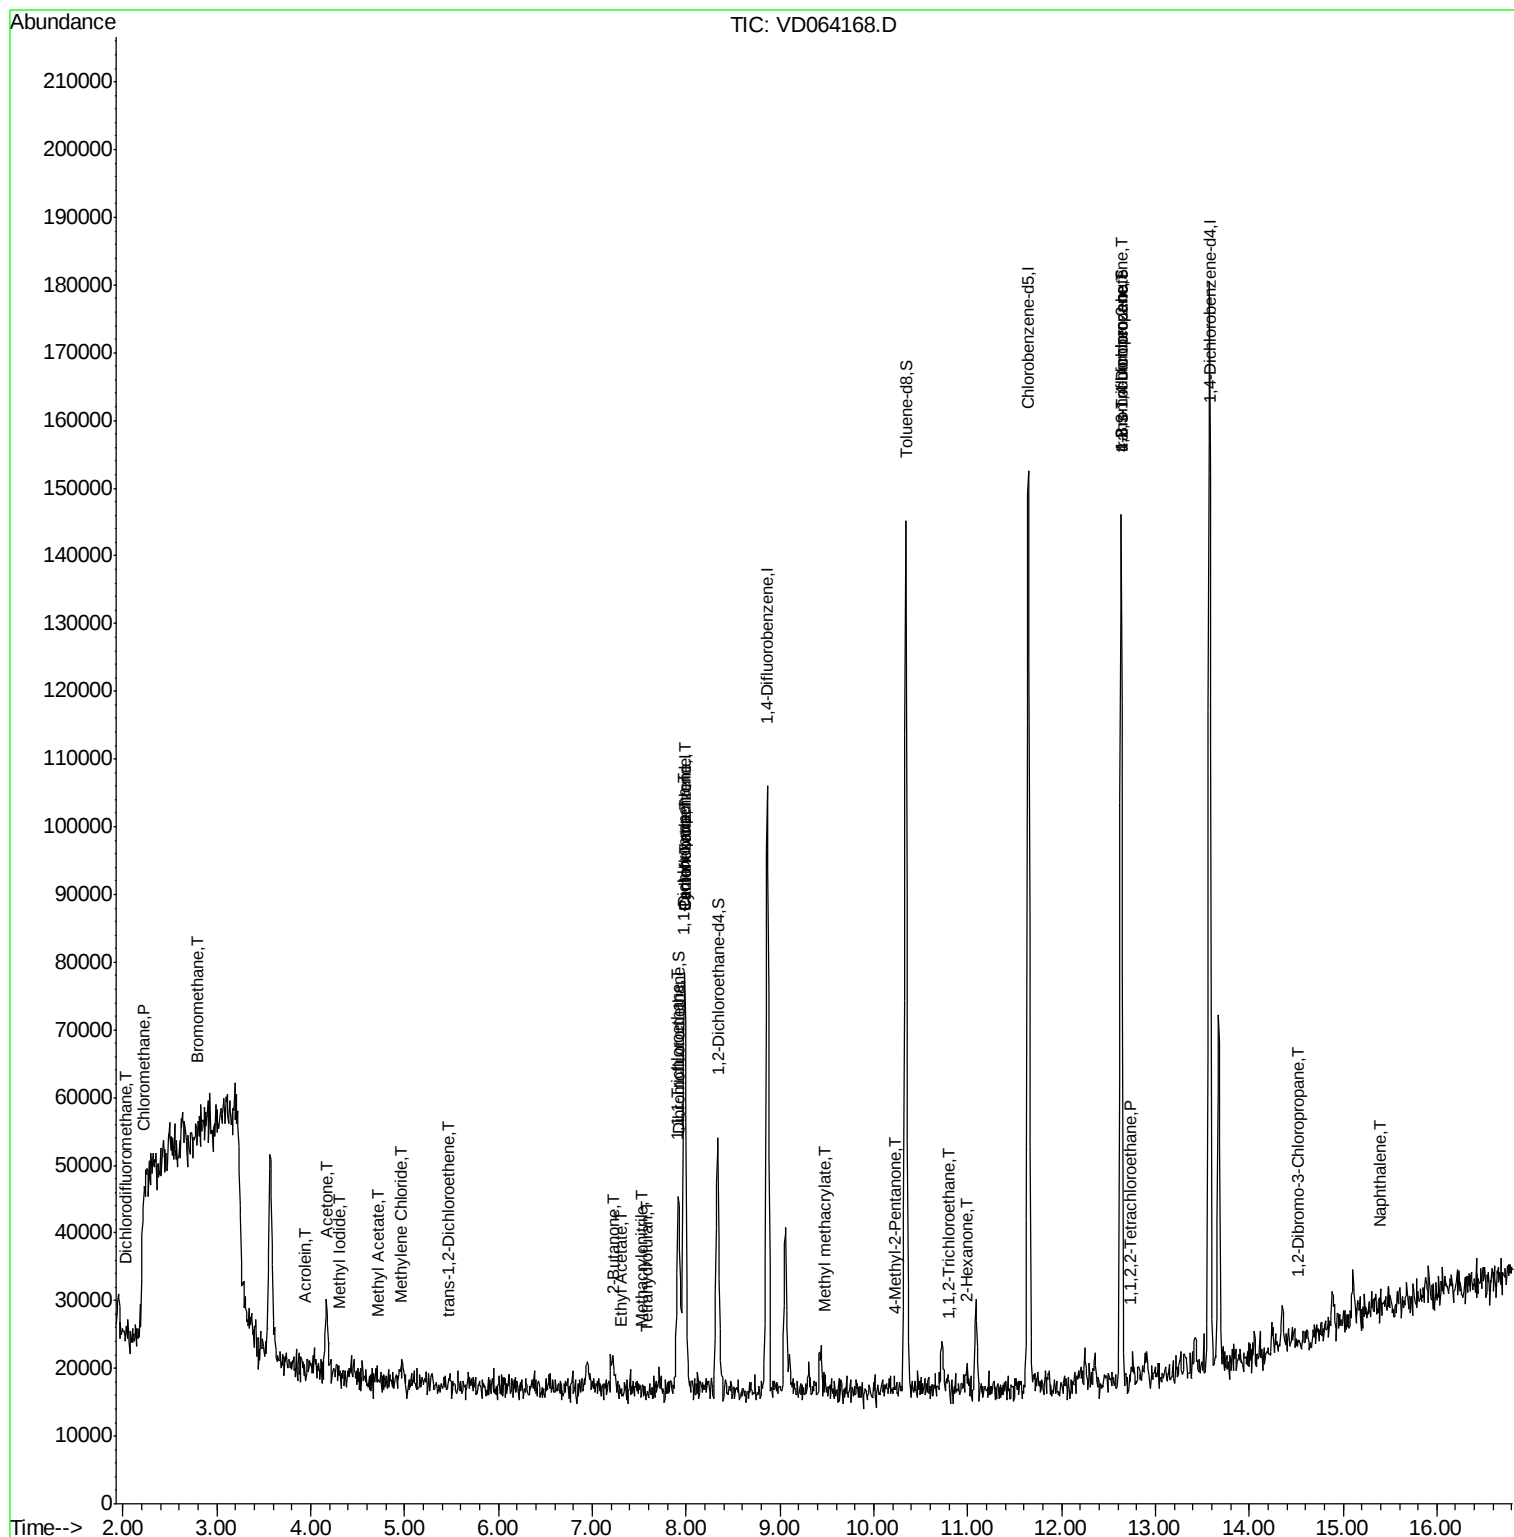

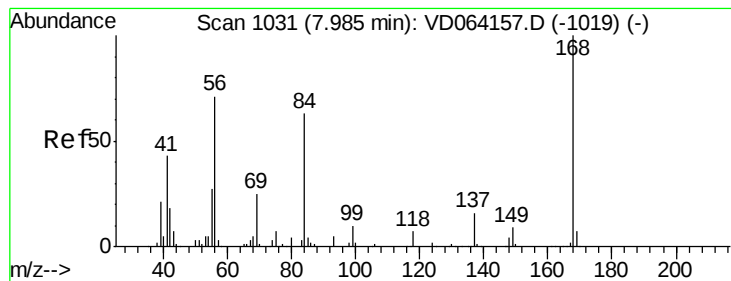

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampleId :


CO-1008

Tgt Ion:168 Resp: 47384

Ion Ratio Lower Upper

168 100

99 47.6 41.6 62.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

25000

20000

15000



10000

5000

0

7.90 7.95 8.00 8.05

Time-->



#2

Dichlorodifluoromethane

Concen: 1.873 ug/l

RT: 2.03 min Scan# 18

Delta R.T. 0.04 min

Lab File: VD064168.D


Acq: 08 Nov 2019 21:37

Tgt Ion: 85 Resp: 736

Ion Ratio Lower Upper

85 100

87 24.1 16.4 49.2



Abundance Ion 84.90 (84.60 to 85.60): VDC

Ion 86.90 (86.60 to 87.60): VDC

2.03

1200

1000

800

600


400


200

0

2.00 2.02 2.04 2.06

Time-->



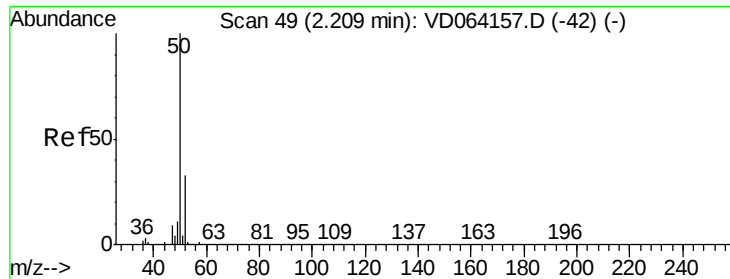

#3

Chloromethane

Concen: 2.152 ug/l

RT: 2.21 min Scan# 50

Delta R.T. 0.01 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampleId :


CO-1008

Tgt Ion: 50 Resp: 907

Ion Ratio Lower Upper




50 100

52 0.0 26.2 39.4#



Abundance Ion 49.90 (49.60 to 50.60): VDC

Ion 51.90 (51.60 to 52.60): VDC

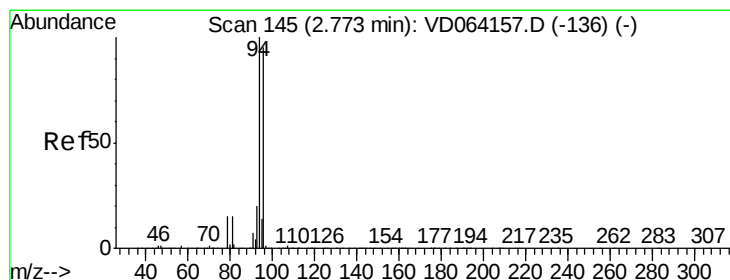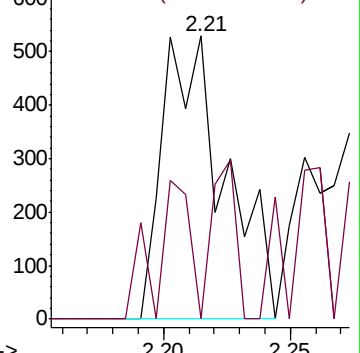

#5

Bromomethane

Concen: 1.890 ug/l

RT: 2.79 min Scan# 148

Delta R.T. 0.02 min

Lab File: VD064168.D


Acq: 08 Nov 2019 21:37

Tgt Ion: 94 Resp: 538

Ion Ratio Lower Upper



94 100


96 16.1 76.2 114.4#



Abundance Ion 93.90 (93.60 to 94.60): VDC

Ion 95.90 (95.60 to 96.60): VDC




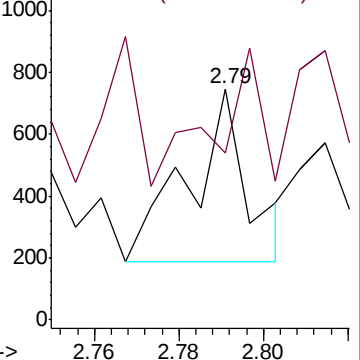


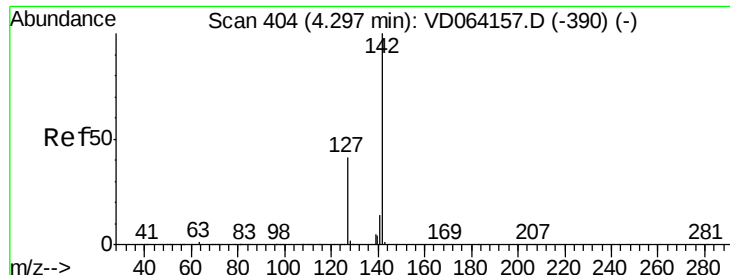

#10
Methyl Iodide
Concen: 2.174 ug/l
RT: 4.31 min Scan# 406
Delta R.T. 0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37




Instrument :
MSVOA_D
ClientSampleId :
CO-1008


Tgt Ion: 142 Resp: 71
Ion Ratio Lower Upper
142 100
127 87.3 34.4 51.6#
141 0.0 11.2 16.8#

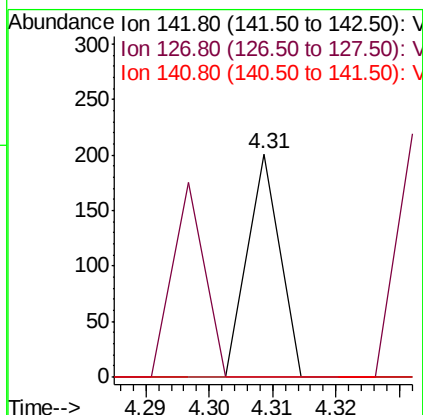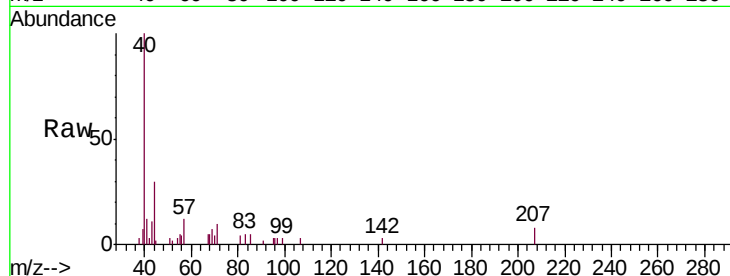

#13
Acrolein
Concen: 15.808 ug/l
RT: 3.93 min Scan# 342
Delta R.T. 0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 56 Resp: 364
Ion Ratio Lower Upper
56 100
55 48.6 56.1 84.1#



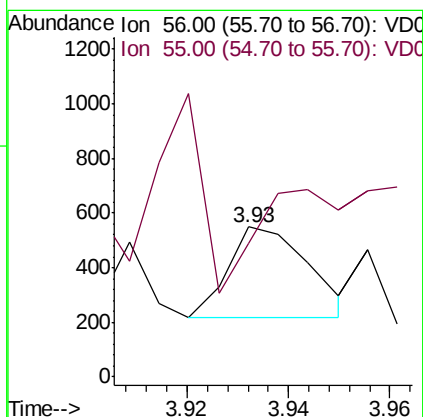
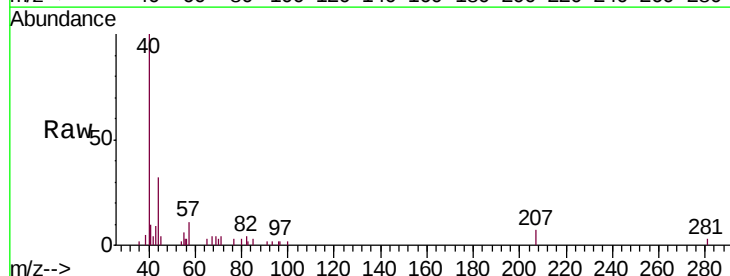




#16
Acetone
Concen: 189.804 ug/l
RT: 4.17 min Scan# 383
Delta R.T. 0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37




Instrument :
MSVOA_D
ClientSampleId :
CO-1008


Tgt Ion: 43 Resp: 17523
Ion Ratio Lower Upper
43 100
58 20.6 24.1 36.1#

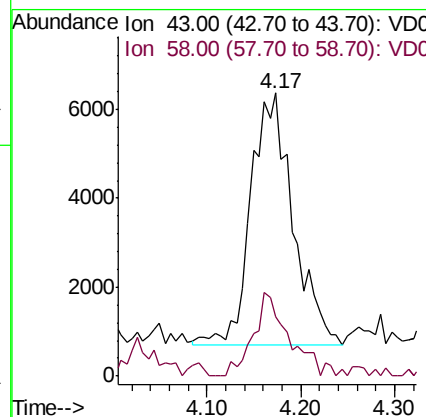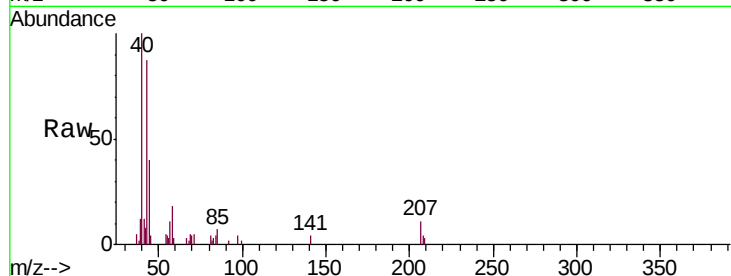

#18
Methyl Acetate
Concen: 1.214 ug/l
RT: 4.73 min Scan# 477
Delta R.T. 0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 43 Resp: 313
Ion Ratio Lower Upper
43 100
74 0.0 18.4 27.6#



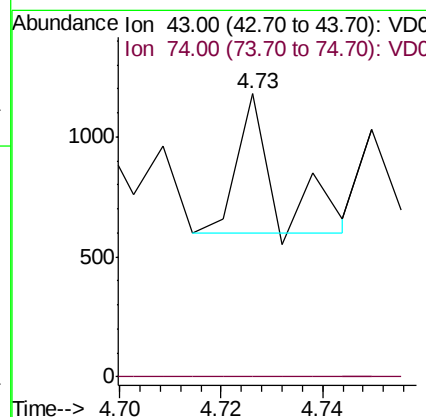





#20
Methylene Chloride
Concen: 2.706 ug/l
RT: 4.96 min Scan# 517
Delta R.T. -0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37




Instrument :
MSVOA_D
ClientSampleId :
CO-1008


Tgt Ion: 84 Resp: 1262
Ion Ratio Lower Upper
84 100
49 100.9 102.1 153.1#
51 34.8 32.2 48.2
86 39.4 49.9 74.9#

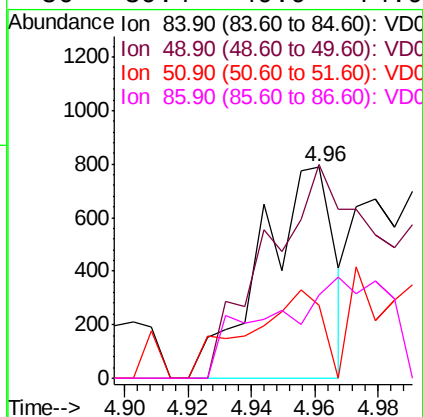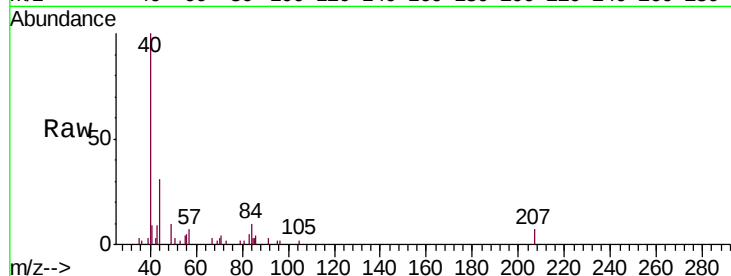

#21
trans-1,2-Dichloroethene
Concen: 1.046 ug/l
RT: 5.47 min Scan# 604
Delta R.T. -0.00 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 96 Resp: 472
Ion Ratio Lower Upper
96 100
61 0.0 111.8 167.6#
98 0.0 50.3 75.5#

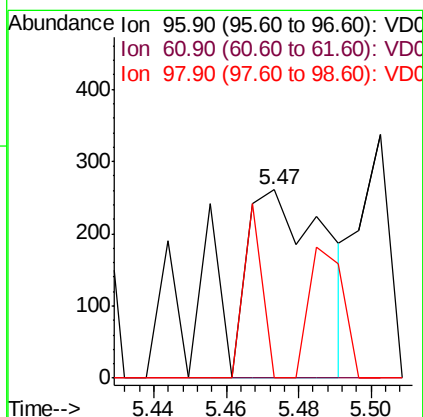



#25

2-Butanone

Concen: 34.593 ug/l

RT: 7.23 min Scan# 902

Delta R.T. -0.00 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampleId :


CO-1008

Tgt Ion: 43 Resp: 4126

Ion Ratio Lower Upper




43 100

72 20.9 20.6 30.8



Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 72.00 (71.70 to 72.70): VDC

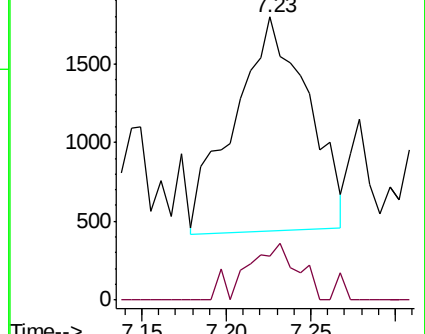

#29

Tetrahydrofuran

Concen: 9.531 ug/l

RT: 7.58 min Scan# 962

Delta R.T. 0.01 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37


Tgt Ion: 42 Resp: 683

Ion Ratio Lower Upper

42 100

72 0.0 33.4 50.2#



71 52.4 31.0 46.4#




Abundance Ion 42.00 (41.70 to 42.70): VDC

Ion 72.00 (71.70 to 72.70): VDC

Ion 71.00 (70.70 to 71.70): VDC

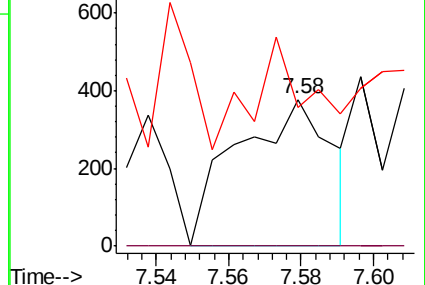


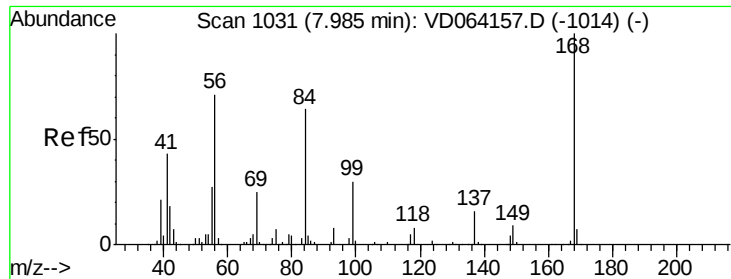




#31
Cyclohexane
Concen: 1.642 ug/l
RT: 7.99 min Scan# 1032
Delta R.T. 0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Instrument :
MSVOA_D
ClientSampled :
CO-1008

Tgt Ion: 56 Resp: 1256
Ion Ratio Lower Upper
56 100
69 113.9 28.2 42.4#
84 161.1 71.8 107.6#

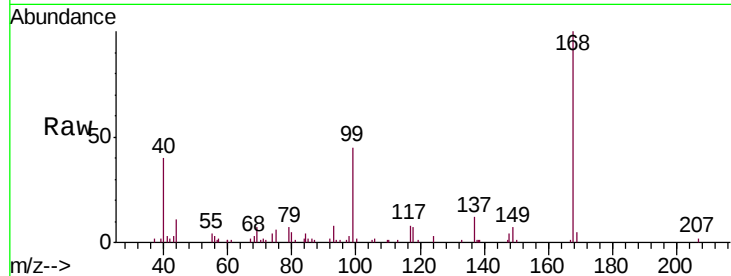


Abundance Ion 56.00 (55.70 to 56.70): VDC
Ion 69.00 (68.70 to 69.70): VDC
Ion 84.00 (83.70 to 84.70): VDC


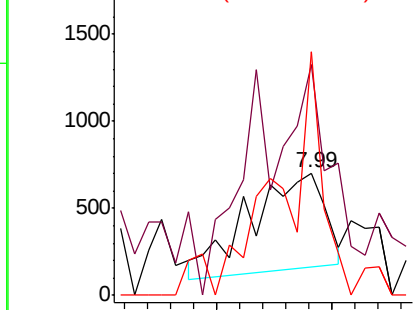



#32
1,1,1-Trichloroethane
Concen: 1.014 ug/l
RT: 7.91 min Scan# 1018
Delta R.T. -0.00 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 97 Resp: 753
Ion Ratio Lower Upper
97 100
99 0.0 51.6 77.4#
61 0.0 34.2 51.2#



Abundance Ion 96.90 (96.60 to 97.60): VDC
Ion 98.90 (98.60 to 99.60): VDC
Ion 60.90 (60.60 to 61.60): VDC




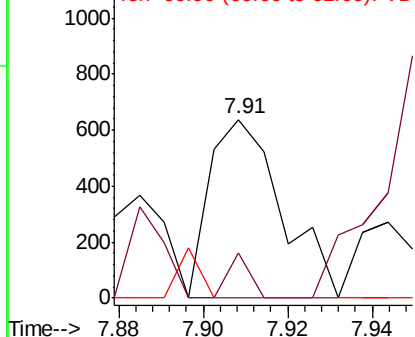




#33
 1,2-Dichloroethane-d4
 Concen: 74.857 ug/l
 RT: 8.34 min Scan# 1091
 Delta R.T. -0.00 min
 Lab File: VD064168.D
 Acq: 08 Nov 2019 21:37




Instrument :
 MSVOA_D
 ClientSampleId :
 CO-1008


Tgt Ion: 65 Resp: 29172
 Ion Ratio Lower Upper
 65 100
 67 58.4 0.0 104.4

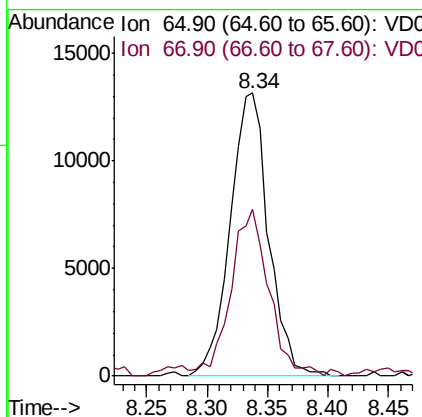

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. -0.00 min
 Lab File: VD064168.D
 Acq: 08 Nov 2019 21:37

Tgt Ion: 114 Resp: 73491
 Ion Ratio Lower Upper
 114 100
 63 21.1 0.0 40.0
 88 15.8 0.0 30.2

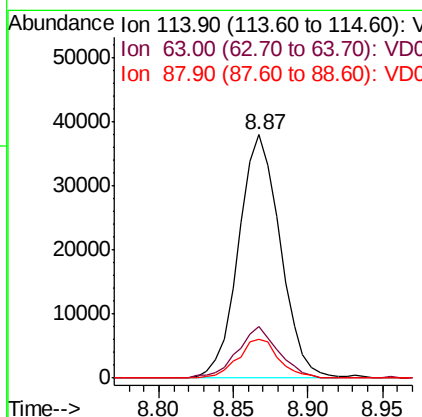



#35

Dibromofluoromethane

Concen: 47.614 ug/l

RT: 7.93 min Scan# 1021

Delta R.T. 0.01 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampleId :

CO-1008


Tgt Ion:113 Resp: 20086

Ion Ratio Lower Upper

113 100

111 102.5 81.5 122.3




192 23.7 18.8 28.2



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

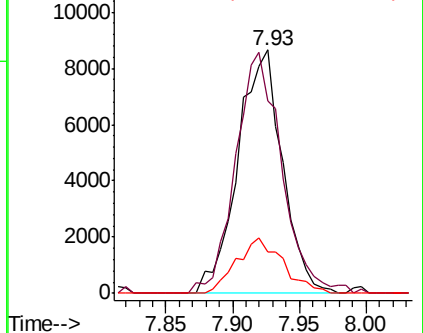

#36

1,1-Dichloropropene

Concen: 5.414 ug/l

RT: 7.97 min Scan# 1029

Delta R.T. -0.14 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37


Tgt Ion: 75 Resp: 3672

Ion Ratio Lower Upper

75 100

110 14.1 18.3 54.9#



77 0.0 25.0 37.6#




Abundance Ion 74.90 (74.60 to 75.60): V

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): V

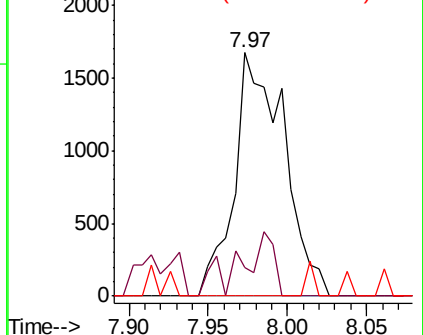







#37
Ethyl Acetate
Concen: 1.829 ug/l
RT: 7.31 min Scan# 916
Delta R.T. 0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Instrument :
MSVOA_D
ClientSampled :
CO-1008

Tgt Ion: 43 Resp: 523
Ion Ratio Lower Upper
43 100
61 0.0 10.2 15.2#
70 16.3 8.5 12.7#




Abundance Ion 43.00 (42.70 to 43.70): VDC
Ion 60.90 (60.60 to 61.60): VDC
Ion 70.00 (69.70 to 70.70): VDC


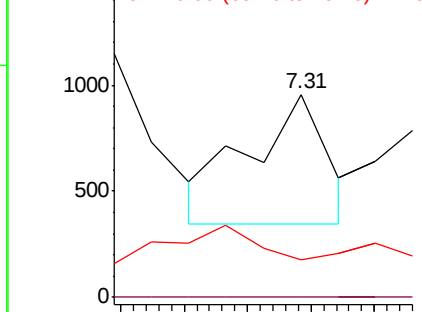



#38
Carbon Tetrachloride
Concen: 5.744 ug/l
RT: 7.98 min Scan# 1031
Delta R.T. -0.11 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 117 Resp: 4169
Ion Ratio Lower Upper
117 100
119 0.0 77.2 115.8#
121 0.0 25.5 38.3#



Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

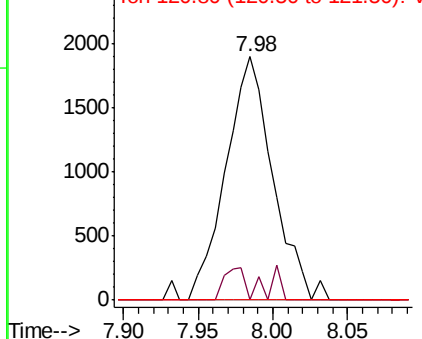



#41

Methacrylonitrile

Concen: 1.558 ug/l

RT: 7.53 min Scan# 953

Delta R.T. -0.01 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampled :

CO-1008

Tgt Ion: 41 Resp: 280





Ion Ratio Lower Upper

41 100

39 0.0 49.4 74.2#

67 116.1 49.6 74.4#

52 0.0 21.4 32.0#

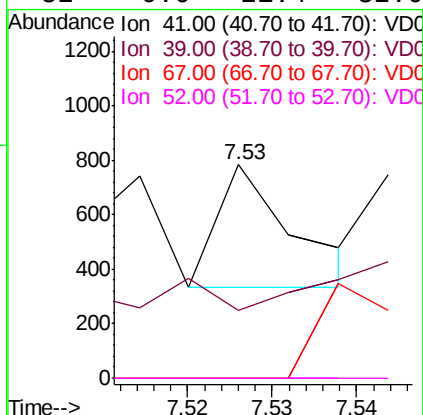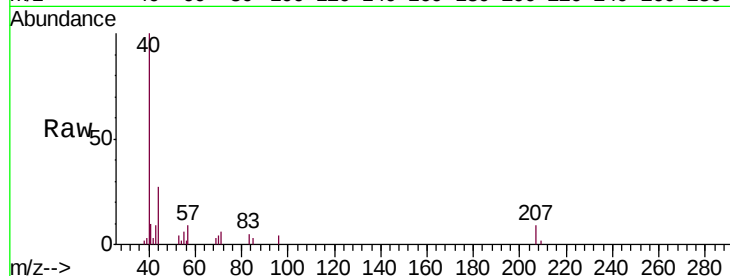

#48

Methyl methacrylate

Concen: 2.381 ug/l

RT: 9.48 min Scan# 1285

Delta R.T. 0.02 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37




Tgt Ion: 41 Resp: 686


Ion Ratio Lower Upper

41 100

69 91.3 64.6 97.0

39 123.2 48.2 72.2#


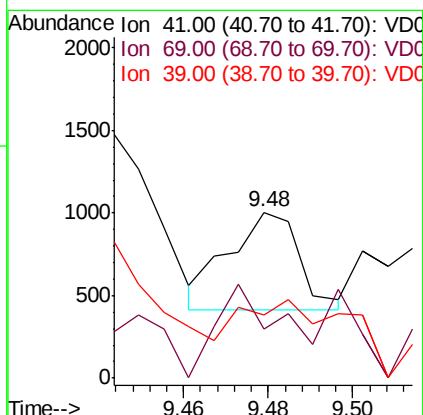






#50
Toluene-d8
Concen: 55.665 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. -0.00 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37




Instrument :
MSVOA_D
ClientSampled :
CO-1008


Tgt Ion: 98 Resp: 88585
Ion Ratio Lower Upper
98 100
100 64.6 52.6 78.8

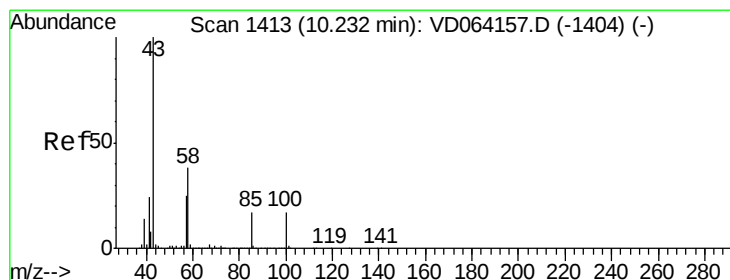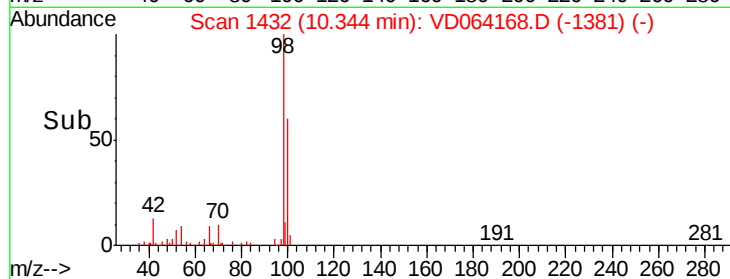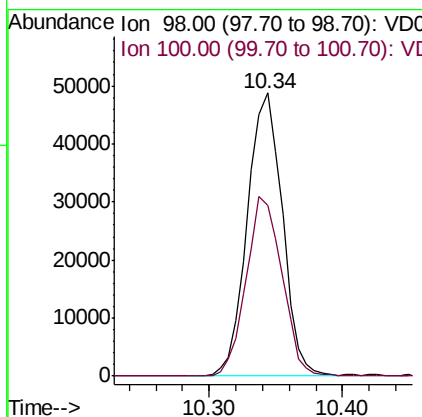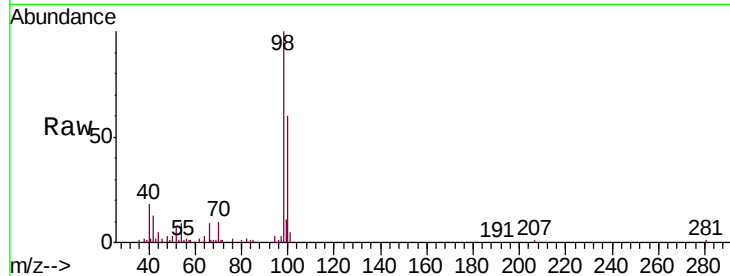

#51
4-Methyl-2-Pentanone
Concen: 8.838 ug/l
RT: 10.23 min Scan# 1412
Delta R.T. -0.01 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 43 Resp: 2497
Ion Ratio Lower Upper
43 100
58 6.6 30.2 45.4#


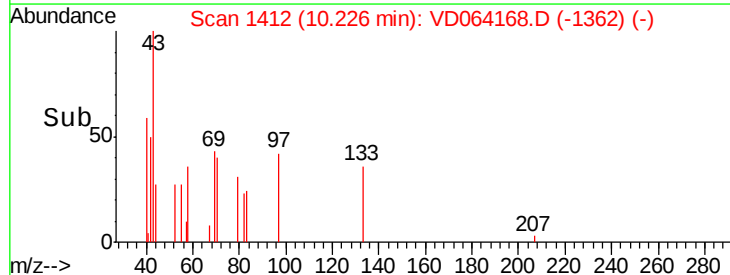
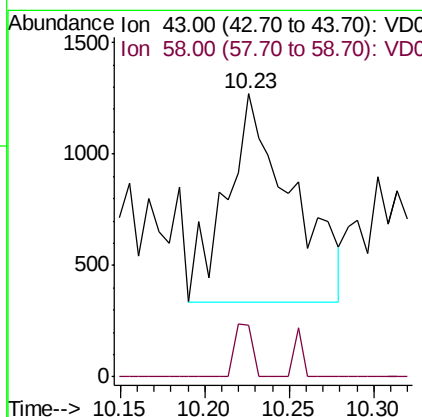



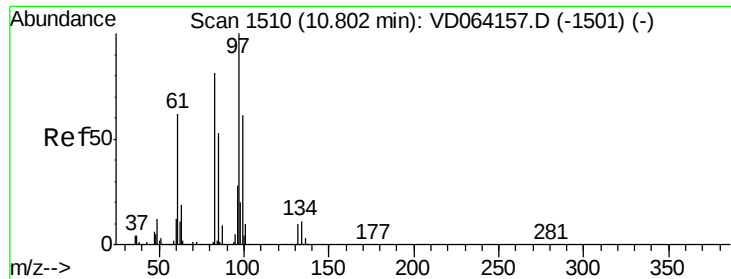

#55
 1,1,2-Trichloroethane
 Concen: 2.921 ug/l
 RT: 10.81 min Scan# 1511
 Delta R.T. 0.01 min
 Lab File: VD064168.D
 Acq: 08 Nov 2019 21:37




Instrument :
 MSVOA_D
 ClientSampleId :
 CO-1008


Tgt Ion: 97 Resp: 957
 Ion Ratio Lower Upper
 97 100
 83 38.3 65.1 97.7#
 85 4.8 42.0 63.0#
 99 0.0 48.9 73.3#

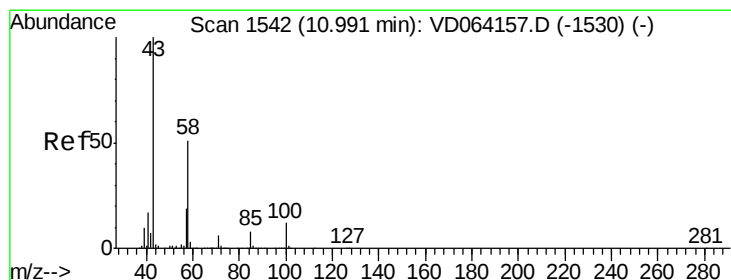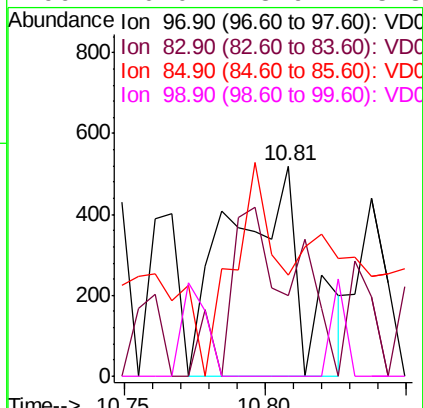

#59
 2-Hexanone
 Concen: 9.423 ug/l
 RT: 10.99 min Scan# 1542
 Delta R.T. -0.00 min
 Lab File: VD064168.D
 Acq: 08 Nov 2019 21:37

Tgt Ion: 43 Resp: 1894
 Ion Ratio Lower Upper
 43 100
 58 59.7 25.9 77.7



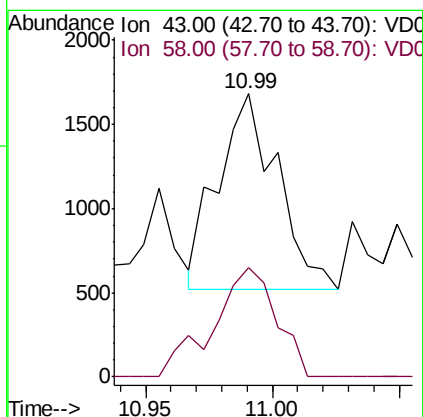



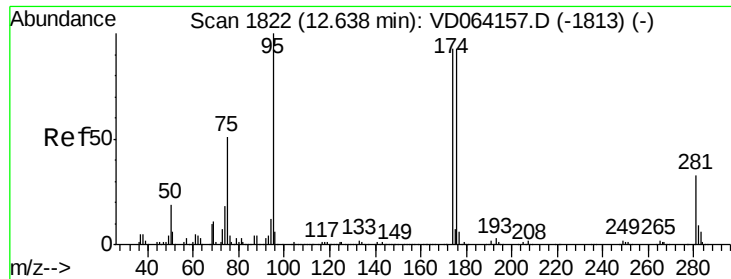

#62
4-Bromofluorobenzene
Concen: 71.537 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. -0.00 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37




Instrument :
MSVOA_D
ClientSampleId :
CO-1008


Tgt Ion: 95 Resp: 39425
Ion Ratio Lower Upper
95 100
174 91.8 0.0 183.6
176 85.0 0.0 180.2

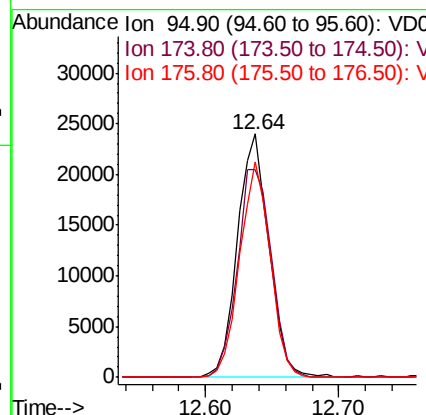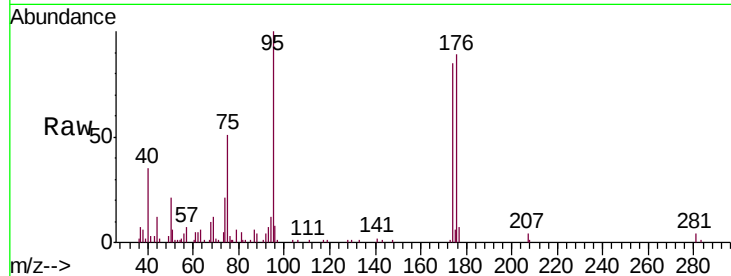

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. -0.00 min
Lab File: VD064168.D
Acq: 08 Nov 2019 21:37

Tgt Ion: 117 Resp: 76347
Ion Ratio Lower Upper
117 100
82 51.4 42.8 64.2
119 32.8 25.6 38.4

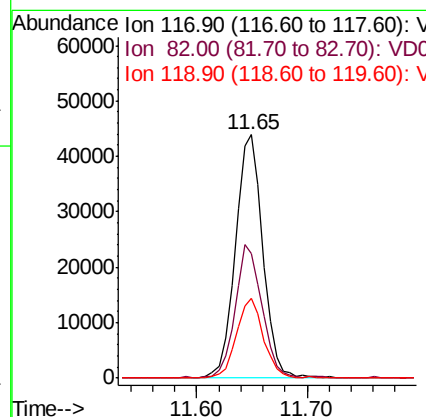



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1982

Delta R.T. -0.00 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampled :

CO-1008


Tgt Ion:152 Resp: 44470

Ion Ratio Lower Upper

152 100

115 56.2 27.4 82.2




150 149.6 0.0 351.6

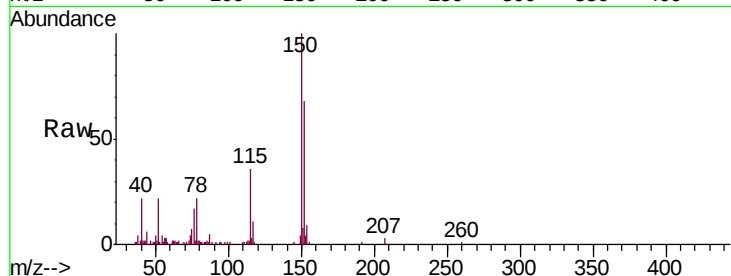

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

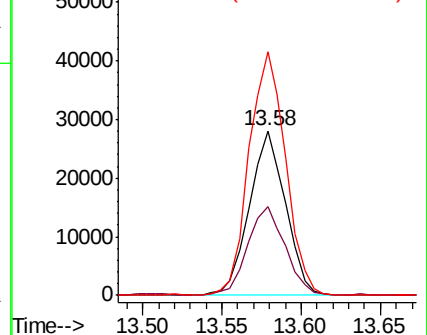

#75

1,1,2,2-Tetrachloroethane

Concen: 1.812 ug/l

RT: 12.74 min Scan# 1840

Delta R.T. 0.01 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37


Tgt Ion: 83 Resp: 891

Ion Ratio Lower Upper

83 100

131 0.0 5.9 17.7#



85 70.5 32.5 97.5




Abundance Ion 82.90 (82.60 to 83.60): VDC

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VDC

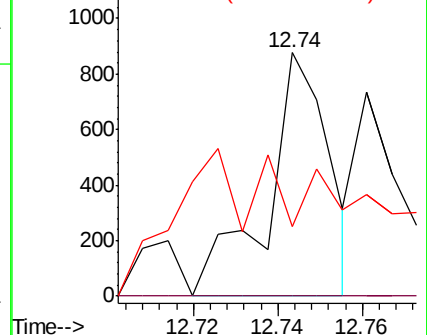

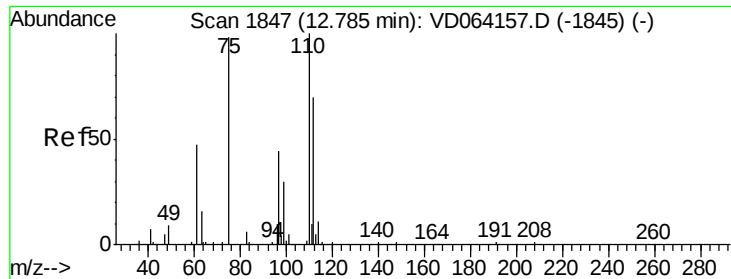

#76

1,2,3-Trichloropropane

Concen: 57.187 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. -0.15 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37

Instrument :

MSVOA_D

ClientSampleId :


CO-1008

Tgt Ion: 75 Resp: 20484

Ion Ratio Lower Upper




75 100

77 4.5 0.0 0.0#

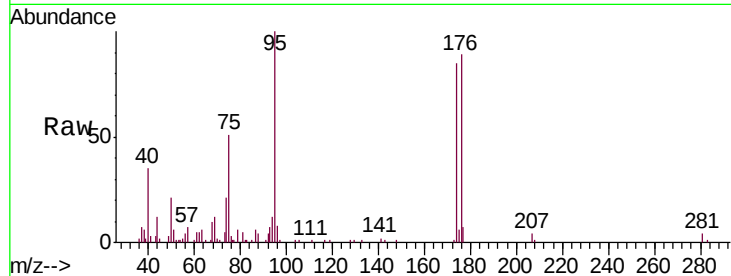

Abundance Ion 74.90 (74.60 to 75.60): VDC

Ion 77.00 (76.70 to 77.70): VDC

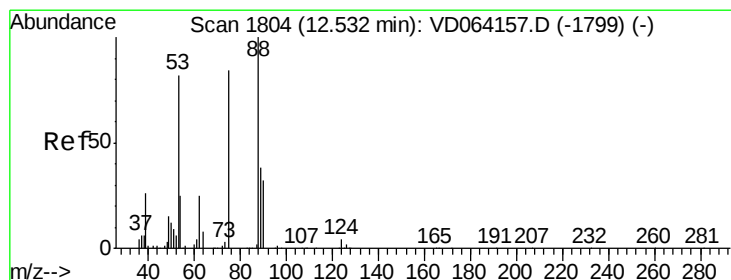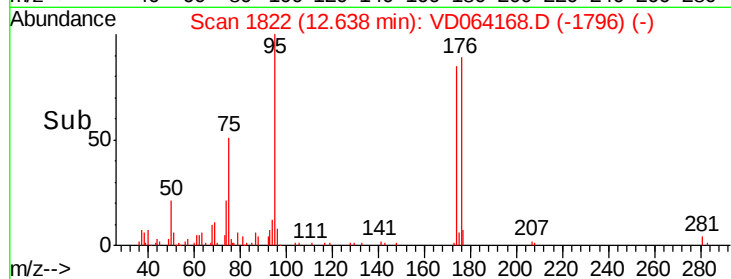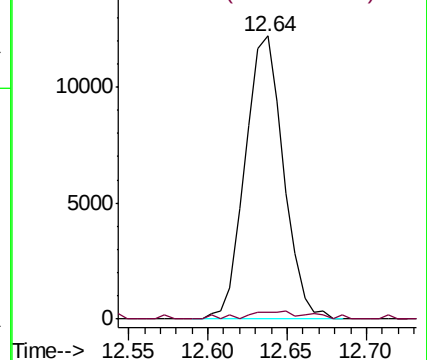

#81

trans-1,4-Dichloro-2-butene

Concen: 113.596 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.11 min

Lab File: VD064168.D

Acq: 08 Nov 2019 21:37


Tgt Ion: 75 Resp: 20484

Ion Ratio Lower Upper

75 100

53 1.2 79.4 119.0#



89 0.0 36.6 55.0#




Abundance Ion 74.90 (74.60 to 75.60): VDC

Ion 53.00 (52.70 to 53.70): VDC

Ion 88.90 (88.60 to 89.60): VDC




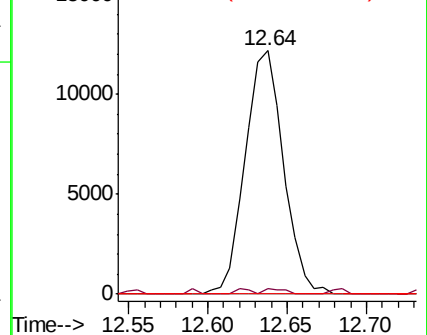


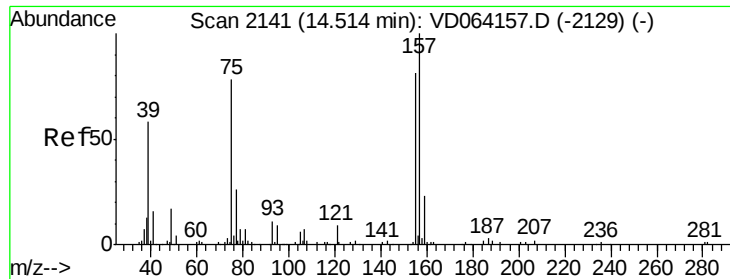

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.365 ug/l
 RT: 14.52 min Scan# 2142
 Delta R.T. 0.01 min
 Lab File: VD064168.D
 Acq: 08 Nov 2019 21:37

Instrument :
 MSVOA_D
 ClientSampleId :
 CO-1008

Tgt Ion: 75 Resp: 120
 Ion Ratio Lower Upper
 75 100
 155 0.0 48.0 144.0#
 157 0.0 61.5 184.4#

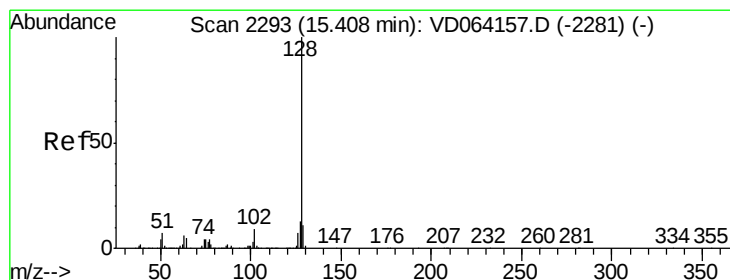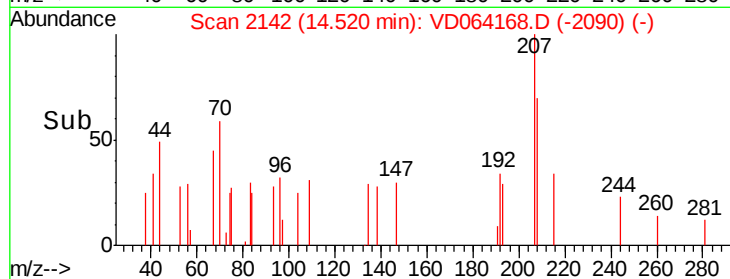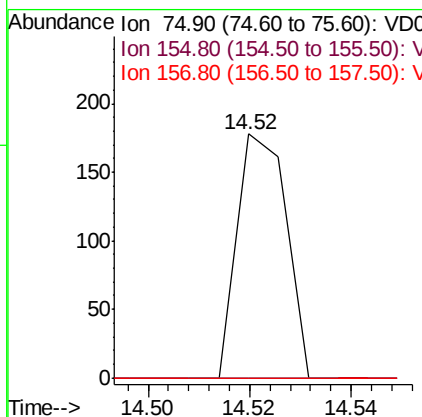

#95
 Naphthalene
 Concen: 1.280 ug/l
 RT: 15.41 min Scan# 2293
 Delta R.T. -0.00 min
 Lab File: VD064168.D
 Acq: 08 Nov 2019 21:37

Tgt Ion: 128 Resp: 2016
 Ion Ratio Lower Upper
 128 100
 127 7.4 10.5 15.7#
 129 14.7 8.6 13.0#

