


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD110819\
Data File : VD064153.D
Acq On : 08 Nov 2019 12:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Title : SW846 8260
Last Update : Tue Nov 12 02:43:24 2019

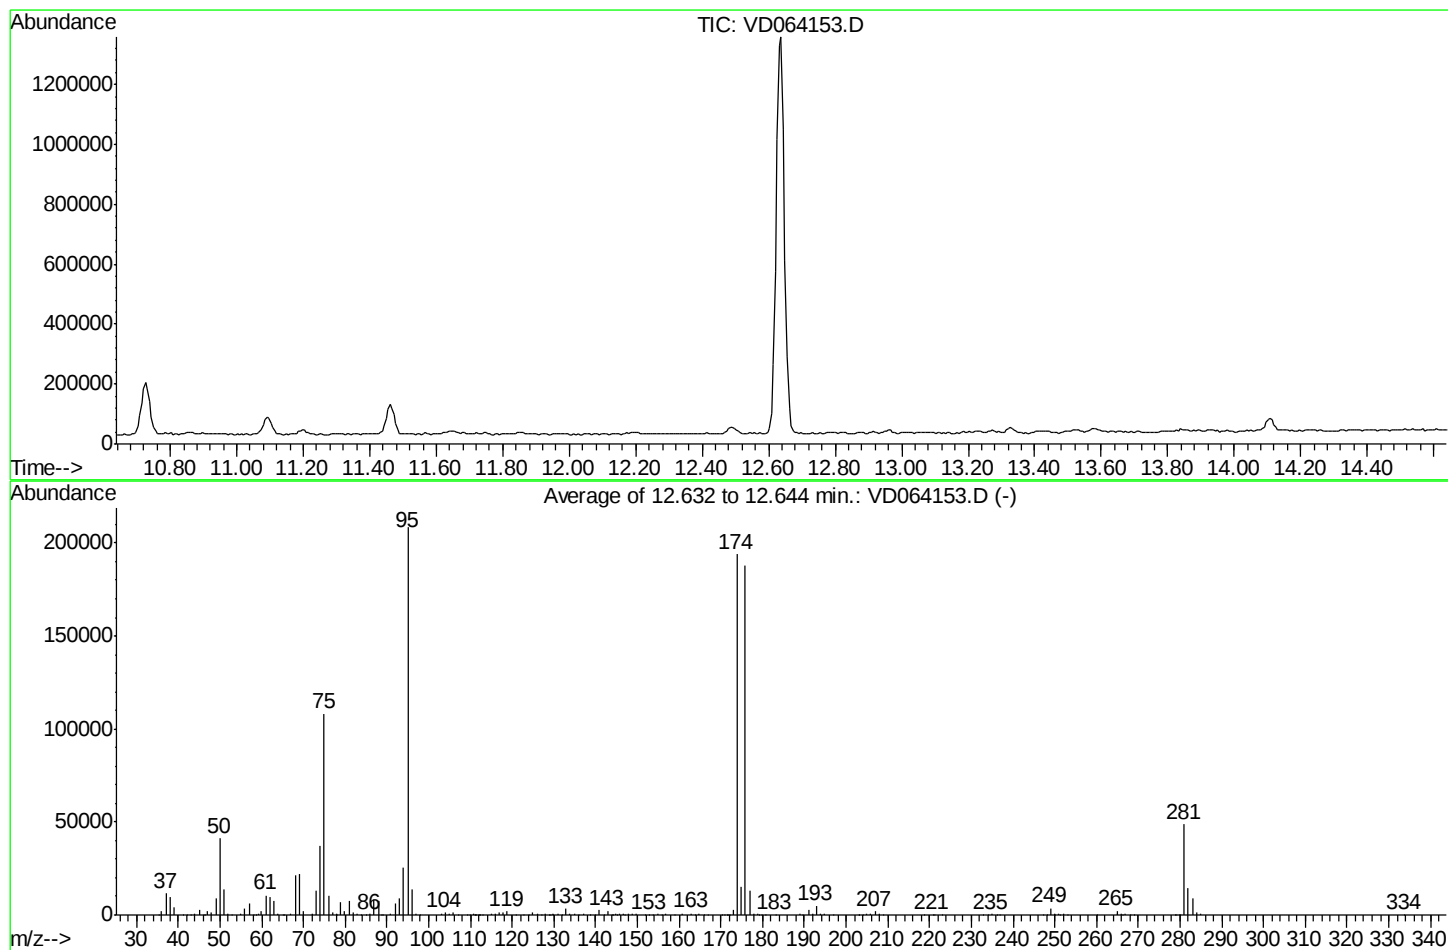

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	41154	PASS
75	95	30	60	51.8	108047	PASS
95	95	100	100	100.0	208400	PASS
96	95	5	9	6.7	13976	PASS
173	174	0.00	2	1.3	2454	PASS
174	95	50	100	93.1	193941	PASS
175	174	5	9	7.7	14994	PASS
176	174	95	101	96.8	187797	PASS
177	176	5	9	7.0	13197	PASS