
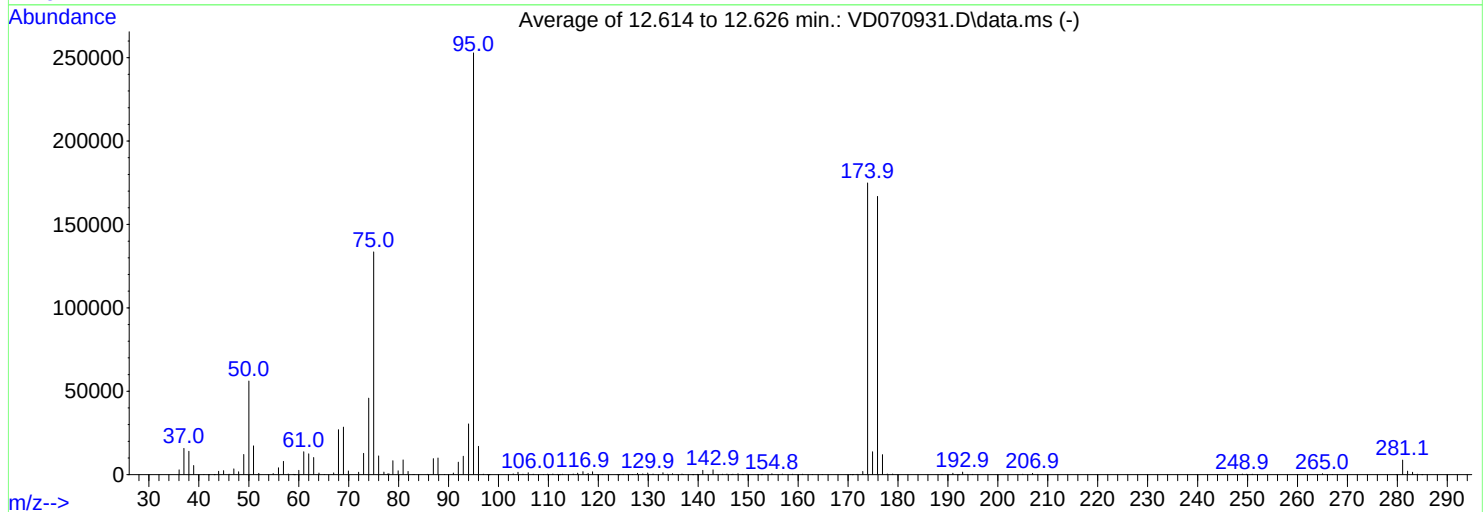


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110821\
 Data File : VD070931.D
 Acq On : 08 Nov 2021 09:58
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110521S.M
 Title : SW846 8260
 Last Update : Mon Nov 08 13:56:36 2021

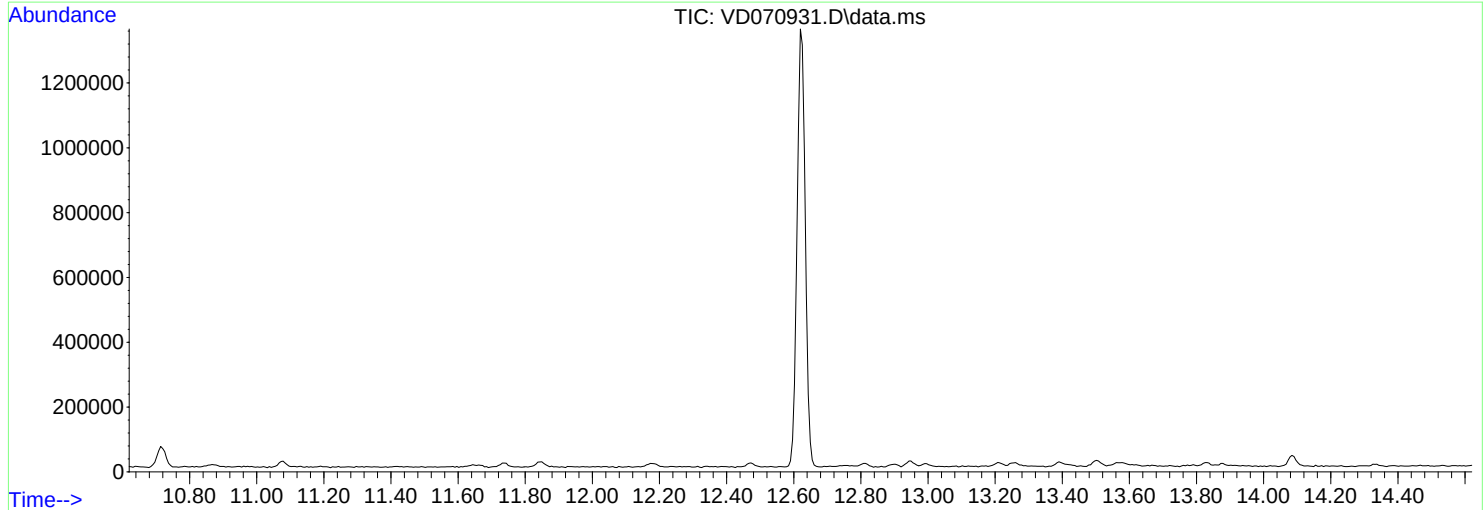

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	56117	PASS
75	95	30	60	52.8	133555	PASS
95	95	100	100	100.0	252885	PASS
96	95	5	9	6.7	16974	PASS
173	174	0.00	2	1.1	1978	PASS
174	95	50	100	69.2	174891	PASS
175	174	5	9	7.9	13745	PASS
176	174	95	101	95.4	166784	PASS
177	176	5	9	7.2	12047	PASS