



Acrolein

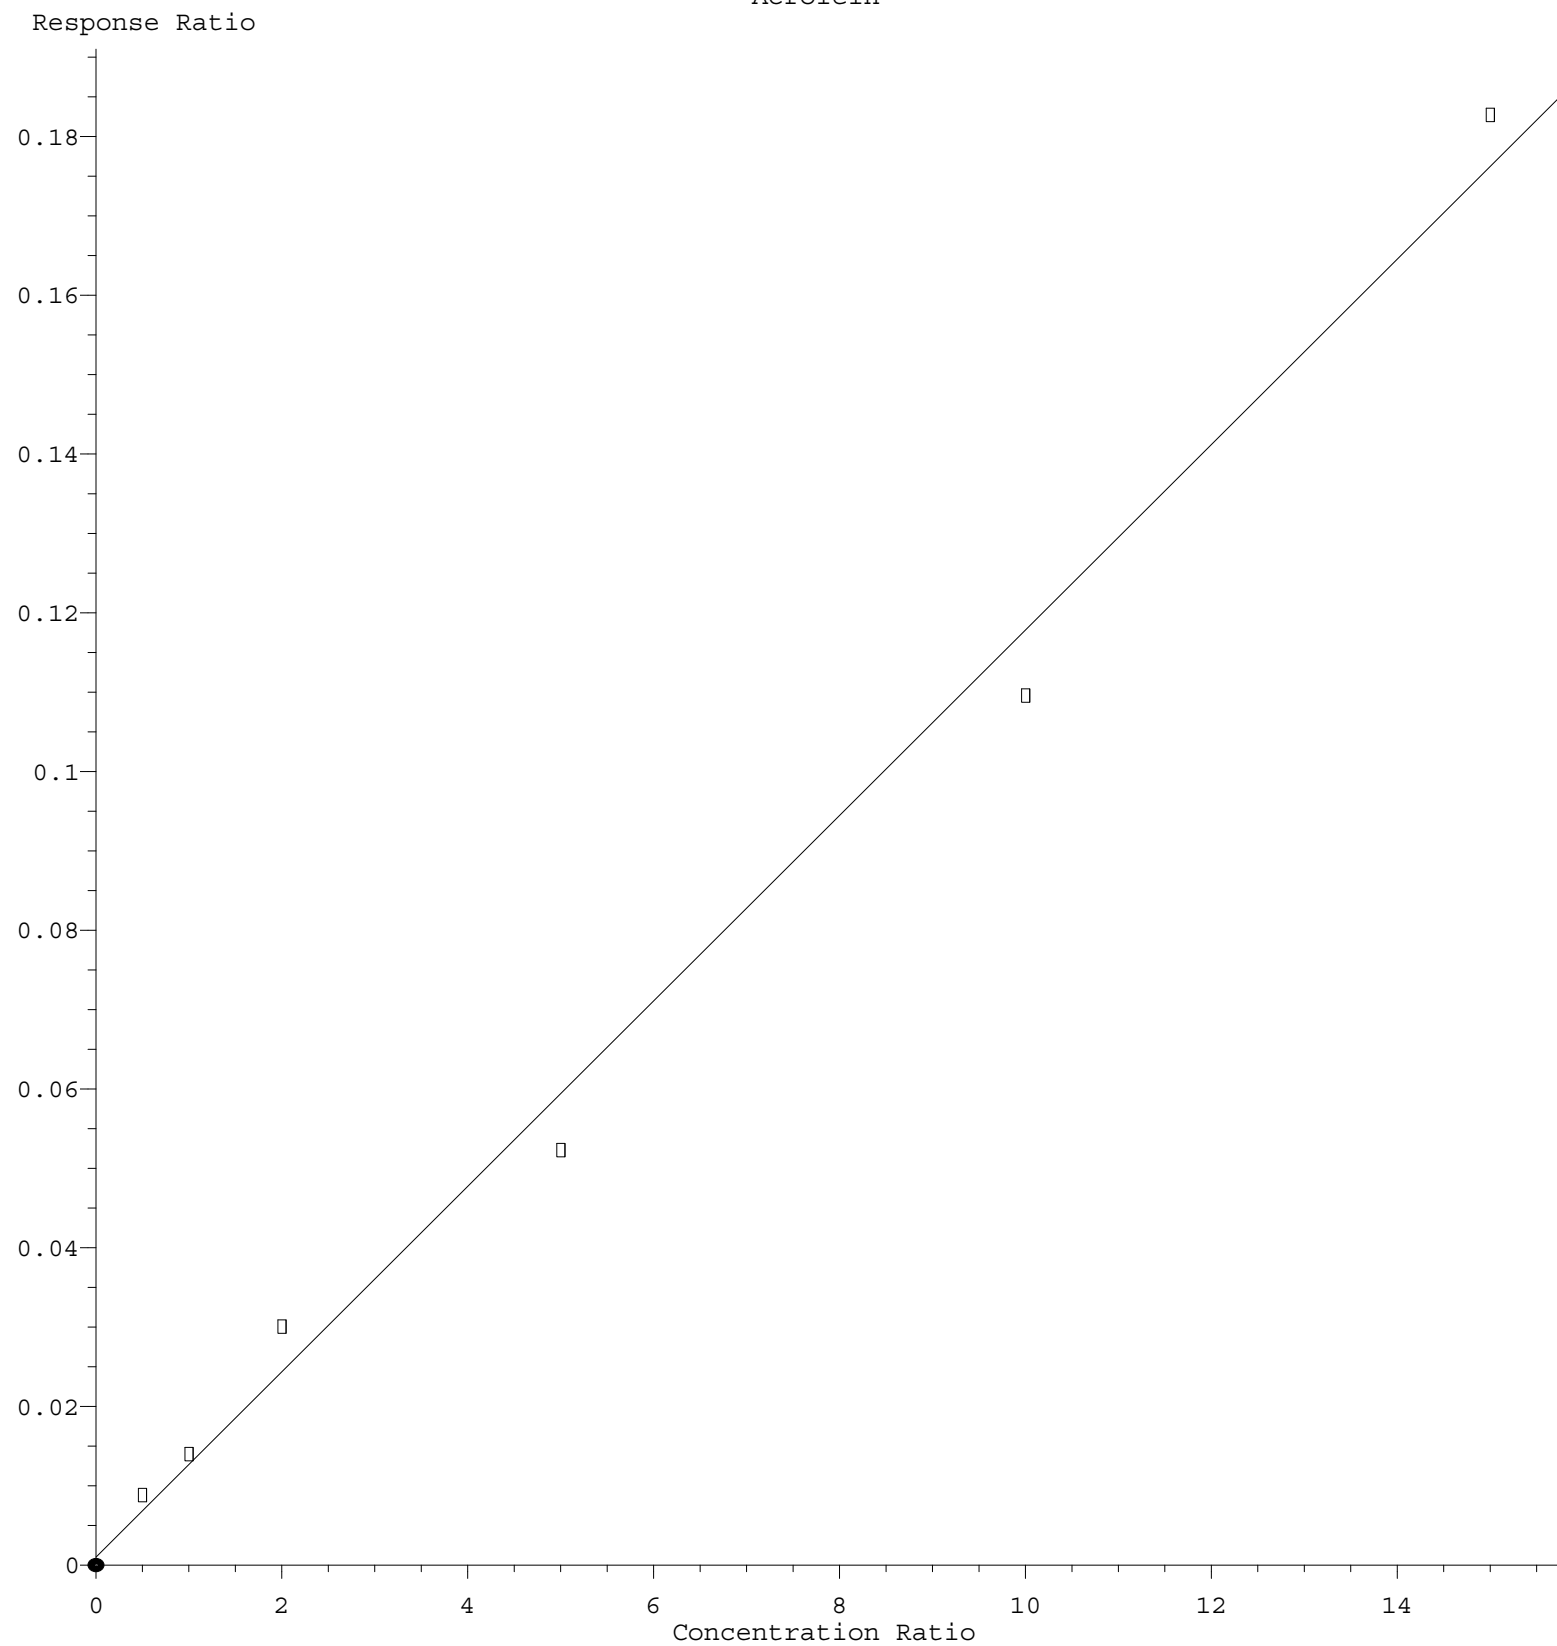

$\text{Response} = 1.164\text{e-}002 * \text{Amt} + 1.275\text{e-}003$
 Coef of Det (r^2) = 0.991353 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M
 Calibration Table Last Updated: Wed Nov 10 03:55:51 2021

Acetone

Response Ratio

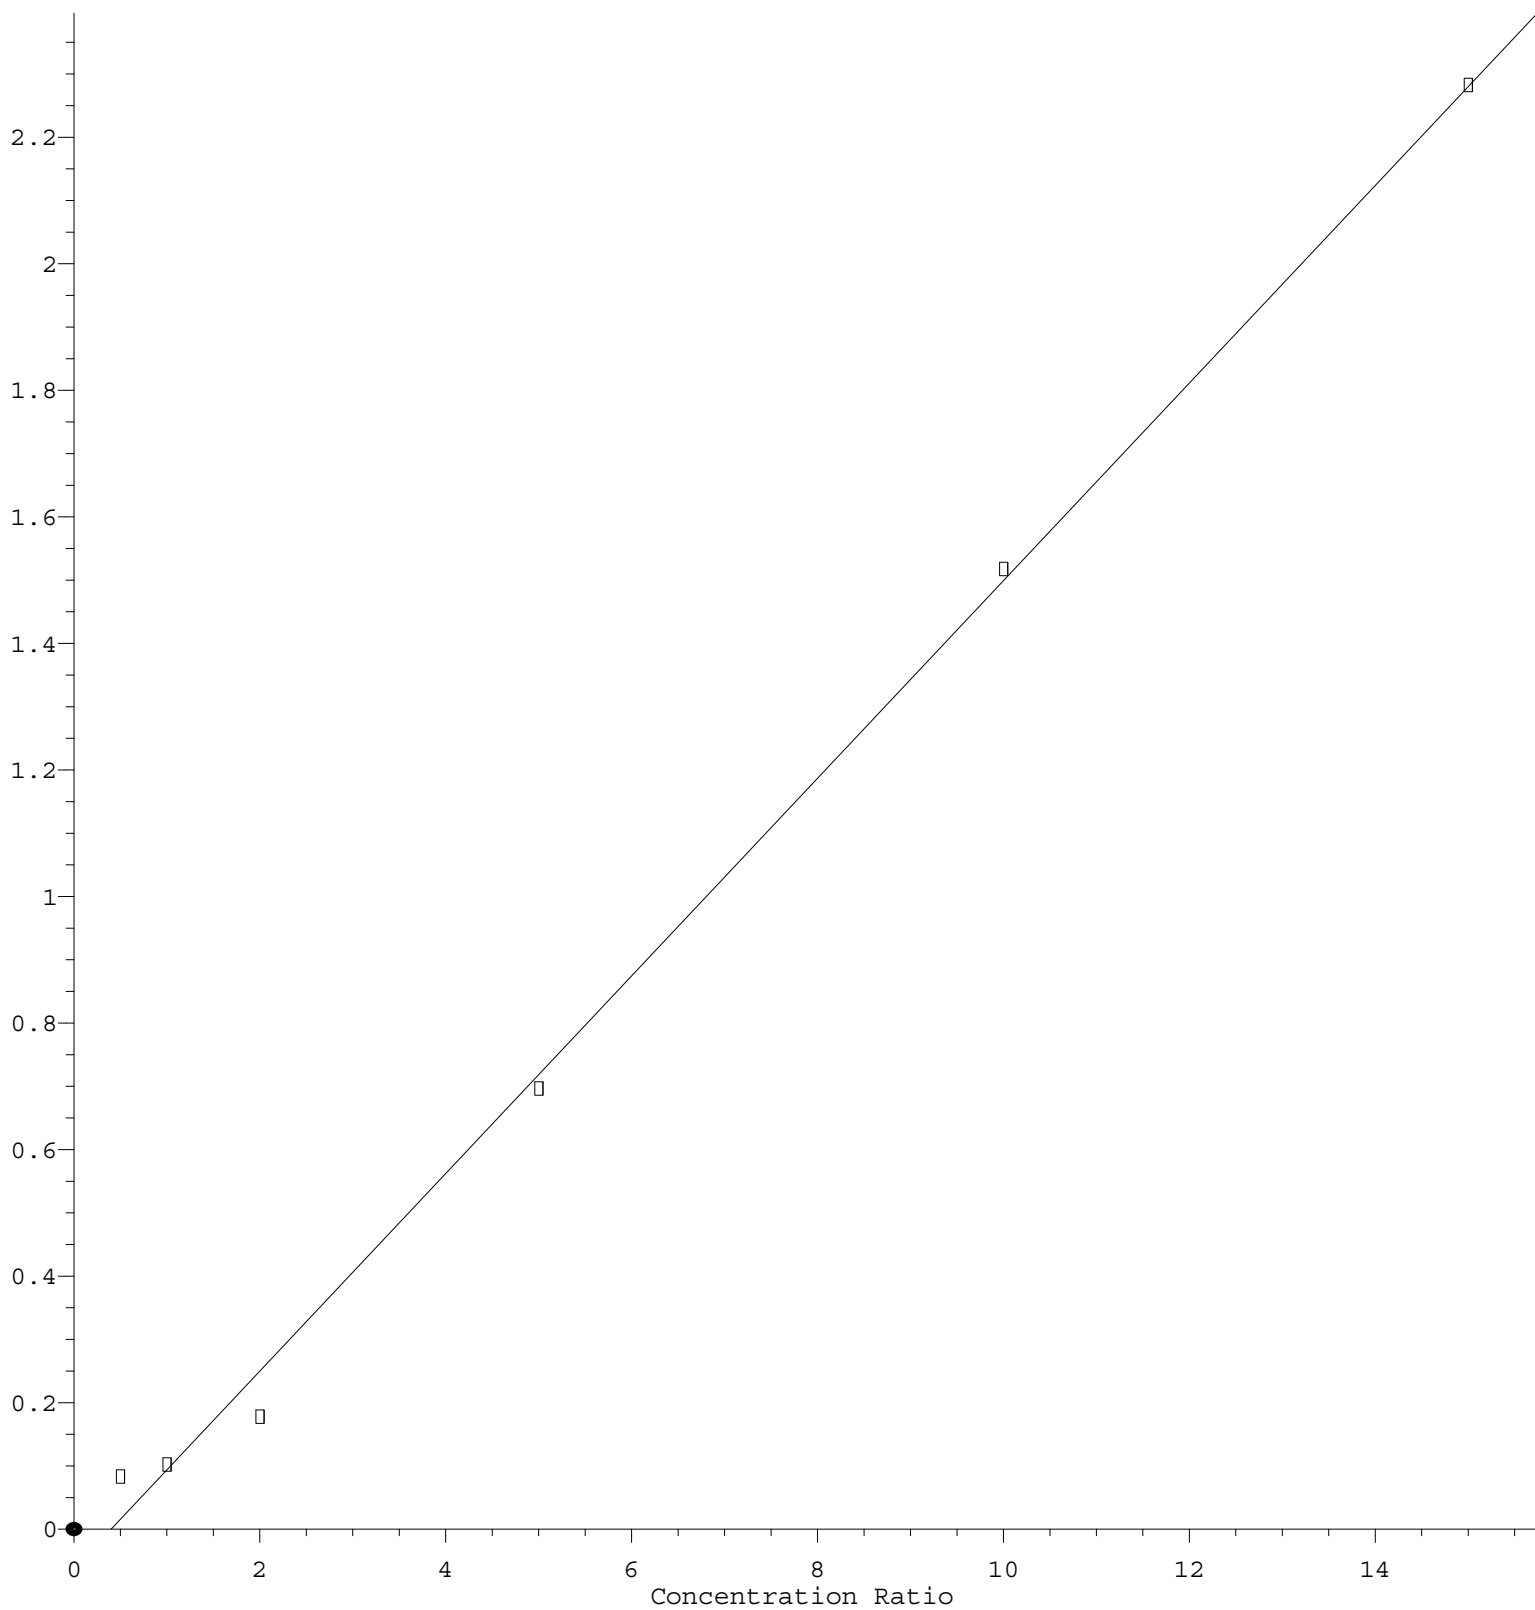

$$\text{Response} = 1.561\text{e-}001 * \text{Amt} - 6.181\text{e-}002$$


Coef of Det (r^2) = 0.997402 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M

Calibration Table Last Updated: Wed Nov 10 03:55:51 2021

Methylene Chloride

Response Ratio

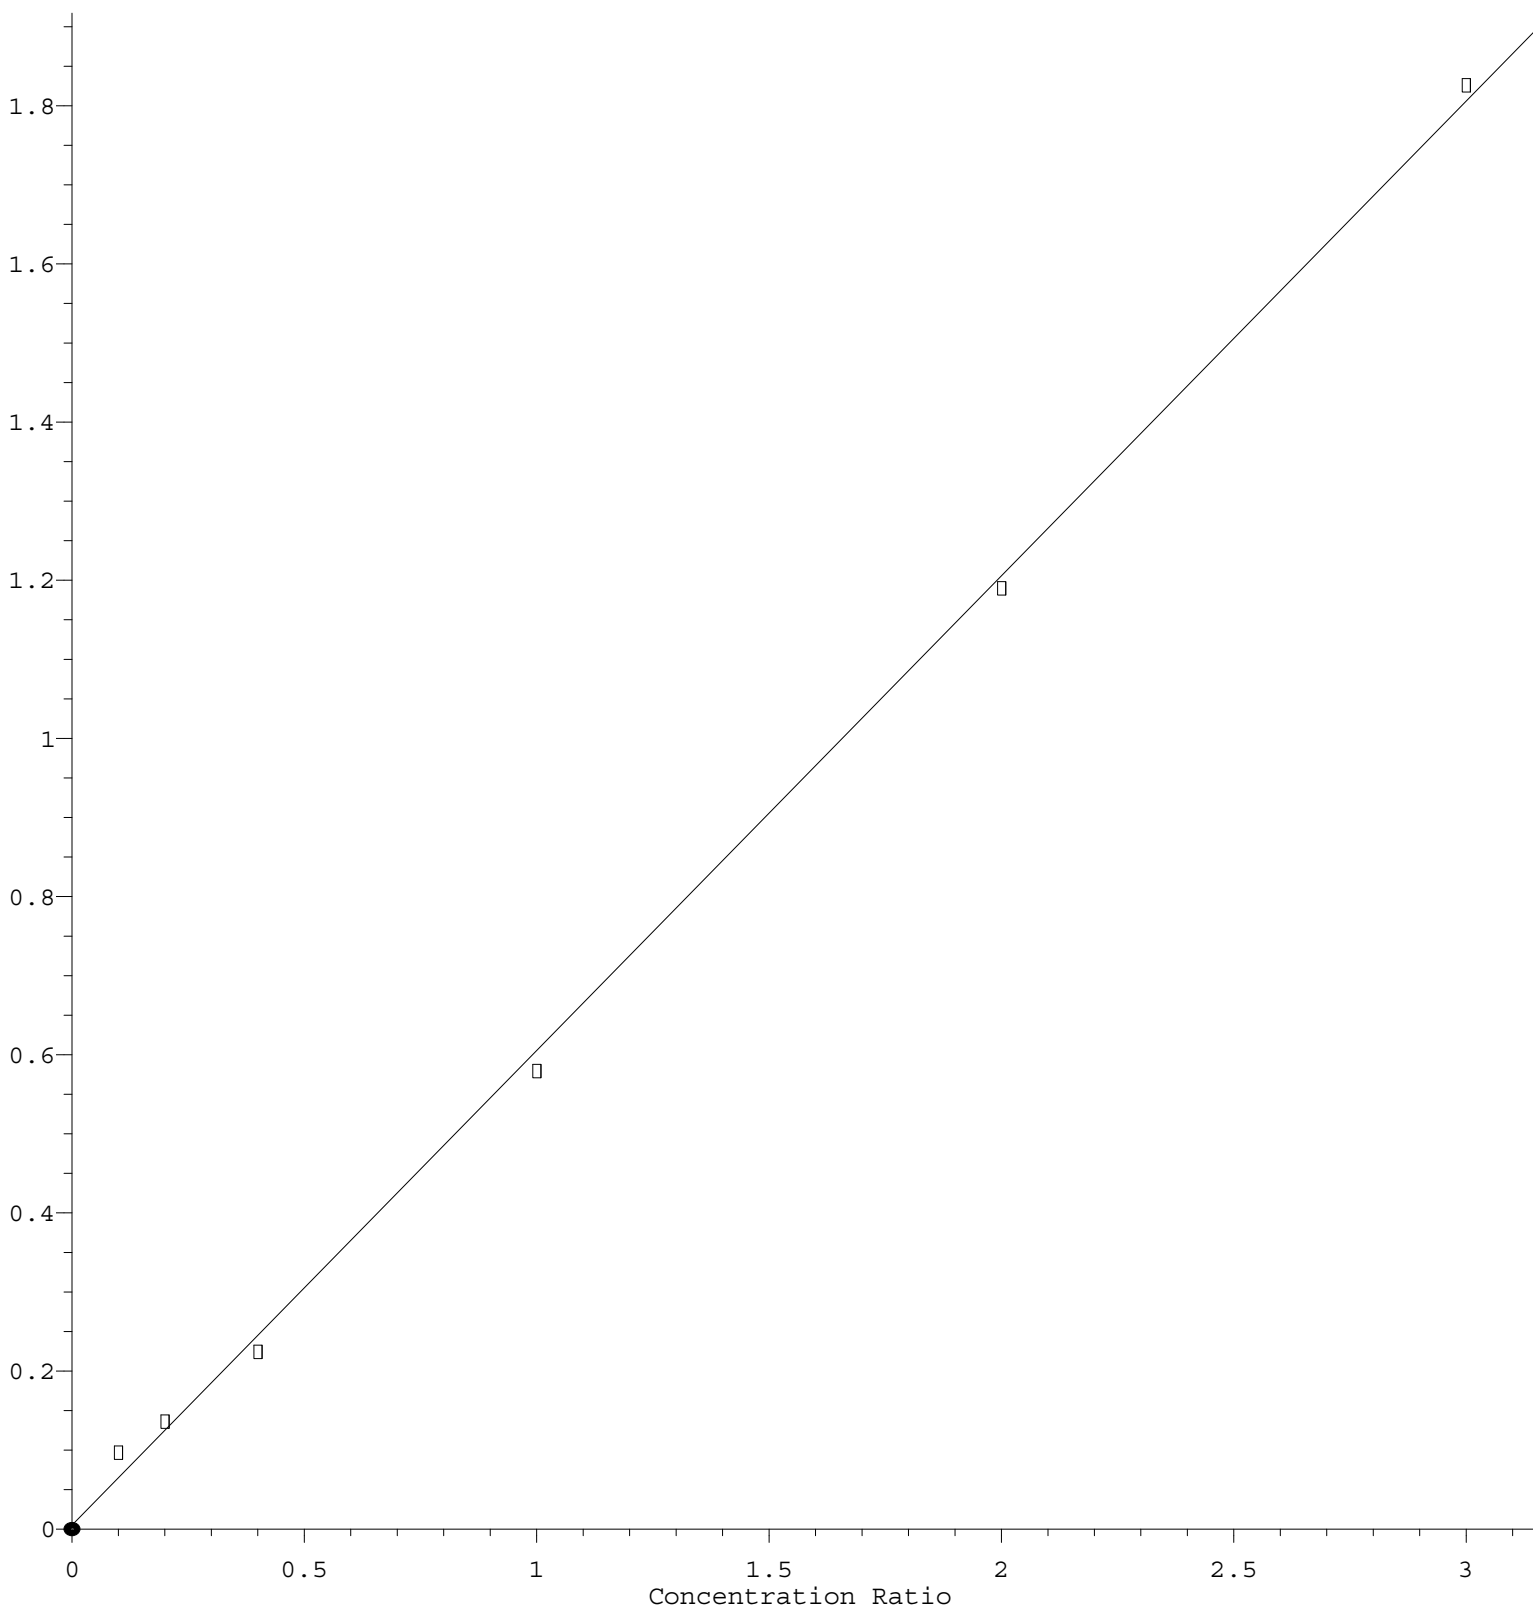

$$\text{Response} = 6.001\text{e-}001 * \text{Amt} + 5.136\text{e-}003$$


Coef of Det (r^2) = 0.998811 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M

Calibration Table Last Updated: Wed Nov 10 03:55:51 2021

Vinyl Acetate

Response Ratio

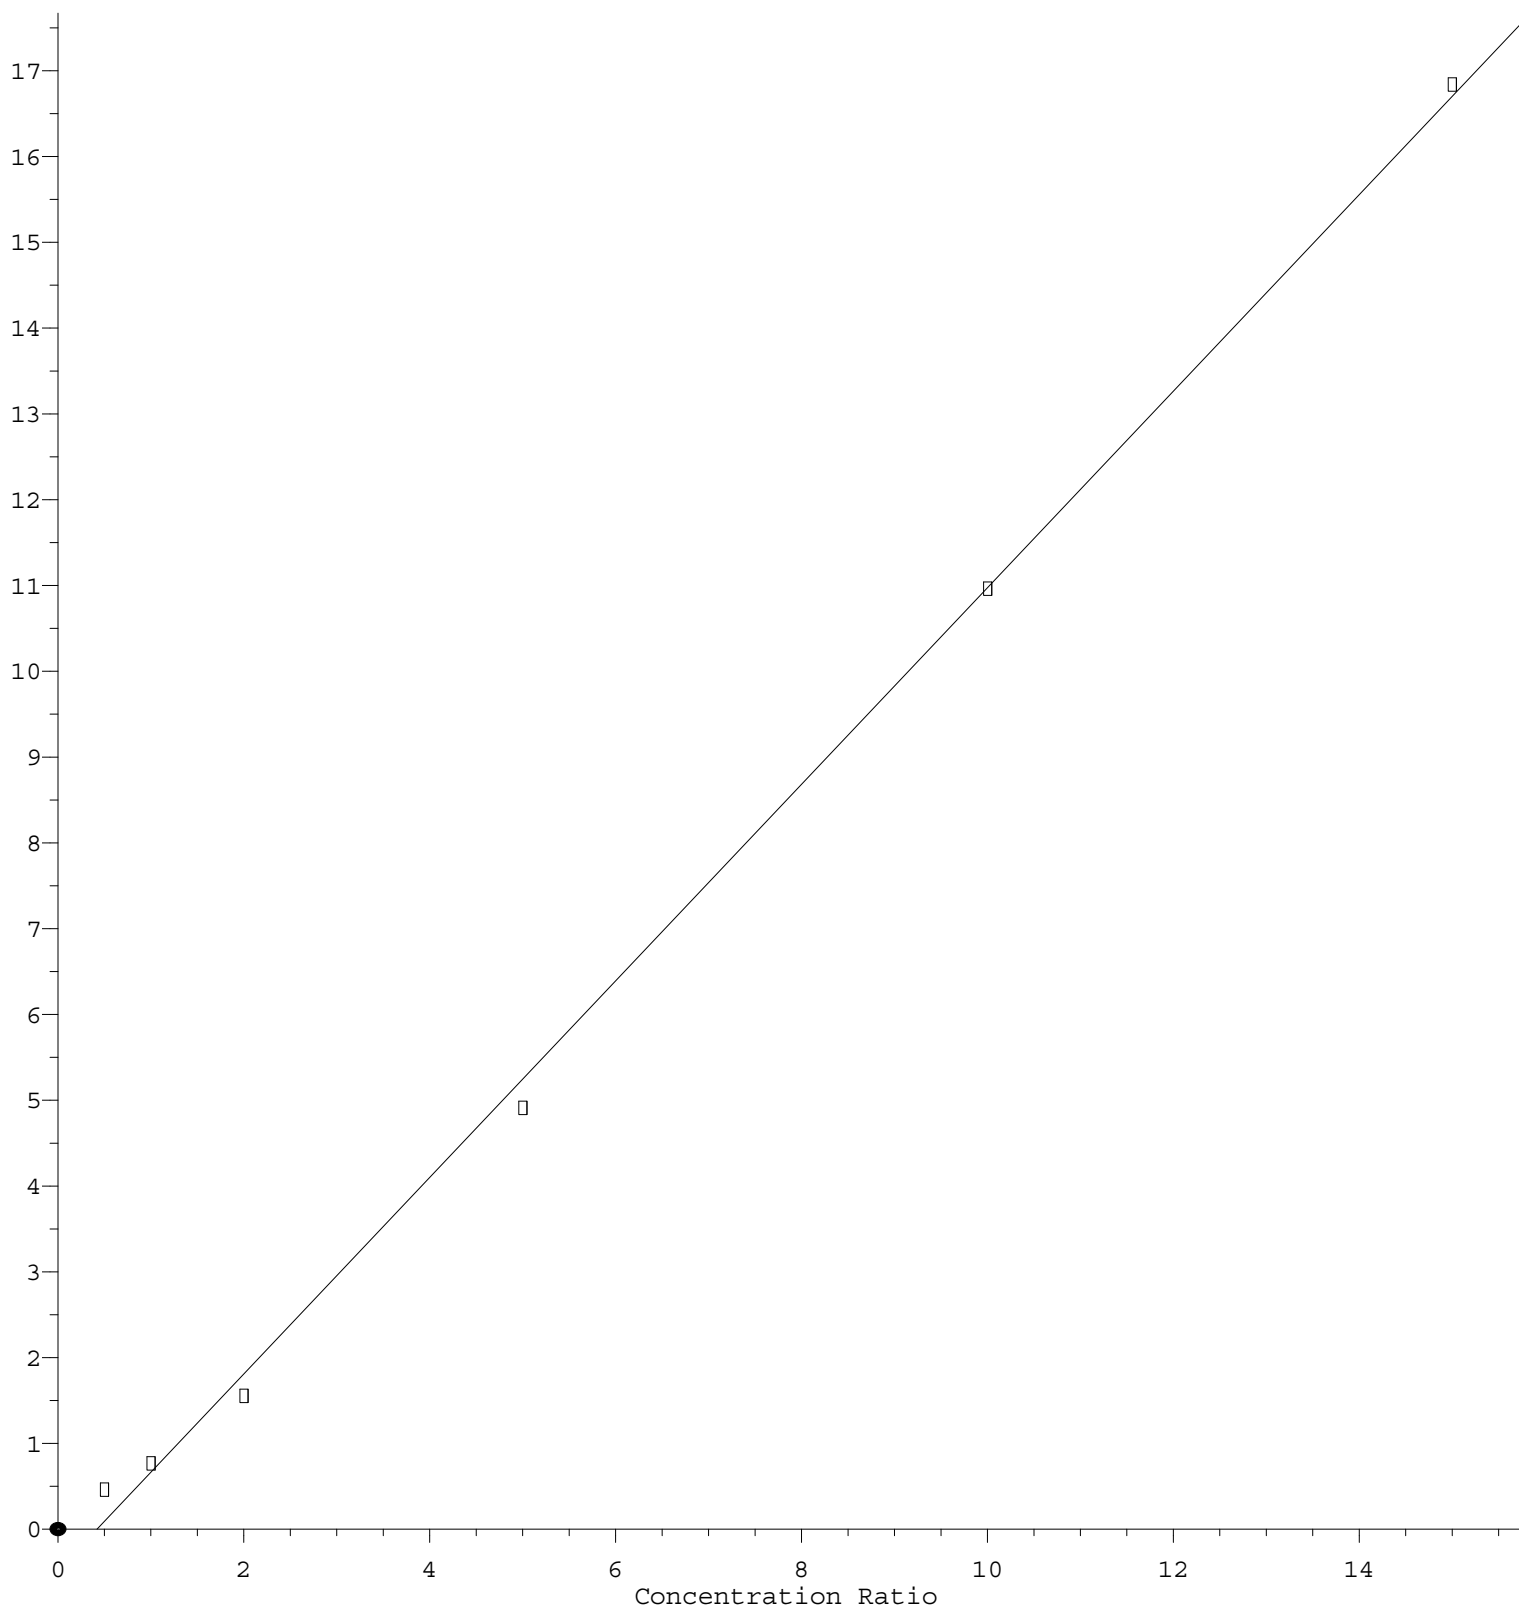

$$\text{Response} = 1.146e+000 * \text{Amt} - 4.807e-001$$


Coef of Det (r^2) = 0.998447 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M

Calibration Table Last Updated: Wed Nov 10 03:55:51 2021

2-Butanone

Response Ratio

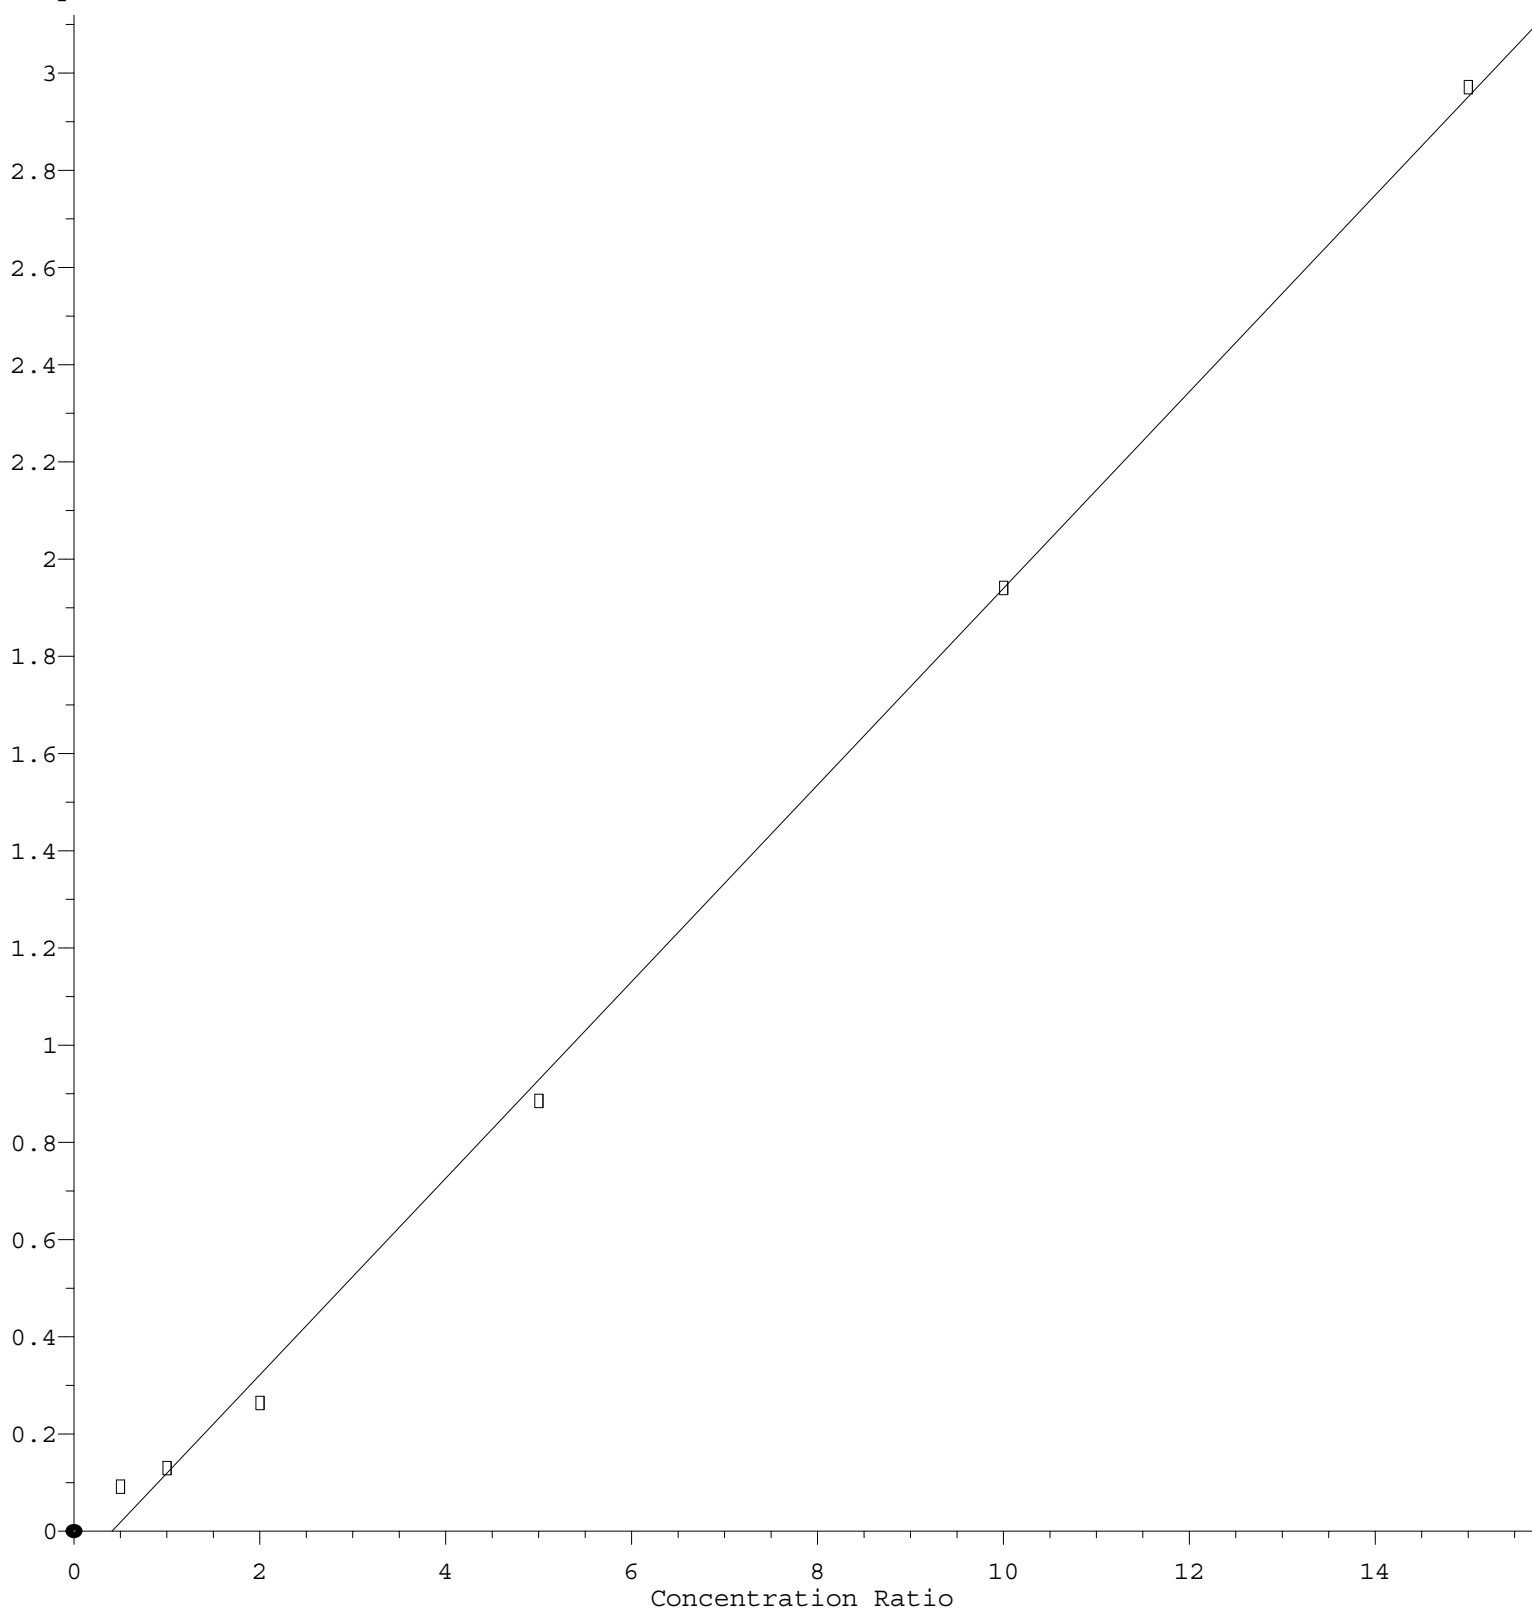


$$\text{Response} = 2.023\text{e-}001 * \text{Amt} - 8.239\text{e-}002$$

Coef of Det (r^2) = 0.998391 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M

Calibration Table Last Updated: Wed Nov 10 03:55:51 2021


Methacrylonitrile

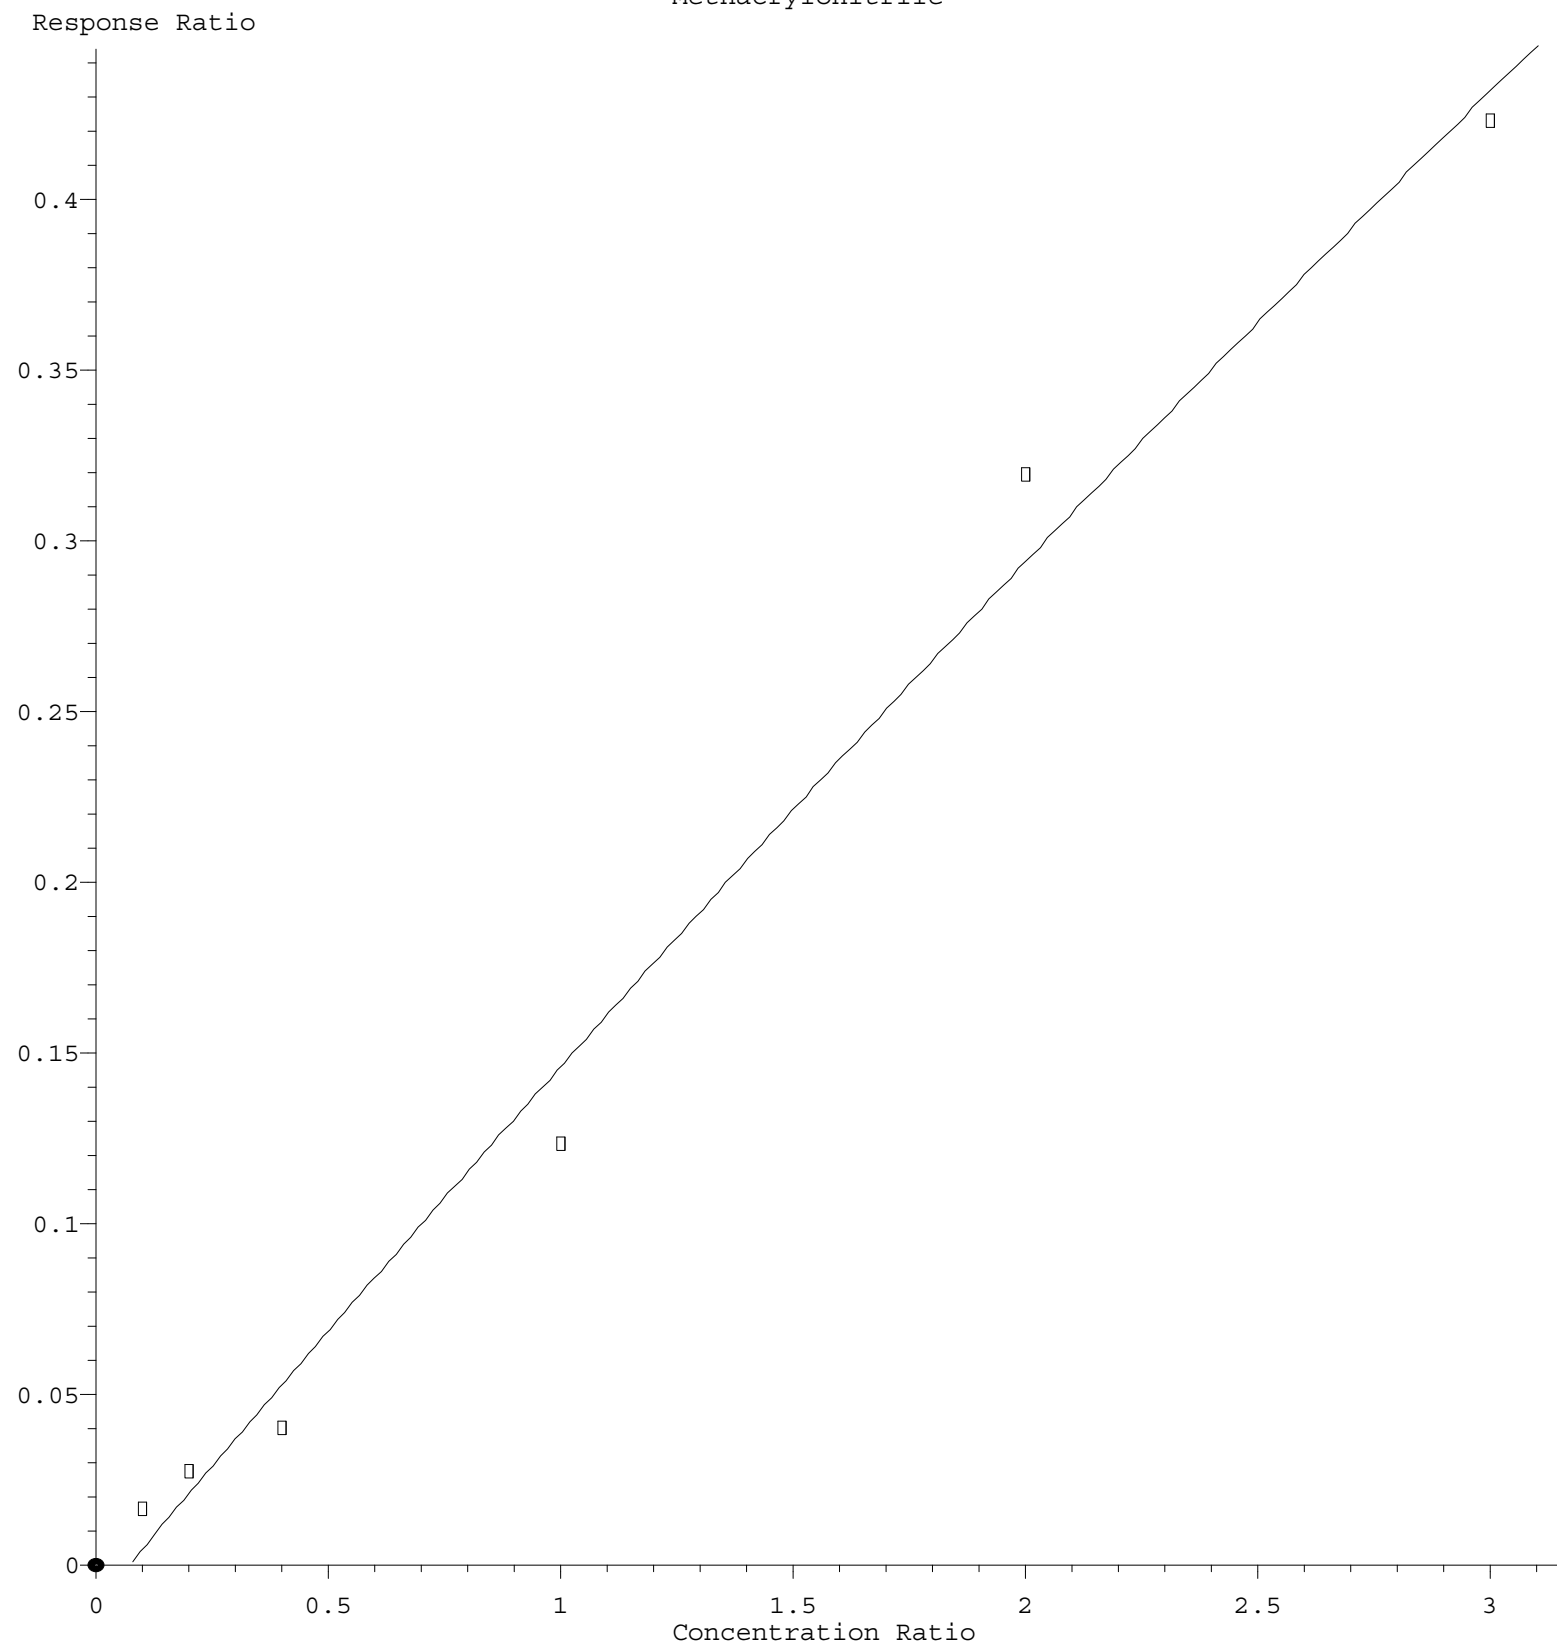

$R = -4.857e-003 A^2 + 1.623e-001 A - 1.136e-002$
Coef of Det (r^2) = 0.989322 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M
Calibration Table Last Updated: Wed Nov 10 03:55:51 2021

2-Hexanone

Response Ratio

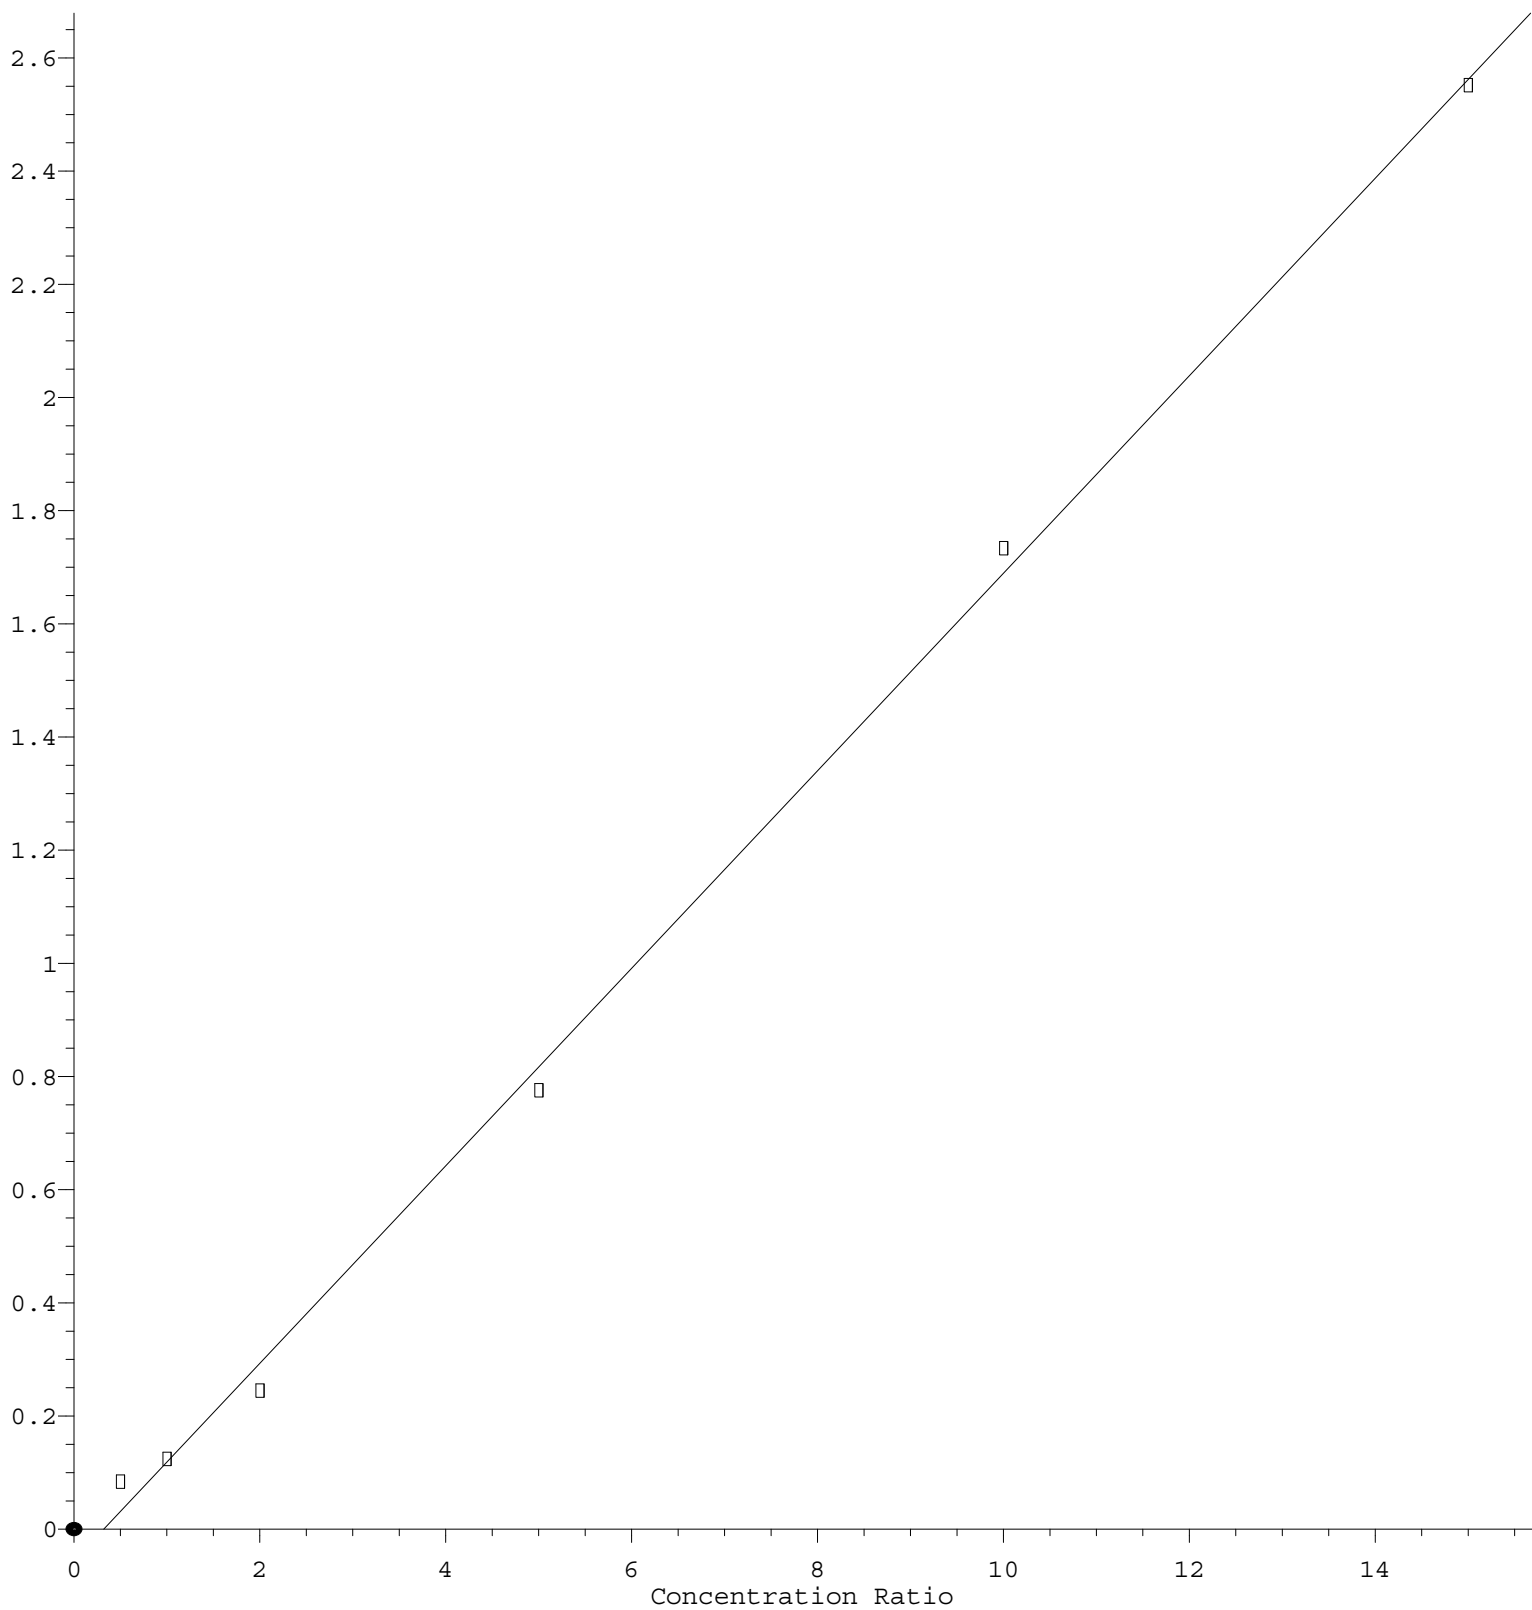


$$\text{Response} = 1.745\text{e-}001 * \text{Amt} - 5.563\text{e-}002$$

Coef of Det (r^2) = 0.998265 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M

Calibration Table Last Updated: Wed Nov 10 03:55:51 2021


trans-1,4-Dichloro-2-butene

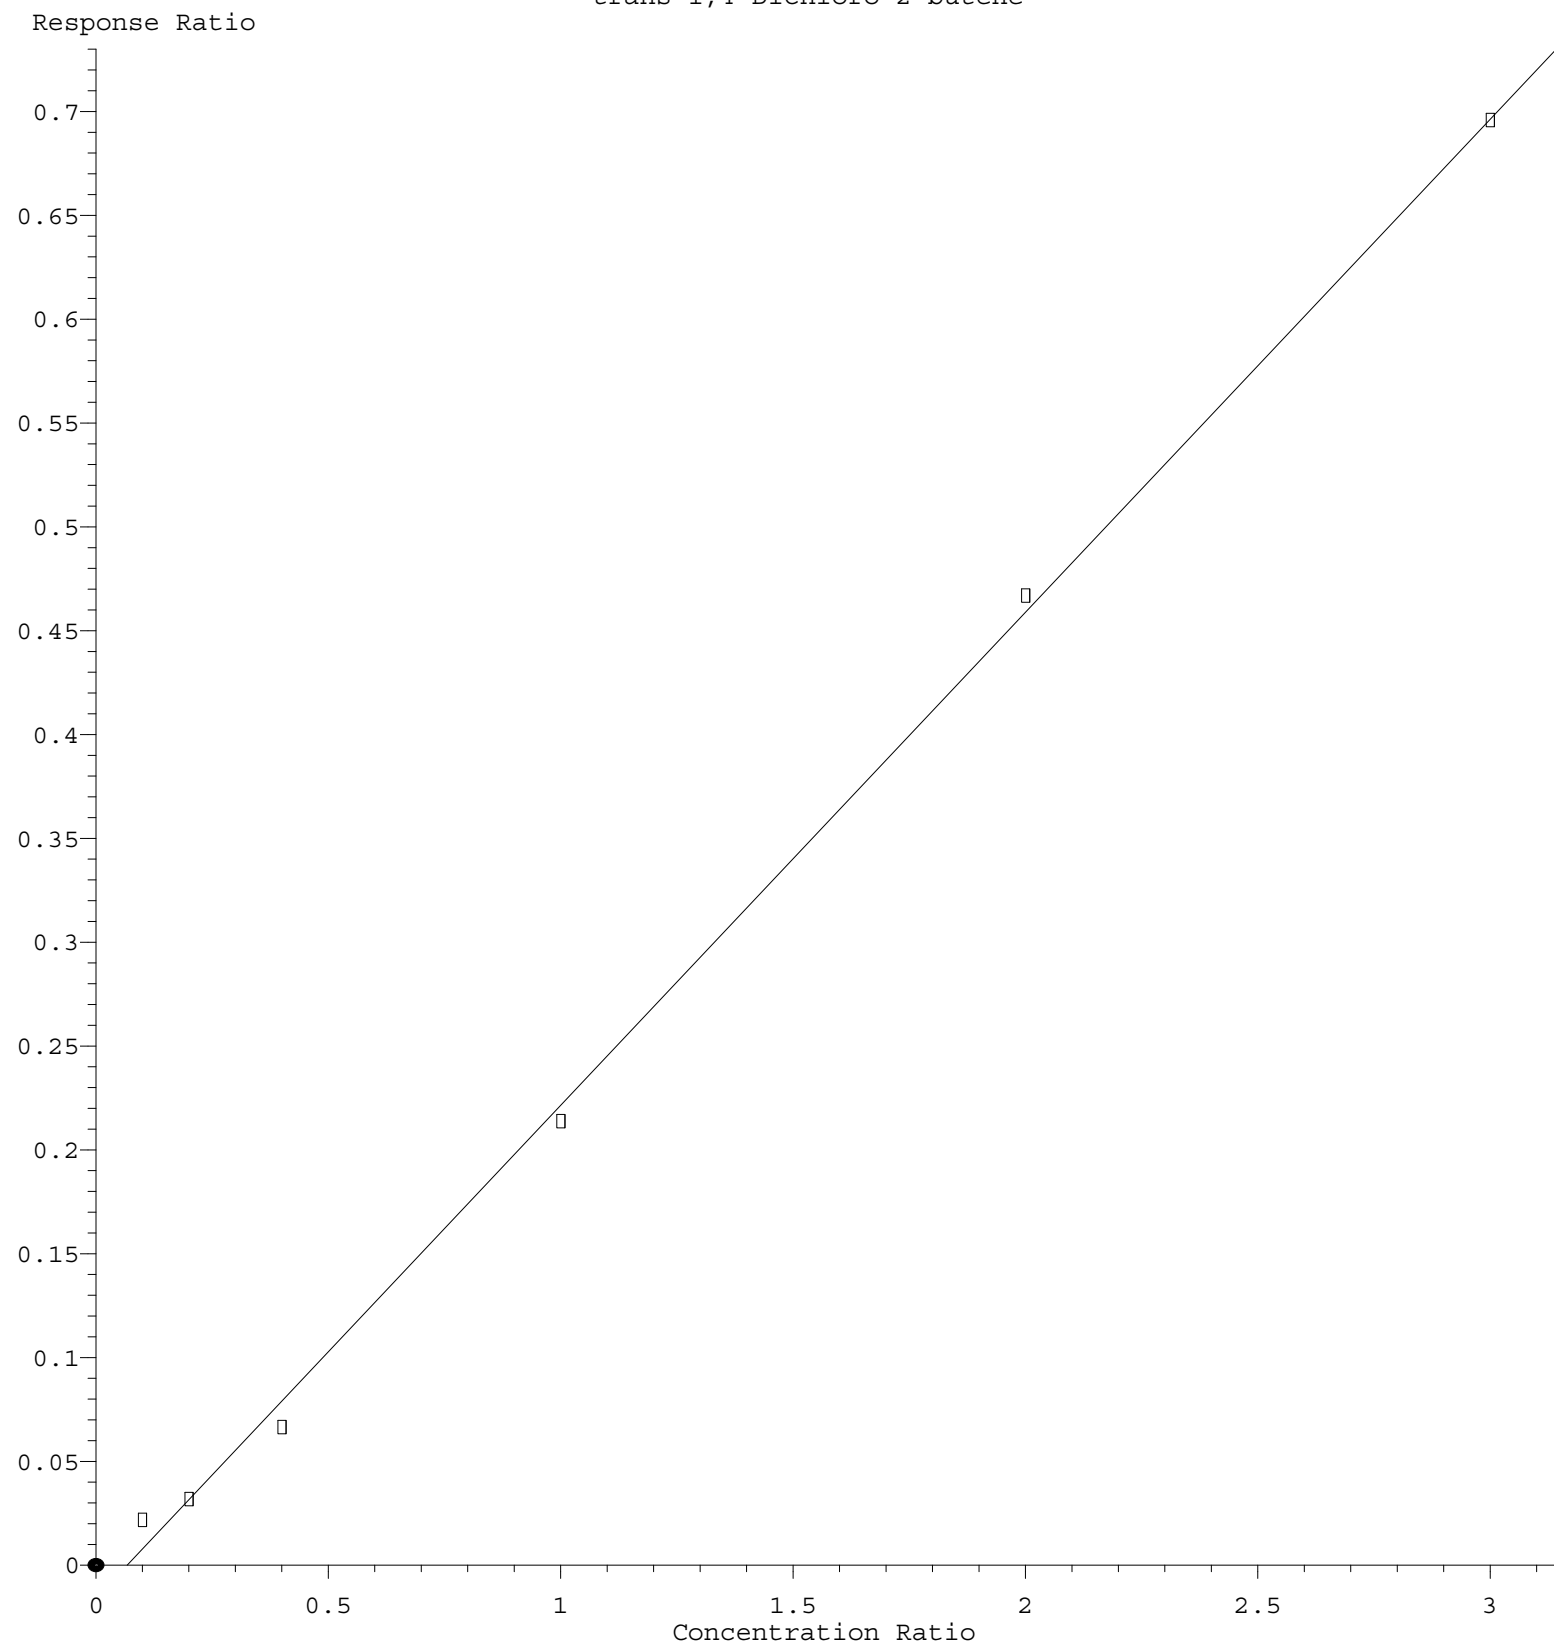

Response = $2.377\text{e-}001 * \text{Amt} - 1.595\text{e-}002$
Coef of Det (r^2) = 0.998750 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M
Calibration Table Last Updated: Wed Nov 10 03:55:51 2021

Methyl Iodide

Response Ratio

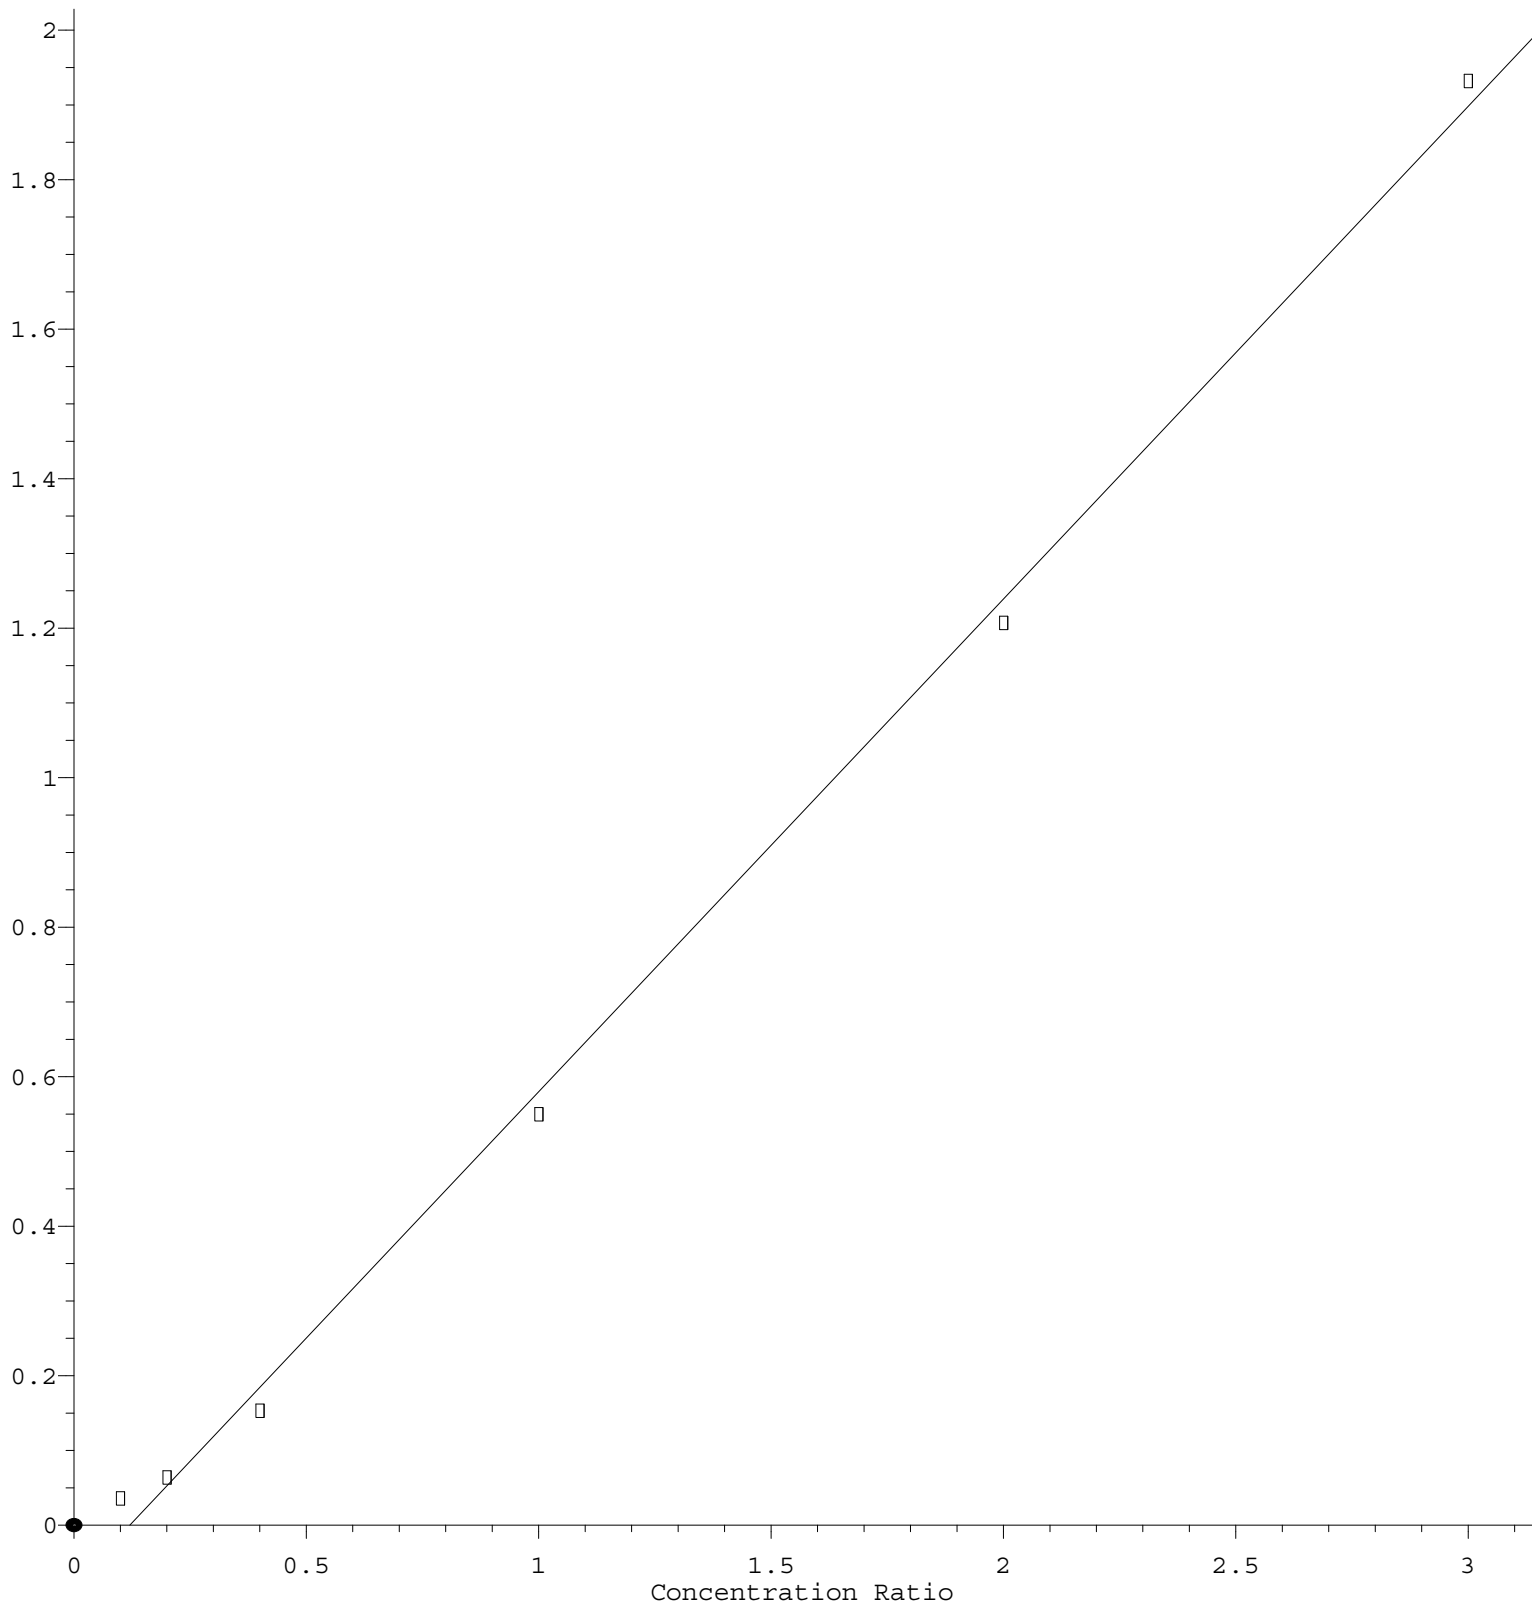

$$\text{Response} = 6.593\text{e-}001 * \text{Amt} - 7.941\text{e-}002$$

Coef of Det (r^2) = 0.997753 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D110921S.M

Calibration Table Last Updated: Wed Nov 10 03:55:51 2021