


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110921\
Data File : VD070943.D
Acq On : 09 Nov 2021 09:01
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
Title : SW846 8260
Last Update : Wed Nov 10 03:55:51 2021

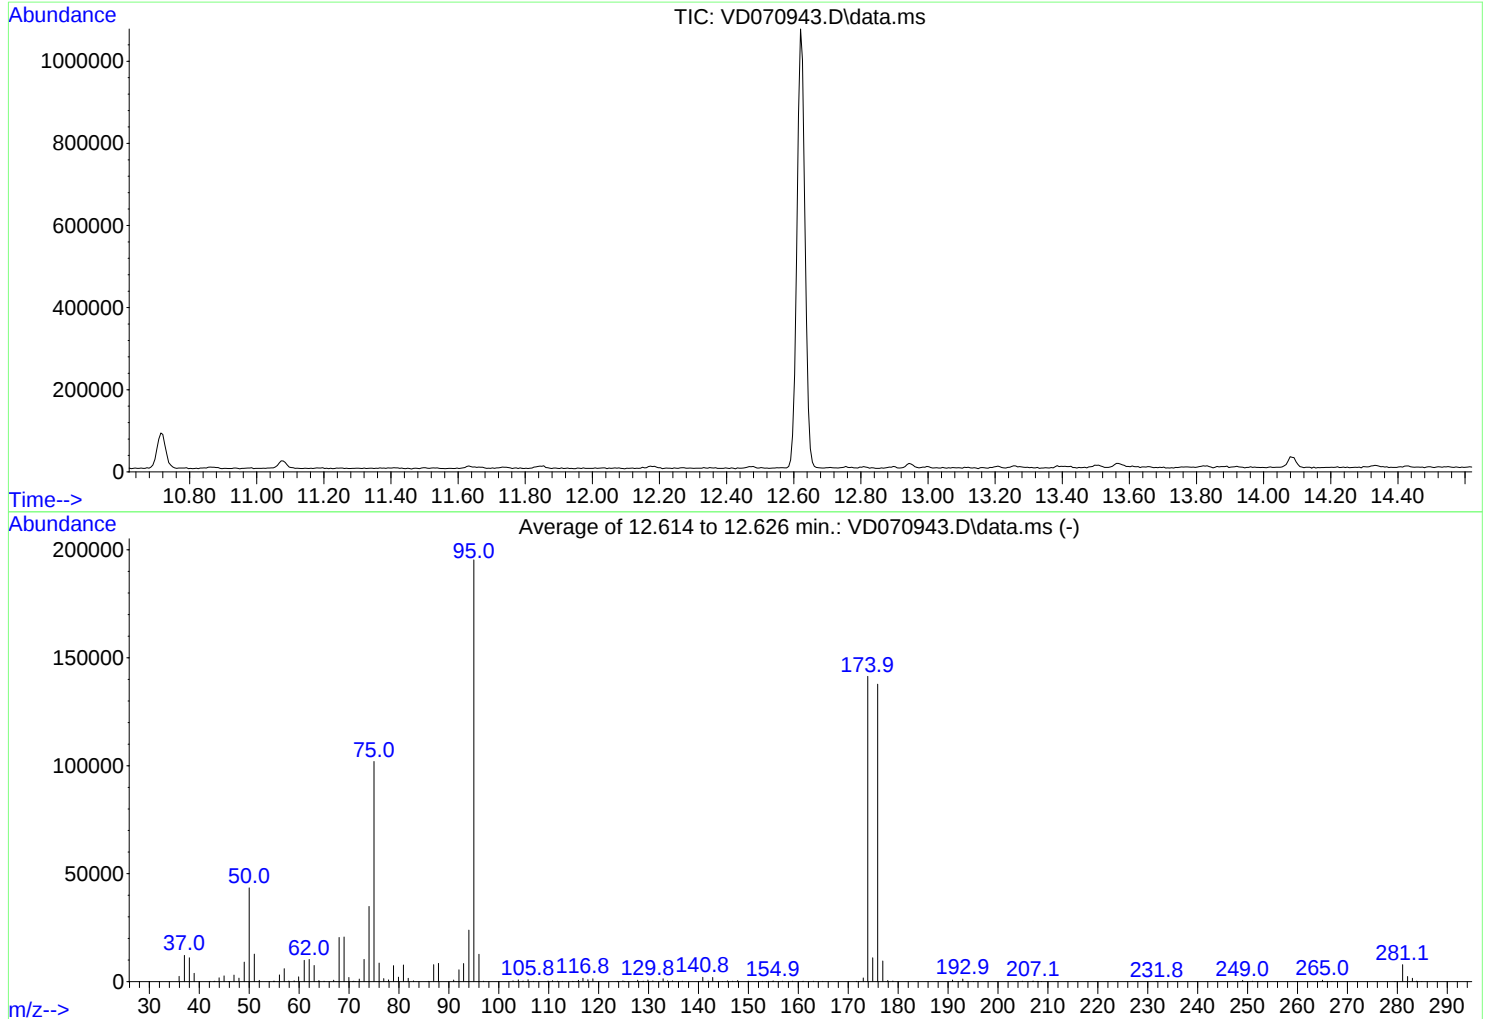

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1808

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	43456	PASS
75	95	30	60	52.2	101965	PASS
95	95	100	100	100.0	195371	PASS
96	95	5	9	6.5	12706	PASS
173	174	0.00	2	1.2	1731	PASS
174	95	50	100	72.4	141395	PASS
175	174	5	9	7.8	11040	PASS
176	174	95	101	97.5	137808	PASS
177	176	5	9	6.9	9532	PASS