
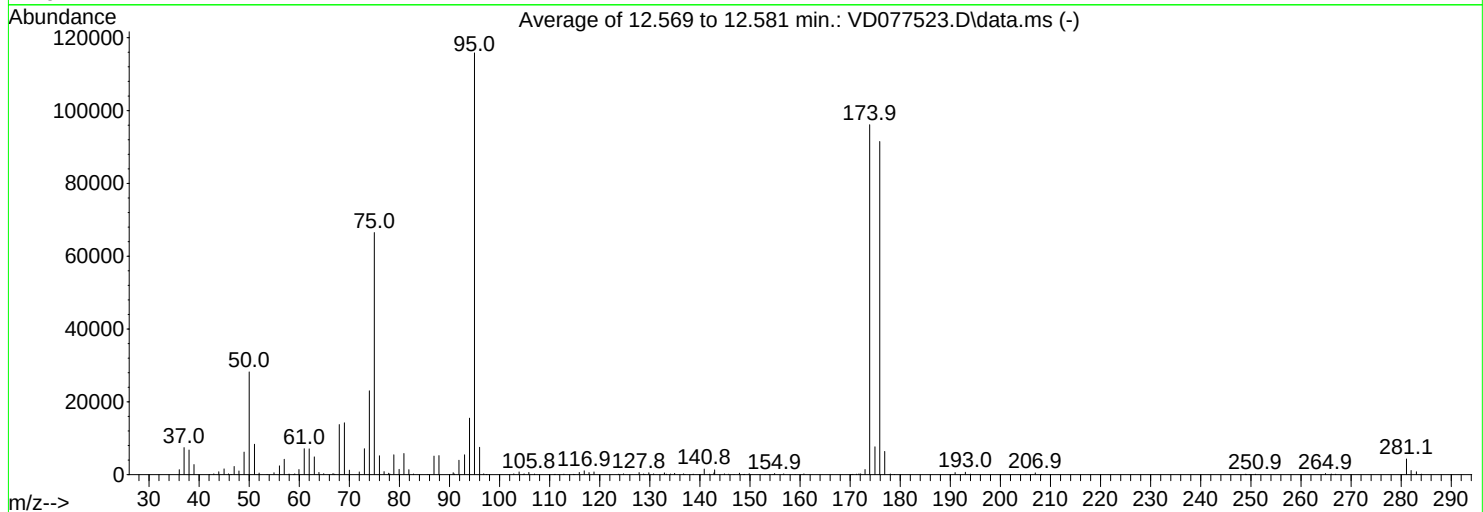


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110923\
Data File : VD077523.D
Acq On : 09 Nov 2023 07:54
Operator : JC/SY
Sample : BFB175
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB175

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Title : SFAM01.0
Last Update : Fri Nov 10 02:07:44 2023

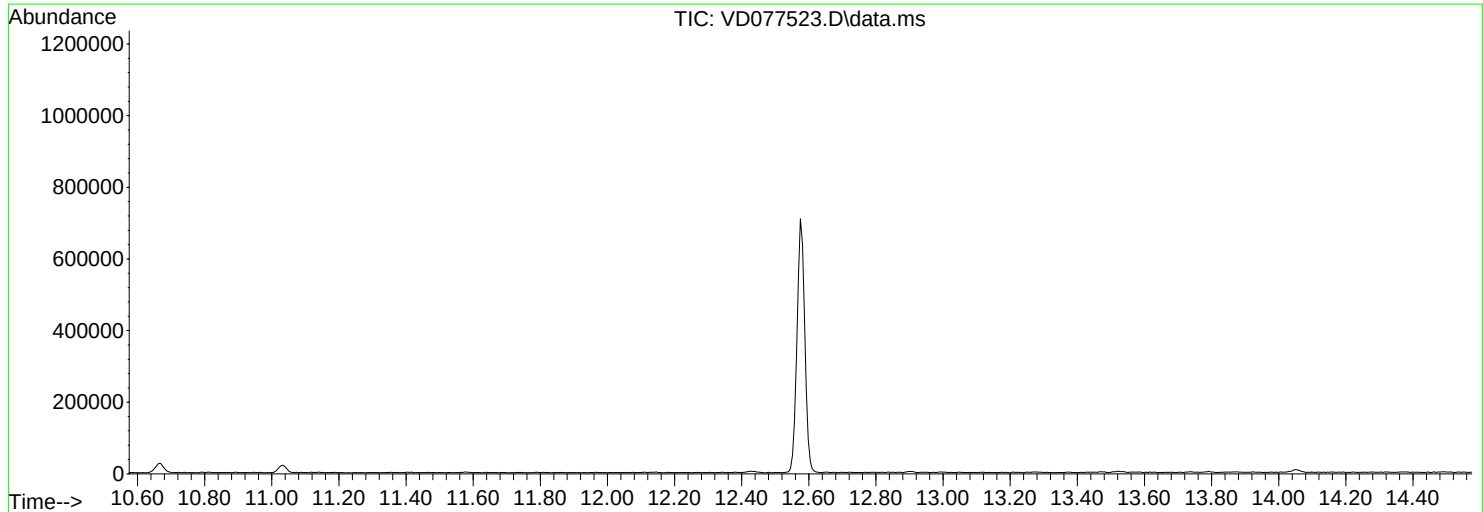

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.3	28203	PASS
75	95	30	80	57.4	66493	PASS
95	95	100	100	100.0	115851	PASS
96	95	5	9	6.5	7531	PASS
173	174	0.00	2	1.5	1421	PASS
174	95	50	120	83.0	96099	PASS
175	174	5	9	8.0	7660	PASS
176	174	95	105	95.2	91523	PASS
177	176	5	10	6.9	6358	PASS

m/z	Abundance
40.00	2277.0
41.00	158.0
42.60	156.0
44.00	1264.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175

m/z	Abundance
36.10	1236.0
37.00	6882.0
38.00	5846.0
39.00	2408.0
40.00	1878.0
42.90	237.0
44.00	2053.0
45.00	1340.0
45.90	218.0
47.00	2380.0
48.00	1075.0
49.00	4943.0
50.00	25760.0
51.00	8092.0
52.00	345.0
53.60	169.0
55.00	373.0
56.00	2082.0
57.00	4065.0
58.90	176.0
59.90	1128.0
61.00	6682.0
62.00	6339.0
63.00	4315.0
64.00	769.0
64.90	234.0
66.80	417.0
68.00	12453.0
69.00	12723.0
70.00	899.0
72.00	590.0
73.00	6443.0
74.00	21576.0
75.00	57872.0
76.00	4830.0
76.90	643.0
77.90	371.0
78.90	4488.0
79.90	1368.0
80.90	4984.0
81.90	1276.0
82.80	170.0
86.90	4313.0
87.90	4068.0
90.70	533.0
91.00	533.0
91.90	3238.0
93.00	5115.0
94.00	12522.0
95.00	101160.0
96.00	6297.0
96.90	217.0
97.40	171.0
102.80	264.0
103.90	470.0
104.70	193.0
106.00	670.0
107.10	203.0
112.80	174.0
115.90	588.0
117.00	739.0
117.90	512.0
118.80	551.0
123.80	180.0
124.90	193.0
127.90	528.0
128.80	241.0
129.90	599.0
130.90	235.0
133.10	271.0
134.20	156.0
135.00	264.0
136.70	415.0
138.70	168.0
140.80	1143.0
142.80	1455.0
144.90	208.0
147.90	419.0
150.00	319.0
153.80	192.0
154.90	364.0
156.80	238.0
160.80	238.0
170.60	170.0
171.30	176.0
171.80	366.0
173.00	1039.0
173.90	84568.0
174.90	6359.0
175.90	76056.0
176.90	5869.0
178.00	235.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175

191.00	431.0
193.10	571.0
206.90	447.0
266.10	177.0
281.10	2774.0
282.10	888.0
283.10	493.0
283.90	161.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175

m/z	Abundance
36.00	1584.0
37.00	8507.0
38.00	8364.0
39.00	3266.0
40.00	1458.0
42.10	173.0
43.00	169.0
44.00	2015.0
45.00	1697.0
45.80	209.0
46.40	176.0
47.00	2515.0
48.00	939.0
49.00	7521.0
50.00	31856.0
51.00	9339.0
52.00	463.0
54.90	674.0
56.10	2820.0
57.00	4643.0
58.00	292.0
59.10	447.0
60.00	1533.0
61.00	7983.0
62.00	7753.0
63.00	5546.0
64.00	587.0
65.00	329.0
66.70	272.0
67.10	373.0
68.00	15432.0
69.00	15892.0
70.00	1382.0
72.10	1057.0
73.00	7643.0
74.00	25408.0
75.00	75256.0
76.00	5502.0
76.90	857.0
77.80	837.0
78.90	6503.0
80.00	1586.0
80.90	6713.0
81.90	1511.0
82.80	350.0
85.70	192.0
86.90	5178.0
87.90	6376.0
90.80	525.0
91.90	4044.0
93.00	6271.0
94.00	17208.0
95.00	130296.0
96.00	9051.0
96.90	197.0
102.80	210.0
103.90	963.0
104.90	275.0
105.80	598.0
106.90	349.0
110.90	254.0
111.10	260.0
112.90	179.0
114.80	273.0
115.90	826.0
116.80	1080.0
117.80	573.0
118.90	1070.0
124.70	203.0
127.80	669.0
129.00	249.0
129.80	488.0
130.70	223.0
132.90	675.0
134.10	346.0
134.90	459.0
137.00	287.0
138.60	236.0
140.00	153.0
140.90	1716.0
141.90	226.0
143.00	1816.0
144.90	340.0
145.70	197.0
147.80	479.0
148.70	178.0
149.80	229.0
153.00	198.0
154.60	166.0
155.00	173.0
156.70	273.0
160.70	232.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175

170.00	168.0
170.50	155.0
171.20	186.0
172.10	619.0
172.90	1490.0
173.90	104512.0
174.90	8392.0
175.90	101984.0
176.90	7024.0
190.90	806.0
193.00	615.0
194.00	351.0
205.10	248.0
206.90	491.0
208.20	235.0
248.90	369.0
249.80	171.0
250.90	171.0
264.90	470.0
266.00	155.0
266.90	167.0
281.10	4770.0
282.00	1316.0
282.90	623.0
284.10	364.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175

m/z	Abundance
36.00	1322.0
37.00	6925.0
38.00	6078.0
39.00	2673.0
39.90	2252.0
40.80	204.0
42.90	258.0
43.90	2050.0
45.00	1732.0
46.00	238.0
47.00	1806.0
47.90	1050.0
49.00	6164.0
50.00	26992.0
51.10	7586.0
52.00	525.0
55.00	528.0
56.00	2378.0
57.00	3897.0
57.90	191.0
59.10	282.0
59.90	1579.0
61.00	6727.0
62.00	7104.0
63.00	4791.0
63.90	458.0
64.80	285.0
66.80	278.0
68.00	13342.0
69.00	14094.0
70.00	1458.0
71.90	625.0
73.00	7246.0
74.00	22096.0
75.00	66352.0
76.00	5182.0
77.00	1062.0
78.10	578.0
78.90	5421.0
79.90	1414.0
80.90	5768.0
81.90	1344.0
86.90	5762.0
87.90	5194.0
90.80	468.0
91.90	4653.0
93.00	4909.0
94.00	16792.0
95.00	116096.0
96.00	7245.0
96.80	275.0
102.90	219.0
103.90	788.0
104.90	341.0
105.80	572.0
109.90	190.0
111.70	199.0
115.00	189.0
115.80	445.0
116.90	1301.0
117.80	610.0
118.80	631.0
123.80	158.0
124.70	244.0
127.90	466.0
128.70	348.0
129.70	550.0
130.60	235.0
132.80	475.0
133.30	378.0
135.00	324.0
136.70	295.0
140.90	1768.0
141.90	222.0
142.90	2195.0
145.00	182.0
145.80	192.0
146.80	184.0
148.00	242.0
148.90	210.0
149.80	184.0
154.80	341.0
156.80	180.0
159.00	186.0
160.80	199.0
170.20	188.0
171.70	324.0
173.00	1733.0
173.90	99216.0
175.00	8229.0
175.90	96528.0
176.90	6180.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175

178.00	276.0
178.80	175.0
190.90	464.0
192.90	819.0
207.00	516.0
249.10	303.0
250.90	213.0
264.90	397.0
266.00	217.0
267.00	200.0
281.00	5390.0
281.90	1178.0
283.10	1206.0

Instrument :
MSVOA_D
ClientSampleId :
BFB175