
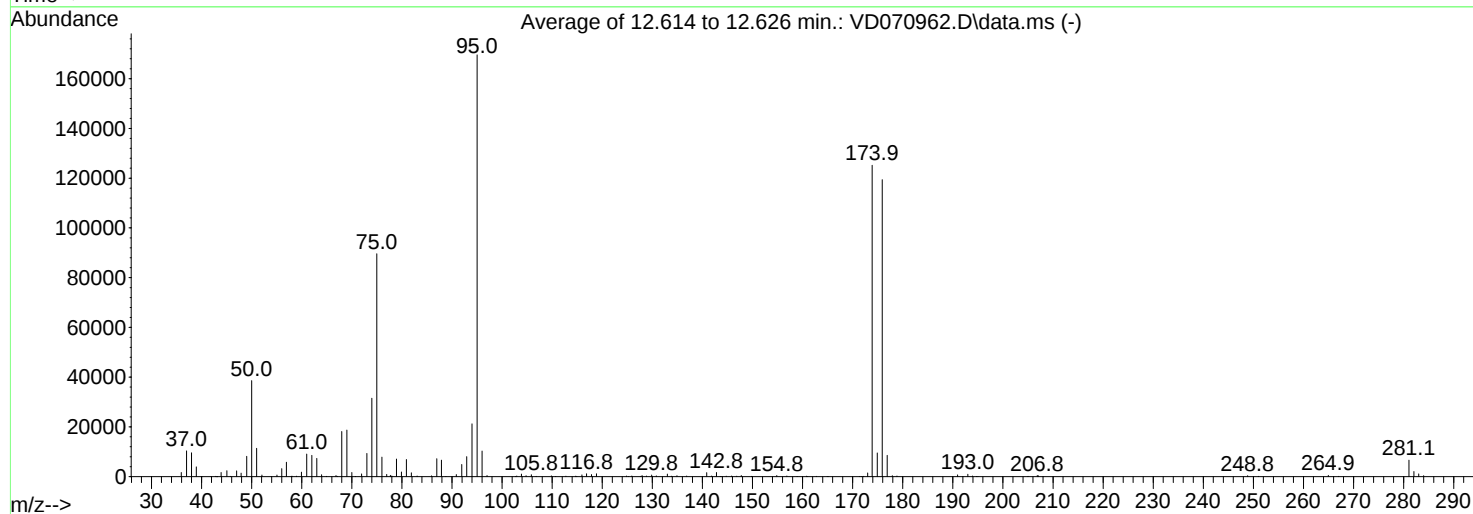


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111021\
Data File : VD070962.D
Acq On : 10 Nov 2021 09:01
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
Title : SW846 8260
Last Update : Wed Nov 10 03:55:51 2021

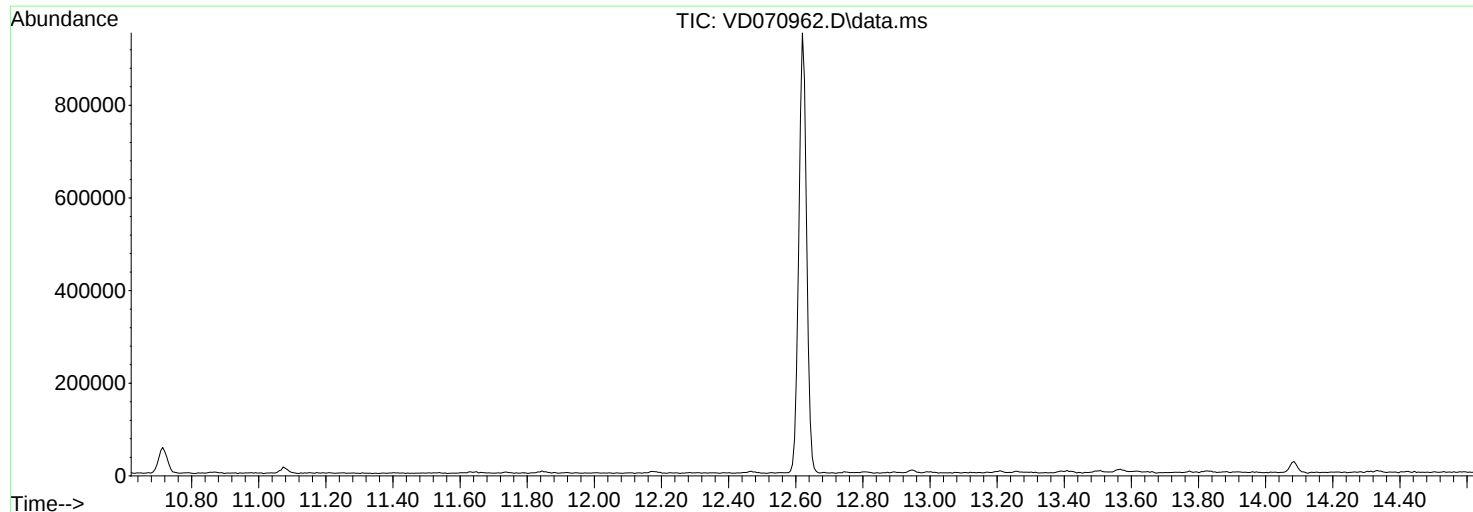

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.8	38616	PASS
75	95	30	60	52.9	89640	PASS
95	95	100	100	100.0	169579	PASS
96	95	5	9	6.1	10303	PASS
173	174	0.00	2	1.2	1519	PASS
174	95	50	100	73.8	125157	PASS
175	174	5	9	7.6	9545	PASS
176	174	95	101	95.4	119365	PASS
177	176	5	9	7.2	8555	PASS