
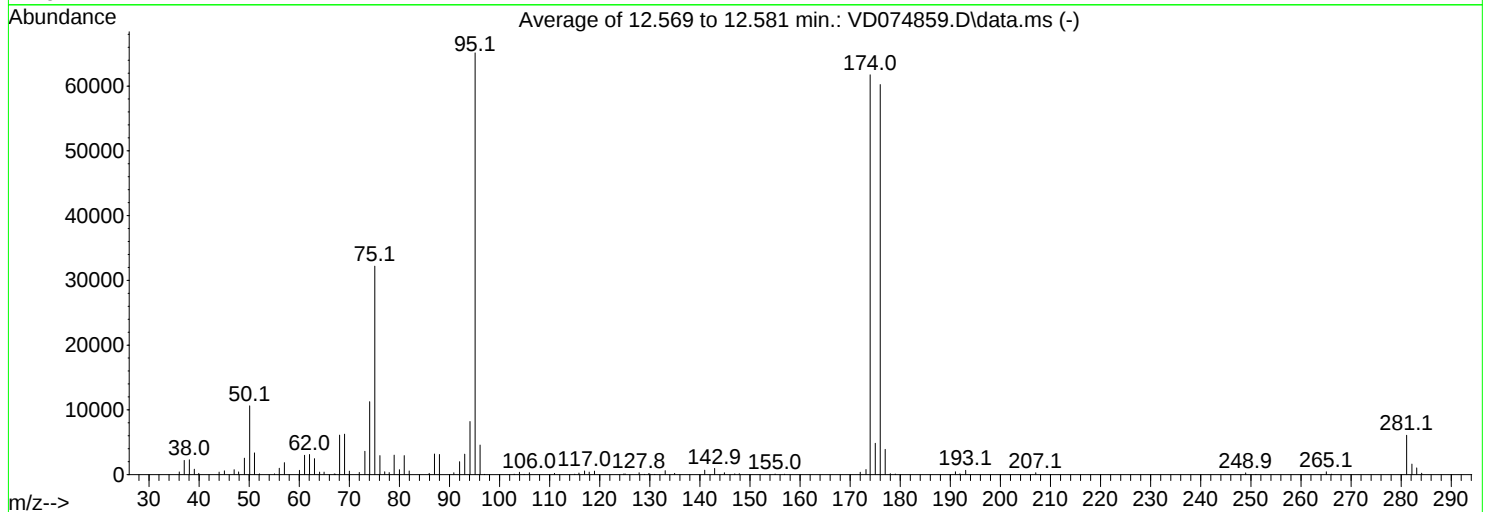


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111022\
Data File : VD074859.D
Acq On : 10 Nov 2022 09:03
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
Title : SW846 8260
Last Update : Thu Nov 03 02:30:45 2022

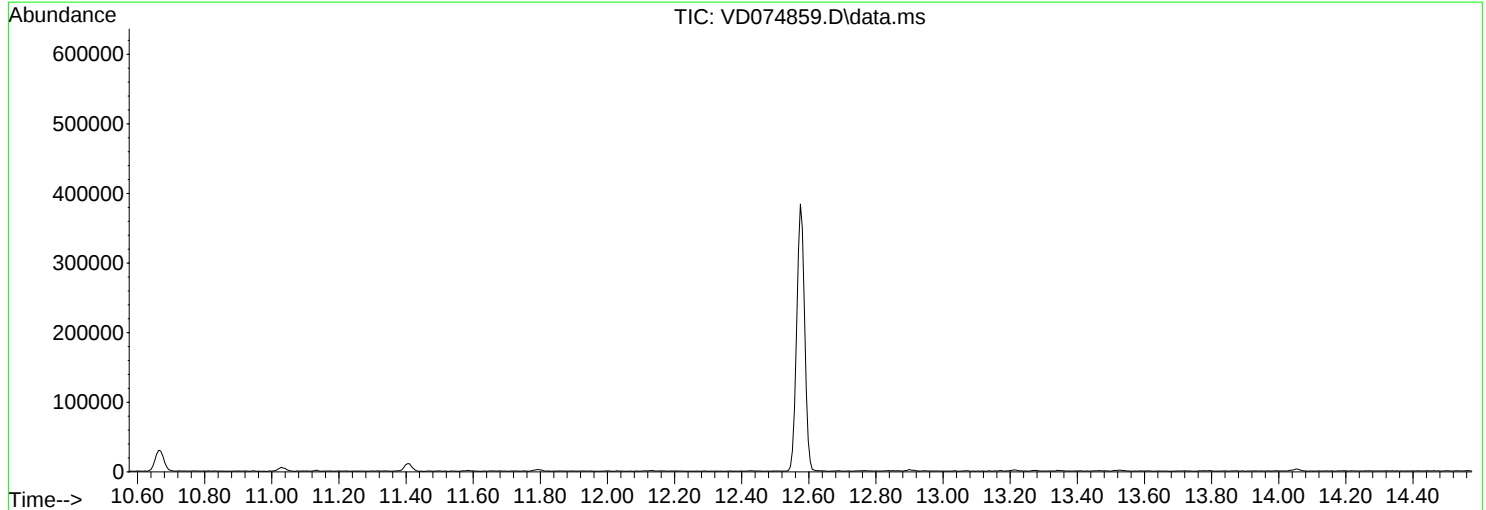

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	10627	PASS
75	95	30	60	49.4	32197	PASS
95	95	100	100	100.0	65133	PASS
96	95	5	9	7.0	4567	PASS
173	174	0.00	2	1.3	788	PASS
174	95	50	100	94.8	61747	PASS
175	174	5	9	7.8	4836	PASS
176	174	95	101	97.5	60232	PASS
177	176	5	9	6.5	3904	PASS