

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111121\
 Data File : VD070988.D
 Acq On : 11 Nov 2021 13:34
 Operator : VA/SY
 Sample : M4576-01
 Misc : 4.54G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Nov 12 08:00:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 10 03:55:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.973	168	190504	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	379781	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	190939	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.549	152	600989	50.000	ug/l	#-0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	158149	77.971	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 155.940%			
35) Dibromofluoromethane	7.908	113	141554	66.053	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 132.100%			
50) Toluene-d8	10.332	98	323157	38.505	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 77.000%			
62) 4-Bromofluorobenzene	12.620	95	410788	135.939	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 271.880%#			
Target Compounds						Qvalue
10) Methyl Iodide	4.285	142	201	6.102	ug/l #	40
11) Tert butyl alcohol	5.209	59	162	1.093	ug/l #	71
13) Acrolein	4.144	56	82	Below Cal	#	13
16) Acetone	4.162	43	4563	27.467	ug/l #	69
17) Carbon Disulfide	4.409	76	19777	3.386	ug/l #	92
23) Vinyl Acetate	6.285	43	161	21.019	ug/l #	72
25) 2-Butanone	7.208	43	843	21.461	ug/l #	45
31) Cyclohexane	7.955	56	26257	6.295	ug/l #	65
38) Carbon Tetrachloride	7.979	117	20431	6.543	ug/l #	17
41) Methacrylonitrile	7.520	41	191	3.662	ug/l #	28
43) Isopropyl Acetate	8.444	43	5516	1.685	ug/l #	47
55) 1,1,2-Trichloroethane	10.773	97	5740	3.398	ug/l #	29
56) Ethyl methacrylate	10.673	69	4033	1.687	ug/l #	1
59) 2-Hexanone	10.944	43	15218	27.413	ug/l #	30
61) 1,2-Dibromoethane	11.126	107	1804	1.098	ug/l #	1
65) Chlorobenzene	11.773	112	205649	60.365	ug/l #	42
67) Ethyl Benzene	11.773	91	39107	6.062	ug/l #	48
68) m/p-Xylenes	11.849	106	3048	1.264	ug/l #	1
74) N-amyl acetate	12.267	43	1642810	132.814	ug/l #	49
75) 1,1,2,2-Tetrachloroethane	12.691	83	1292545	173.443	ug/l #	68
76) 1,2,3-Trichloropropane	12.620	75	38984	7.594	ug/l	25
77) Bromobenzene	12.720	156	13532	1.463	ug/l #	1
78) n-propylbenzene	12.791	91	91051	1.697	ug/l #	58
79) 2-Chlorotoluene	12.961	91	623037	20.368	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.473	75	2521	4.238	ug/l #	1
82) 4-Chlorotoluene	12.961	91	623037	19.735	ug/l	98
89) n-Butylbenzene	13.849	91	128777	3.457	ug/l #	43
92) 1,2-Dibromo-3-Chloropr...	14.561	75	17927	14.667	ug/l #	4
93) 1,2,4-Trichlorobenzene	15.132	180	10283	1.025	ug/l #	1
96) 1,2,3-Trichlorobenzene	15.543	180	16474	1.954	ug/l #	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111121\
Data File : VD070988.D
Acq On : 11 Nov 2021 13:34
Operator : VA/SY
Sample : M4576-01
Misc : 4.54G/5.00ml/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :


Quant Time: Nov 12 08:00:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 10 03:55:51 2021
Response via : Initial Calibration

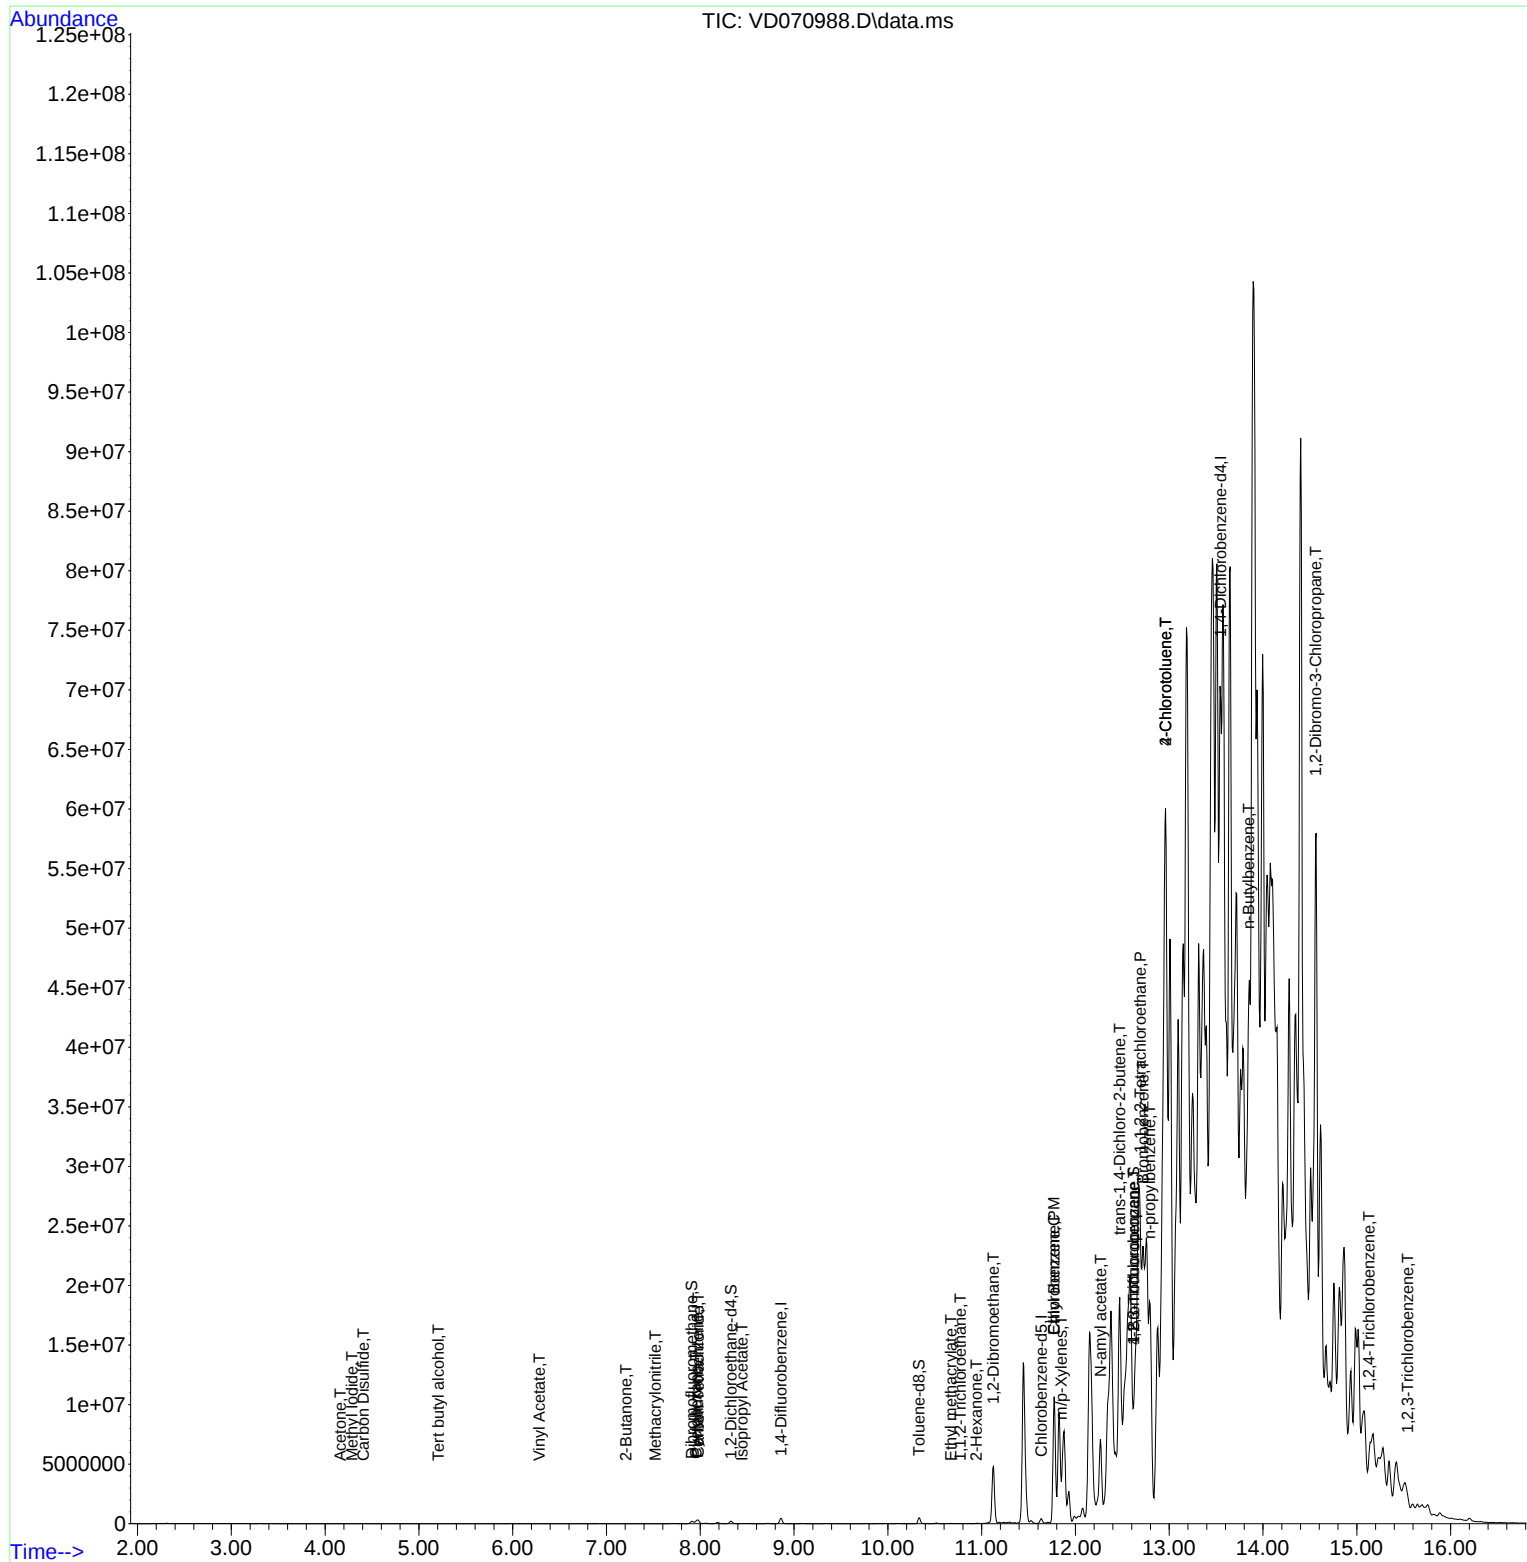



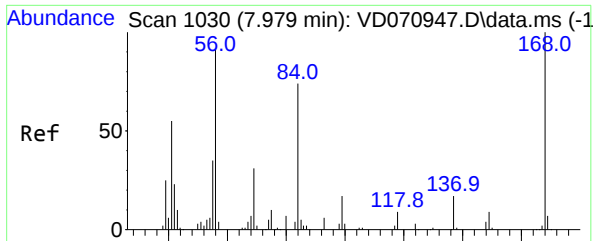


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :



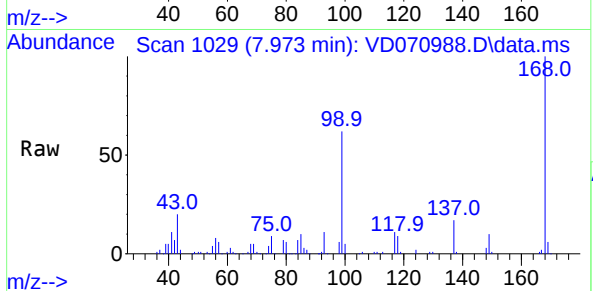



Tgt Ion:168 Resp: 190504
Ion Ratio Lower Upper
168 100
99 62.2 46.6 69.8

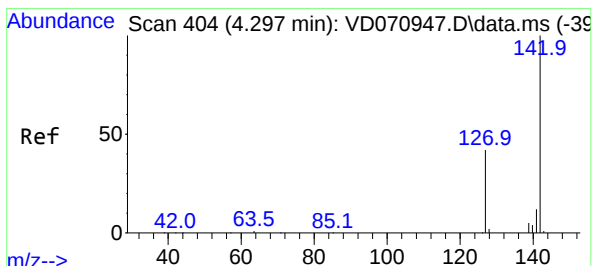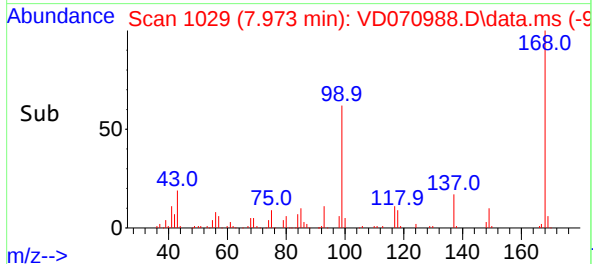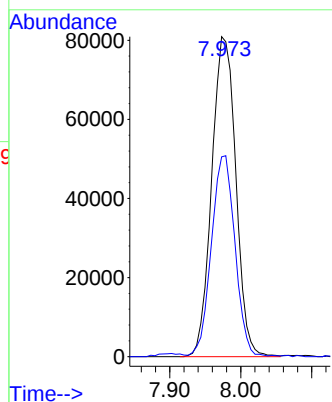

#10
Methyl Iodide
Concen: 6.102 ug/l
RT: 4.285 min Scan# 402
Delta R.T. -0.012 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion:142 Resp: 201
Ion Ratio Lower Upper
142 100
127 0.0 35.0 52.4#
141 0.0 12.0 18.0#

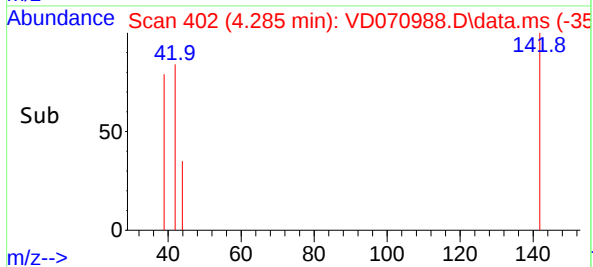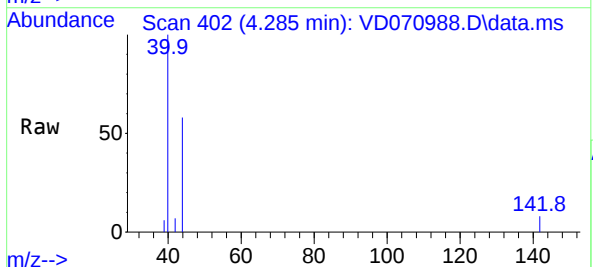






#11
Tert butyl alcohol
Concen: 1.093 ug/l
RT: 5.209 min Scan# 51
Delta R.T. -0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion: 59 Resp: 162
Ion Ratio Lower Upper
59 100
57 0.0 9.0 13.4#

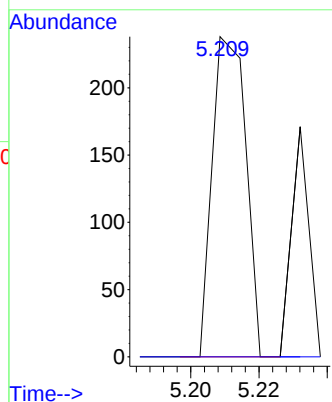

#13
Acrolein
Concen: Below Cal
RT: 4.144 min Scan# 378
Delta R.T. 0.218 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Tgt Ion: 56 Resp: 82
Ion Ratio Lower Upper
56 100
55 0.0 58.6 87.8#









#16
Acetone
Concen: 27.467 ug/l
RT: 4.162 min Scan# 381
Delta R.T. 0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 4563
Ion Ratio Lower Upper
43 100
58 17.0 27.8 41.8#



#17
Carbon Disulfide
Concen: 3.386 ug/l
RT: 4.409 min Scan# 423
Delta R.T. -0.000 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Tgt Ion: 76 Resp: 19777
Ion Ratio Lower Upper
76 100
78 7.0 7.8 11.8#









#23
 Vinyl Acetate
 Concen: 21.019 ug/l
 RT: 6.285 min Scan# 745
 Delta R.T. -0.018 min
 Lab File: VD070988.D
 Acq: 11 Nov 2021 13:34




Instrument :
 MSVOA_D
 ClientSampleId :


Tgt Ion: 43 Resp: 161
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.2 12.4#

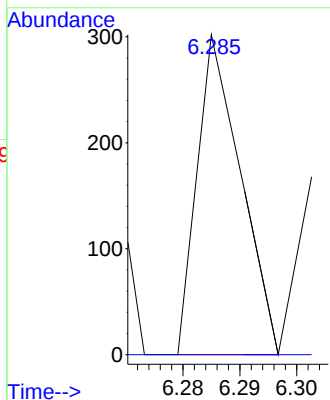

#25
 2-Butanone
 Concen: 21.461 ug/l
 RT: 7.208 min Scan# 899
 Delta R.T. -0.001 min
 Lab File: VD070988.D
 Acq: 11 Nov 2021 13:34


Tgt Ion: 43 Resp: 843
 Ion Ratio Lower Upper
 43 100
 72 0.0 23.8 35.6#

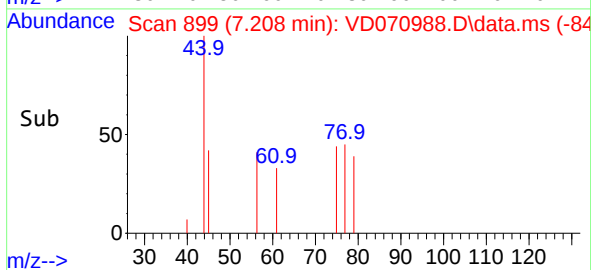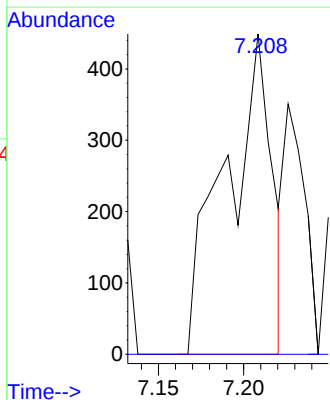



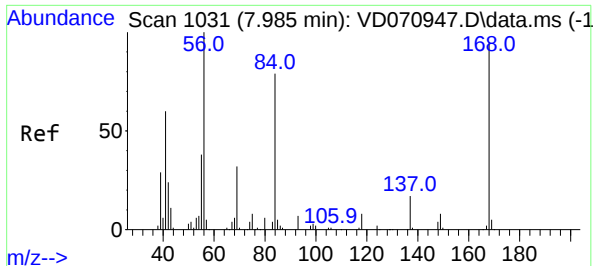


#31
Cyclohexane
Concen: 6.295 ug/l
RT: 7.955 min Scan# 1026
Delta R.T. -0.030 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :



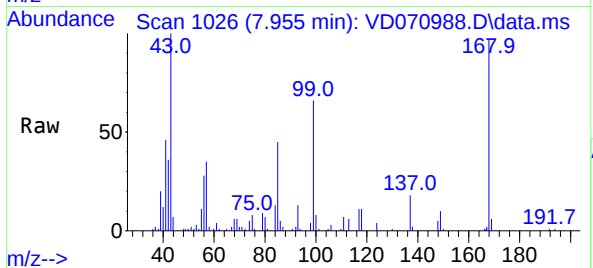



Tgt Ion: 56 Resp: 26257
Ion Ratio Lower Upper
56 100
69 20.4 25.9 38.9#
84 44.8 64.3 96.5#

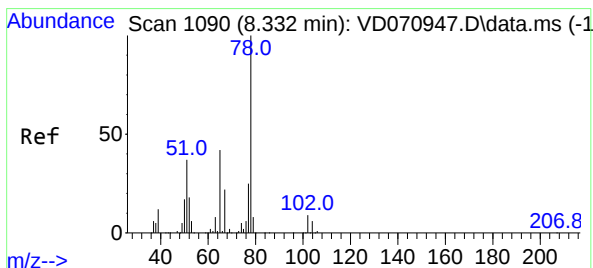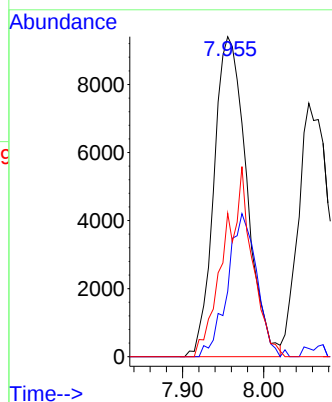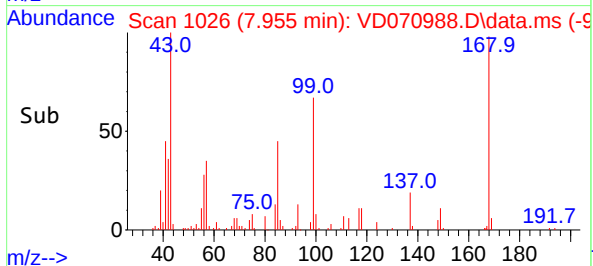

#33
1,2-Dichloroethane-d4
Concen: 77.971 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Tgt Ion: 65 Resp: 158149
Ion Ratio Lower Upper
65 100
67 51.4 0.0 112.2



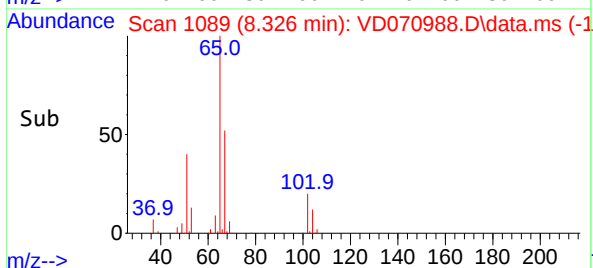
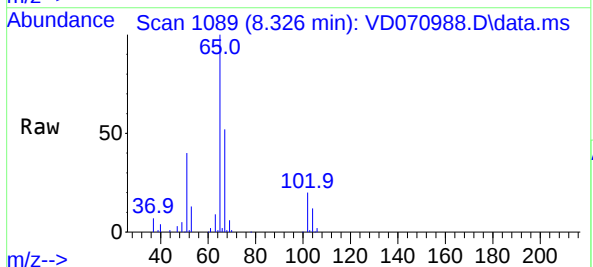


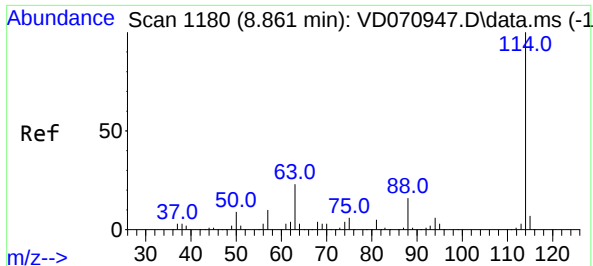

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:114 Resp: 379781
Ion Ratio Lower Upper
114 100
63 21.6 0.0 41.8
88 16.3 0.0 32.8

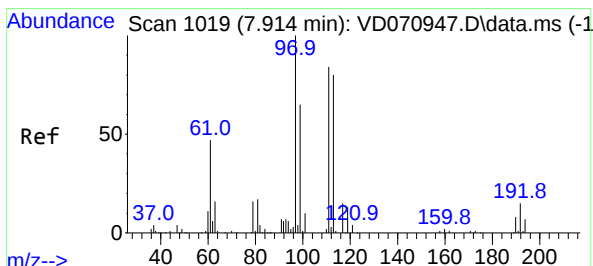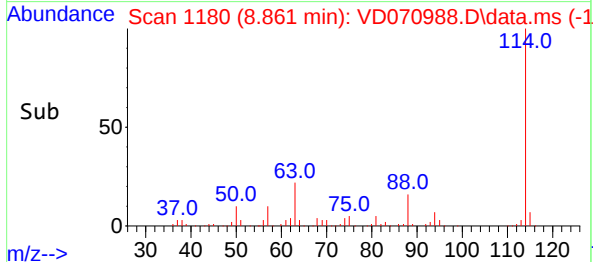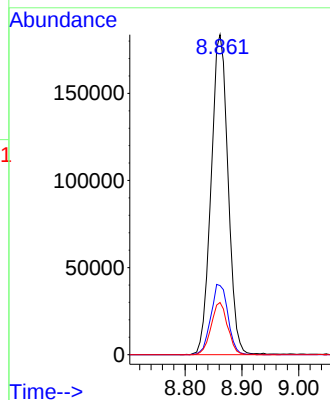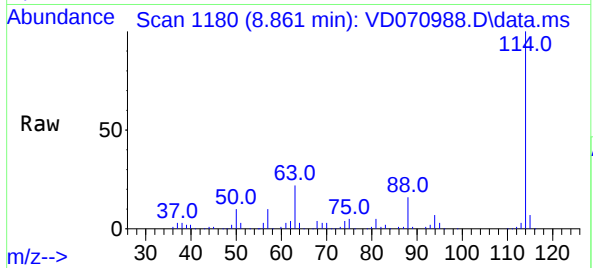

#35
Dibromofluoromethane
Concen: 66.053 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion:113 Resp: 141554
Ion Ratio Lower Upper
113 100
111 100.6 82.0 123.0
192 18.1 15.2 22.8

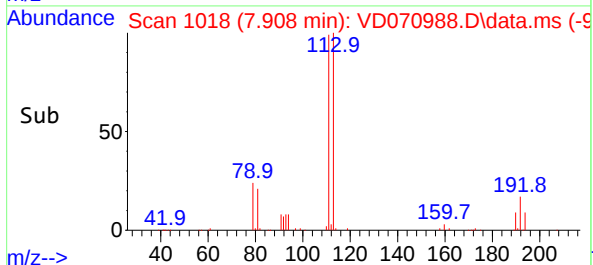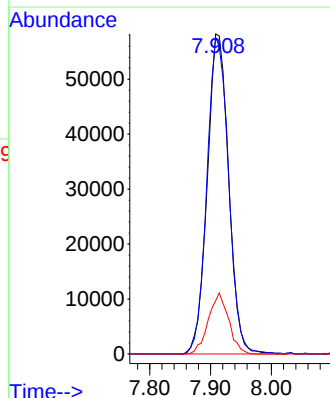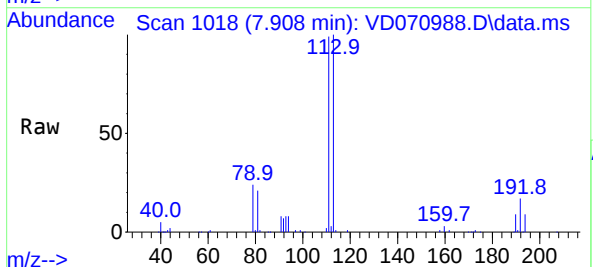






#38
Carbon Tetrachloride
Concen: 6.543 ug/l
RT: 7.979 min Scan# 1050
Delta R.T. -0.118 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion:117 Resp: 20431
Ion Ratio Lower Upper
117 100
119 6.2 75.8 113.6#
121 0.0 23.6 35.4#



#41
Methacrylonitrile
Concen: 3.662 ug/l
RT: 7.520 min Scan# 952
Delta R.T. 0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Tgt Ion: 41 Resp: 191
Ion Ratio Lower Upper
41 100
39 36.6 60.2 90.4#
67 0.0 74.8 112.2#
52 0.0 28.8 43.2#


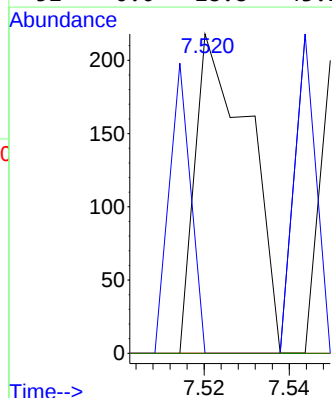




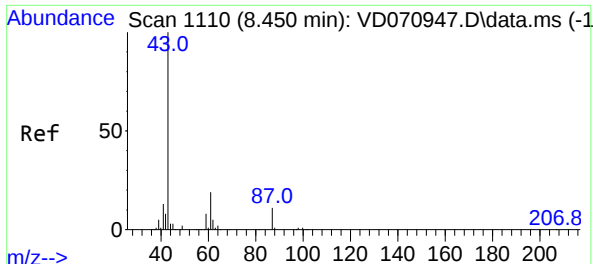

#43
Isopropyl Acetate
Concen: 1.685 ug/l
RT: 8.444 min Scan# 1110
Delta R.T. -0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 5516
Ion Ratio Lower Upper
43 100
61 0.0 28.2 42.4#
87 0.0 10.7 16.1#

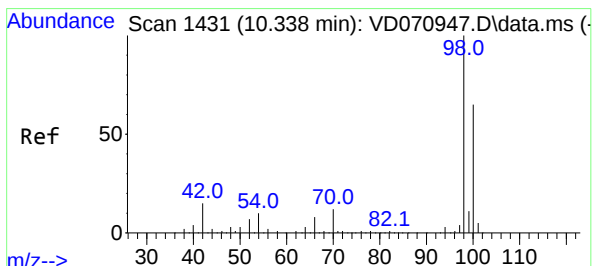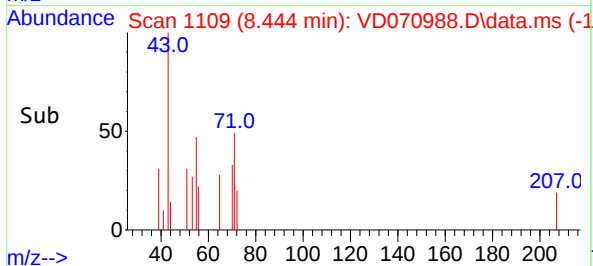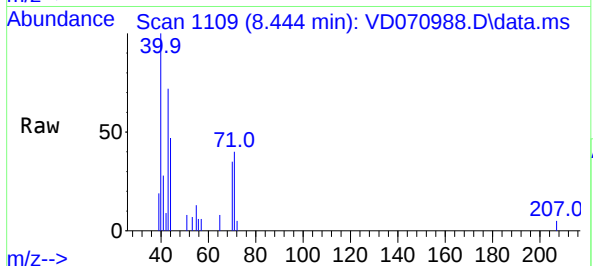

#50
Toluene-d8
Concen: 38.505 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.006 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion: 98 Resp: 323157
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.6

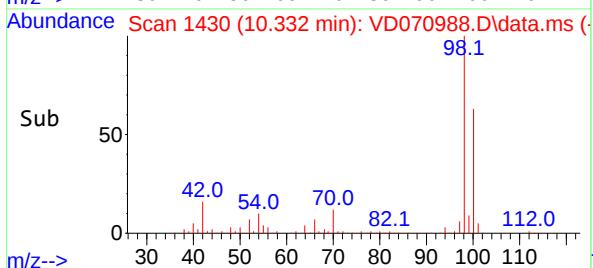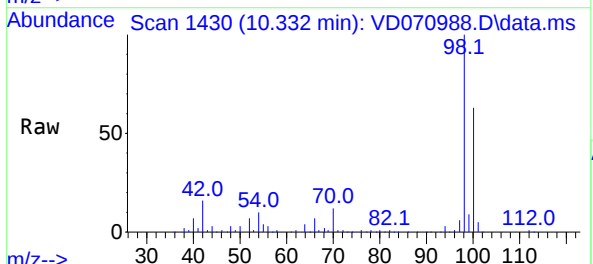






#55
1,1,2-Trichloroethane
Concen: 3.398 ug/l
RT: 10.773 min Scan# 1505
Delta R.T. -0.018 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion:	97	Resp:	5740
Ion	Ratio	Lower	Upper
97	100		
83	18.1	65.2	97.8#
85	13.8	43.4	65.0#
99	0.0	52.1	78.1#

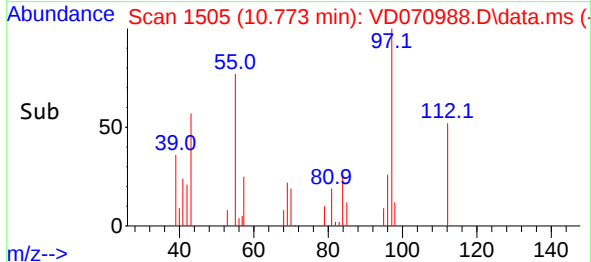


#56
Ethyl methacrylate
Concen: 1.687 ug/l
RT: 10.673 min Scan# 1488
Delta R.T. 0.018 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34



Tgt Ion:	69	Resp:	4033
Ion	Ratio	Lower	Upper
69	100		
41	182.3	50.2	75.2#
39	80.5	19.8	29.8#

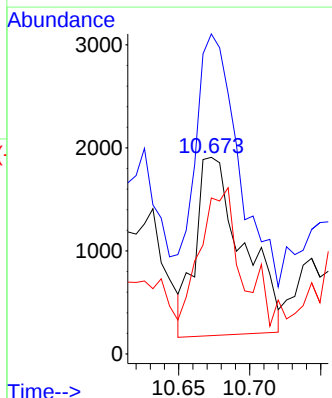



#59

2-Hexanone

Concen: 27.413 ug/l

RT: 10.944 min Scan# 1534

Delta R.T. -0.035 min

Lab File: VD070988.D

Acq: 11 Nov 2021 13:34

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 43 Resp: 15218

Ion Ratio Lower Upper

43 100

58 5.6 28.7 86.1#

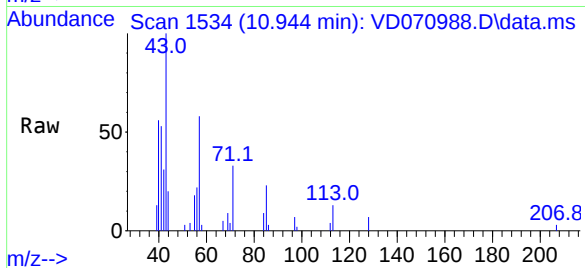

#61

1,2-Dibromoethane

Concen: 1.098 ug/l

RT: 11.126 min Scan# 1565

Delta R.T. -0.112 min

Lab File: VD070988.D




Acq: 11 Nov 2021 13:34


Tgt Ion:107 Resp: 1804

Ion Ratio Lower Upper

107 100

109 1357.9 74.6 112.0#


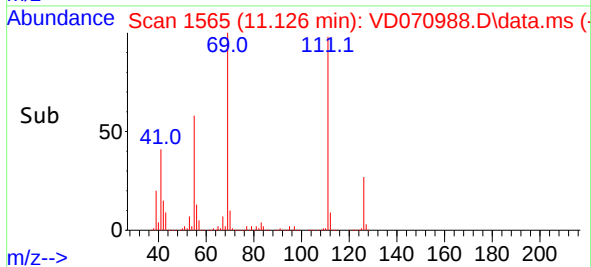

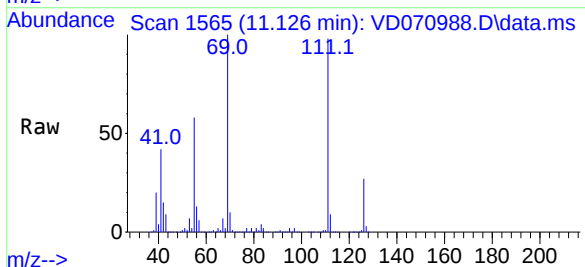


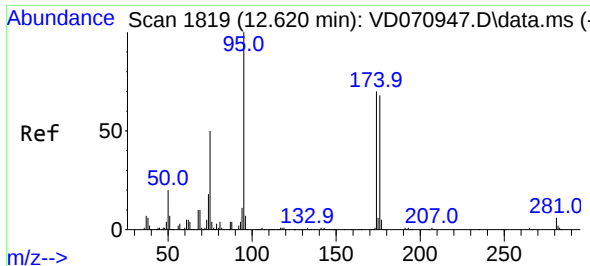

#62
4-Bromofluorobenzene
Concen: 135.939 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 95 Resp: 410788
Ion Ratio Lower Upper
95 100
174 10.6 0.0 159.4
176 10.5 0.0 154.0

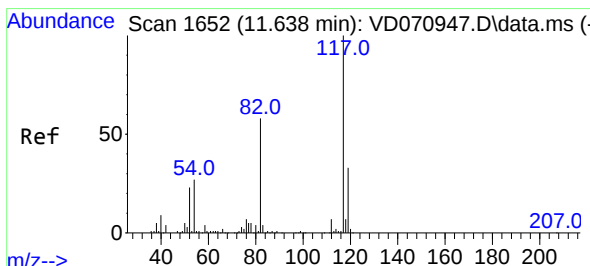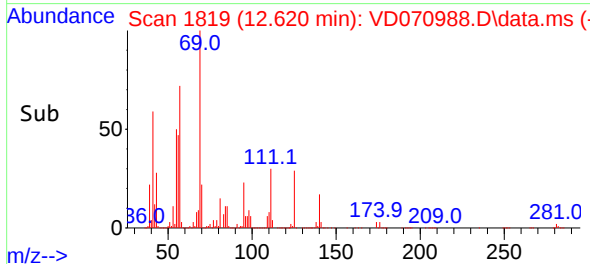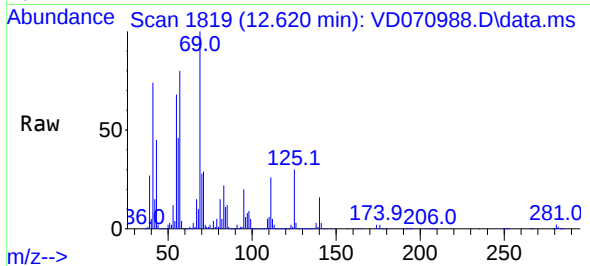

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion: 117 Resp: 190939
Ion Ratio Lower Upper
117 100
82 56.7 44.7 67.1
119 31.3 26.2 39.4

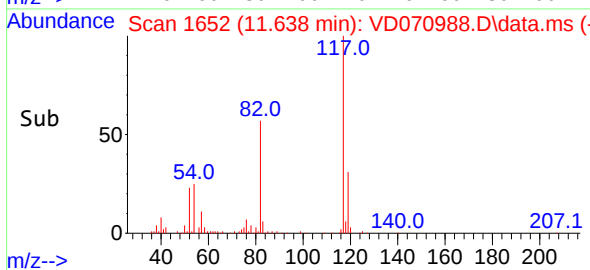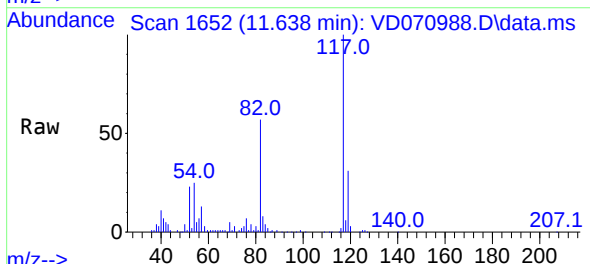



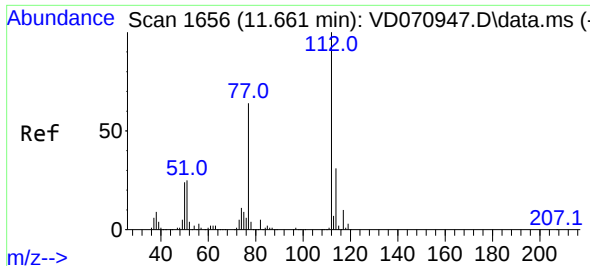


#65
Chlorobenzene
Concen: 60.365 ug/l
RT: 11.773 min Scan# 1675
Delta R.T. 0.112 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :



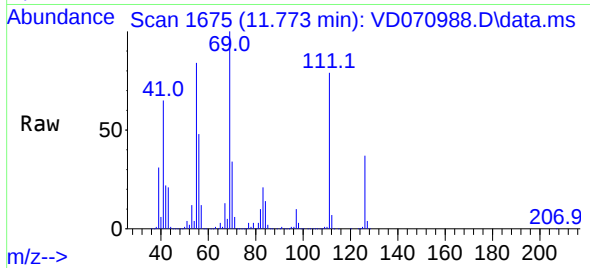



Tgt Ion:112 Resp: 205649
Ion Ratio Lower Upper
112 100
114 0.0 26.0 39.0#

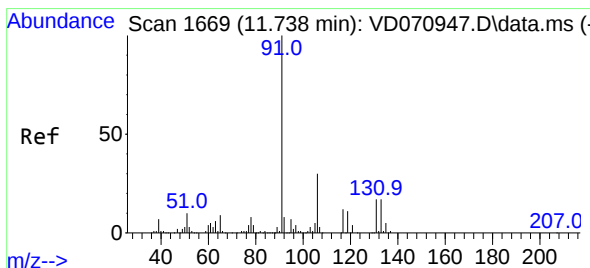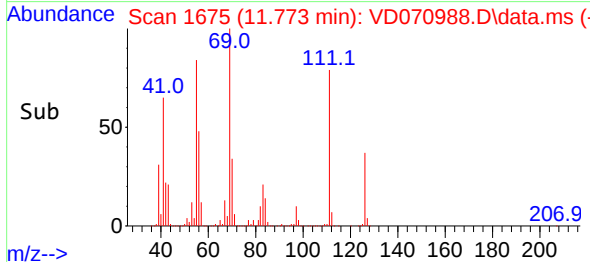

#67
Ethyl Benzene
Concen: 6.062 ug/l
RT: 11.773 min Scan# 1675
Delta R.T. 0.035 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Tgt Ion: 91 Resp: 39107
Ion Ratio Lower Upper
91 100
106 2.5 24.6 36.8#


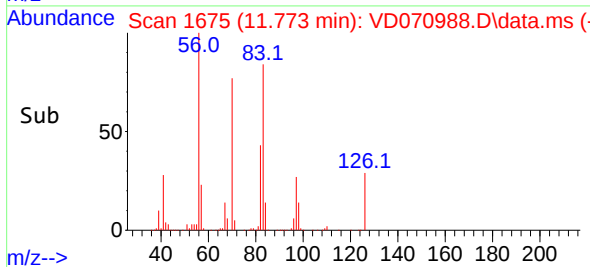

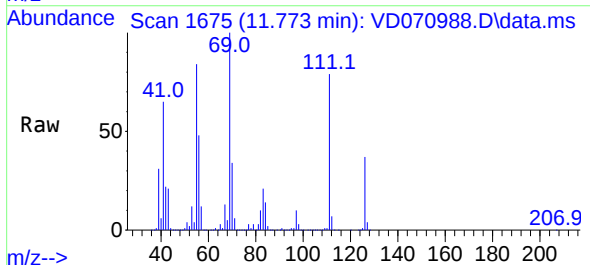




#68
m/p-Xylenes
Concen: 1.264 ug/l
RT: 11.849 min Scan# 11
Delta R.T. 0.005 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:106 Resp: 3048
Ion Ratio Lower Upper
106 100
91 0.0 160.1 240.1#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.549 min Scan# 1977
Delta R.T. -0.012 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion:152 Resp: 600989
Ion Ratio Lower Upper
152 100
115 6.2 29.8 89.3#
150 8.1 0.0 349.2

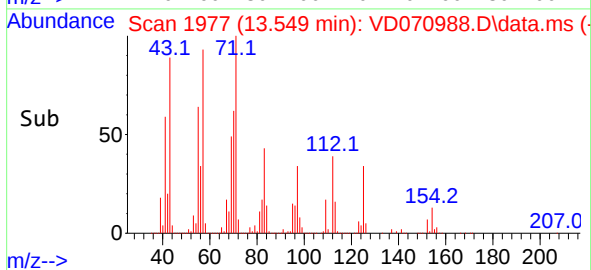






#74
N-amy1 acetate
Concen: 132.814 ug/l
RT: 12.267 min Scan# 1
Delta R.T. -0.012 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion: 43 Resp: 1642810
Ion Ratio Lower Upper
43 100
70 13.6 36.6 55.0#
55 0.0 22.5 33.7#
61 0.0 20.5 30.7#

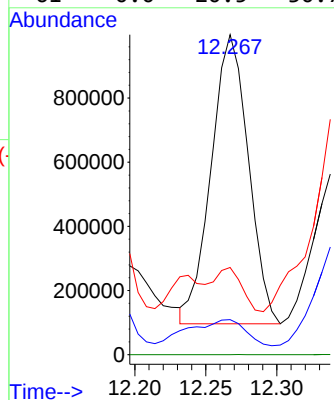


#75
1,1,2,2-Tetrachloroethane
Concen: 173.443 ug/l
RT: 12.691 min Scan# 1831
Delta R.T. -0.029 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34



Tgt Ion: 83 Resp: 1292545
Ion Ratio Lower Upper
83 100
131 0.0 4.9 14.7#
85 38.2 32.0 96.2

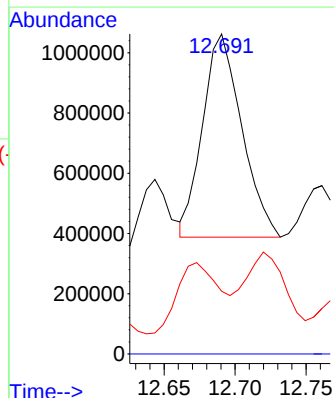



#76

1,2,3-Trichloropropane

Concen: 7.594 ug/l

RT: 12.620 min Scan# 1819

Delta R.T. -0.165 min

Lab File: VD070988.D

Acq: 11 Nov 2021 13:34

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 75 Resp: 38984

Ion Ratio Lower Upper

75 100

77 164.8 158.4 475.3

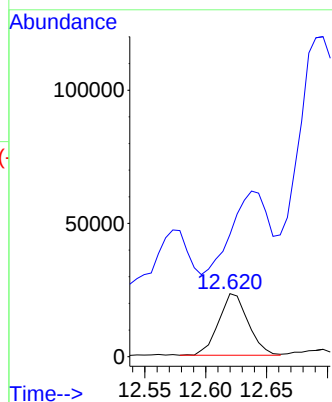

#77

Bromobenzene

Concen: 1.463 ug/l

RT: 12.720 min Scan# 1836

Delta R.T. -0.029 min

Lab File: VD070988.D

Acq: 11 Nov 2021 13:34




Tgt Ion:156 Resp: 13532


Ion Ratio Lower Upper

156 100

77 0.0 96.6 289.8#


158 0.0 49.1 147.4#

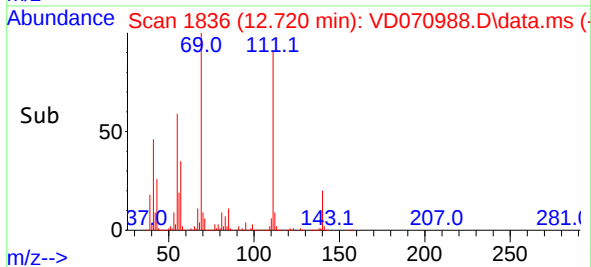






#78
n-propylbenzene
Concen: 1.697 ug/l
RT: 12.791 min Scan# 1848
Delta R.T. -0.017 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion: 91 Resp: 91051
Ion Ratio Lower Upper
91 100
120 1.8 10.9 32.9#

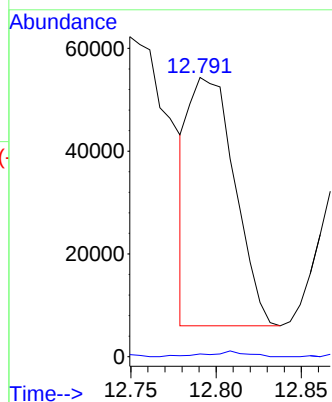

#79
2-Chlorotoluene
Concen: 20.368 ug/l
RT: 12.961 min Scan# 1877
Delta R.T. 0.065 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion: 91 Resp: 623037
Ion Ratio Lower Upper
91 100
126 31.6 16.6 49.7

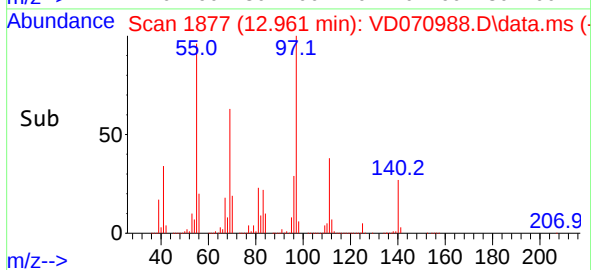






#81
trans-1,4-Dichloro-2-butene
Concen: 4.238 ug/l
RT: 12.473 min Scan# 1794
Delta R.T. -0.041 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion: 75 Resp: 2521
Ion Ratio Lower Upper
75 100
53 14908.5 62.6 94.0#
89 206.5 34.5 51.7#

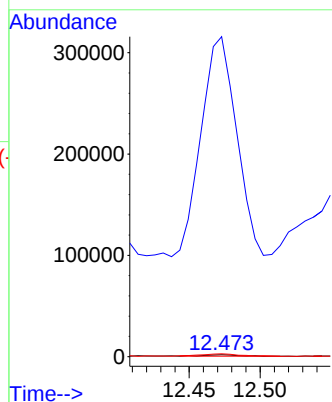

#82
4-Chlorotoluene
Concen: 19.735 ug/l
RT: 12.961 min Scan# 1877
Delta R.T. -0.035 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion: 91 Resp: 623037
Ion Ratio Lower Upper
91 100
126 31.6 16.4 49.1

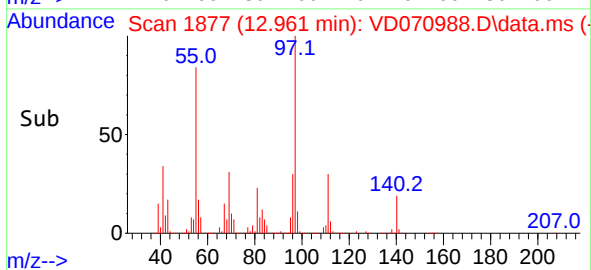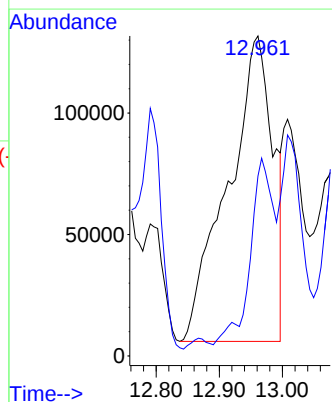






#89
n-Butylbenzene
Concen: 3.457 ug/l
RT: 13.849 min Scan# 2028
Delta R.T. 0.023 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion: 91 Resp: 128777
Ion Ratio Lower Upper
91 100
92 10.6 27.3 81.9#
134 0.0 12.3 36.9#

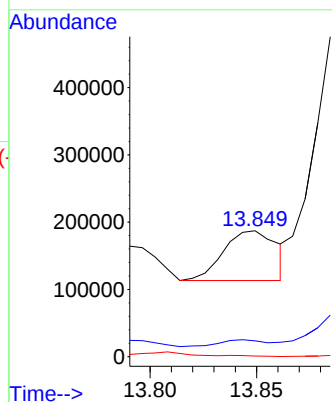

#92
1,2-Dibromo-3-Chloropropane
Concen: 14.667 ug/l
RT: 14.561 min Scan# 2149
Delta R.T. 0.070 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34


Tgt Ion: 75 Resp: 17927
Ion Ratio Lower Upper
75 100
155 0.0 40.0 120.0#
157 0.0 49.8 149.3#

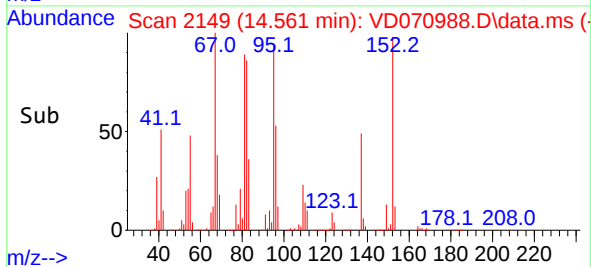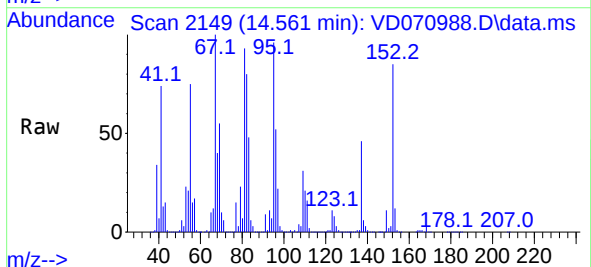






#93
1,2,4-Trichlorobenzene
Concen: 1.025 ug/l
RT: 15.132 min Scan# 21
Delta R.T. -0.011 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Instrument :
MSVOA_D
ClientSampleId :

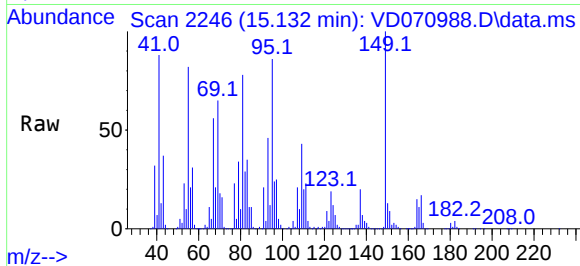

Tgt Ion:180 Resp: 10283
Ion Ratio Lower Upper
180 100
182 327.9 48.2 144.6#
145 50.4 15.4 46.2#



#96
1,2,3-Trichlorobenzene
Concen: 1.954 ug/l
RT: 15.543 min Scan# 2316
Delta R.T. -0.030 min
Lab File: VD070988.D
Acq: 11 Nov 2021 13:34

Tgt Ion:180 Resp: 16474
Ion Ratio Lower Upper
180 100
182 28.0 46.7 140.1#
145 7.7 15.9 47.6#

