
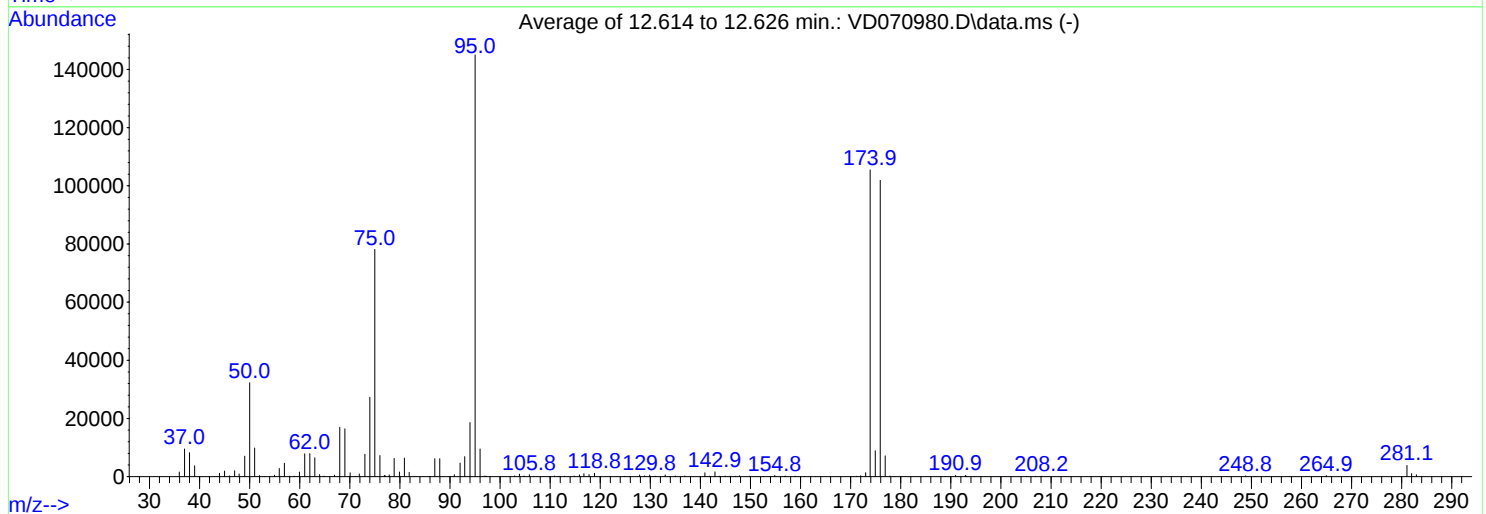


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111121\
 Data File : VD070980.D
 Acq On : 11 Nov 2021 09:02
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
 Title : SW846 8260
 Last Update : Wed Nov 10 03:55:51 2021

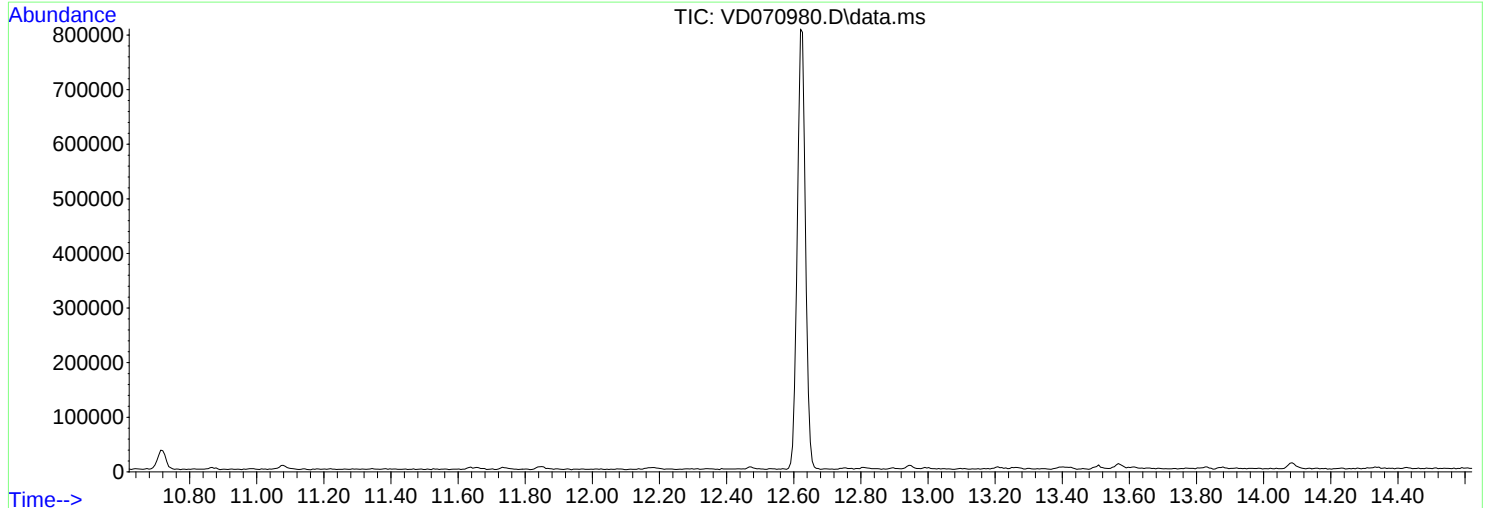

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	32301	PASS
75	95	30	60	53.9	78112	PASS
95	95	100	100	100.0	145040	PASS
96	95	5	9	6.5	9499	PASS
173	174	0.00	2	1.3	1386	PASS
174	95	50	100	72.7	105456	PASS
175	174	5	9	8.4	8890	PASS
176	174	95	101	96.6	101875	PASS
177	176	5	9	7.0	7131	PASS