
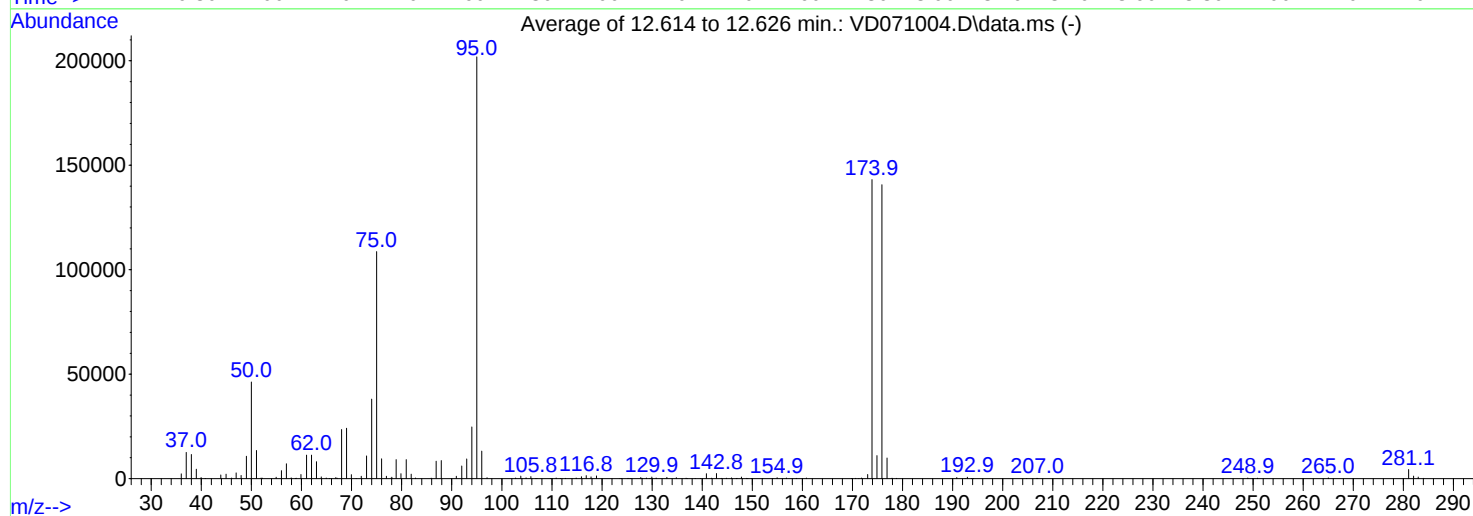


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111121\
Data File : VD071004.D
Acq On : 11 Nov 2021 23:59
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
Title : SW846 8260
Last Update : Wed Nov 10 03:55:51 2021

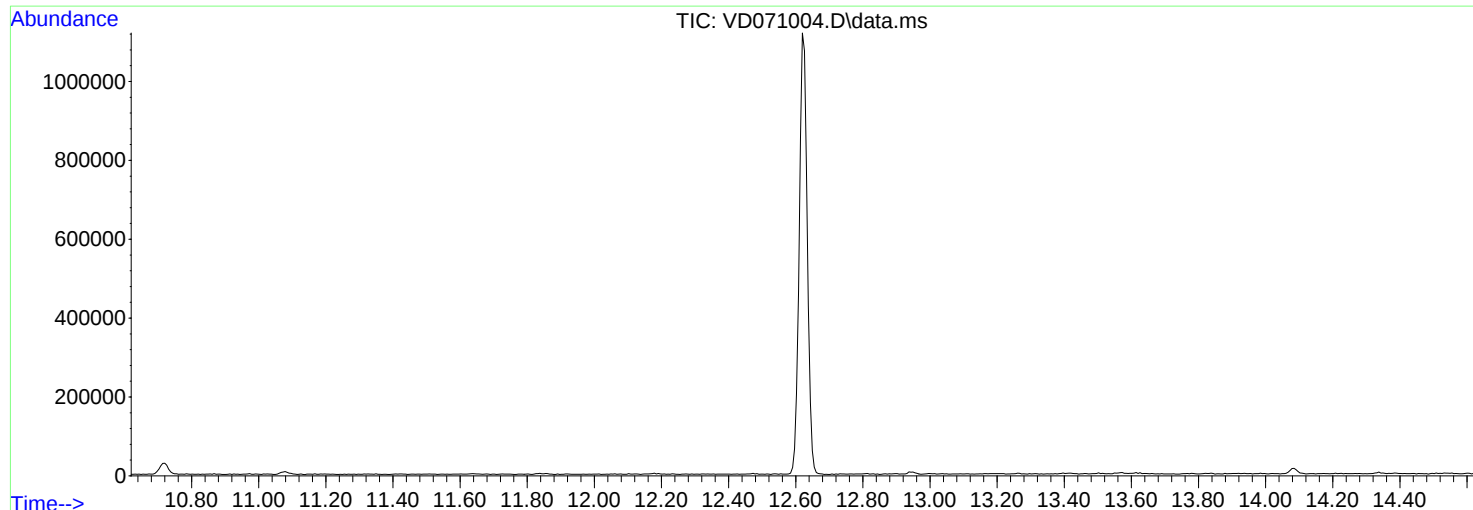

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	46224	PASS
75	95	30	60	53.8	108688	PASS
95	95	100	100	100.0	201877	PASS
96	95	5	9	6.5	13177	PASS
173	174	0.00	2	1.4	1984	PASS
174	95	50	100	70.9	143163	PASS
175	174	5	9	7.7	11010	PASS
176	174	95	101	98.3	140669	PASS
177	176	5	9	7.0	9901	PASS