

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD111218\
 Data File : VD060337.D
 Acq On : 12 Nov 2018 15:05
 Operator : JC/SY
 Sample : J5889-07
 Misc : 9.08g/5ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DUP

Quant Time: Nov 13 01:25:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 06 13:56:04 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.39	168	944779	50.00	ug/l	-0.04
34) 1,4-Difluorobenzene	7.42	114	1409173	50.00	ug/l	-0.04
63) Chlorobenzene-d5	11.27	117	1325589	50.00	ug/l	-0.03
72) 1,4-Dichlorobenzene-d4	13.37	152	769826	50.00	ug/l	-0.02
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.76	65	365456	54.02	ug/l	-0.04
Spiked Amount 50.000			Recovery	=	108.04%	
35) Dibromofluoromethane	6.30	113	430215	40.94	ug/l	-0.04
Spiked Amount 50.000			Recovery	=	81.88%	
50) Toluene-d8	9.43	98	1166622	37.93	ug/l	-0.04
Spiked Amount 50.000			Recovery	=	75.86%	
62) 4-Bromofluorobenzene	12.41	95	546534	49.04	ug/l	-0.03
Spiked Amount 50.000			Recovery	=	98.08%	
Target Compounds						
					Qvalue	
16) Acetone	3.14	43	58776	50.089	ug/l	97
20) Methylene Chloride	3.69	84	100814	9.685	ug/l	98
31) Cyclohexane	6.34	56	70882	4.389	ug/l #	82
39) Methylcyclohexane	8.01	83	26328	1.644	ug/l #	87
52) Toluene	9.53	92	344887	15.193	ug/l	96
67) Ethyl Benzene	11.42	91	267422	5.443	ug/l	96
68) m/p-Xylenes	11.55	106	357603	19.731	ug/l	90
69) o-Xylene	11.92	106	174439	9.962	ug/l	96
78) n-propylbenzene	12.63	91	138827	1.983	ug/l	99
80) 1,3,5-Trimethylbenzene	12.79	105	188630	4.328	ug/l	97
84) 1,2,4-Trimethylbenzene	13.08	105	458538	10.533	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD111218\
Data File : VD060337.D
Acq On : 12 Nov 2018 15:05
Operator : JC/SY
Sample : J5889-07
Misc : 9.08g/5ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DUP

Quant Time: Nov 13 01:25:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 06 13:56:04 2018
Response via : Initial Calibration

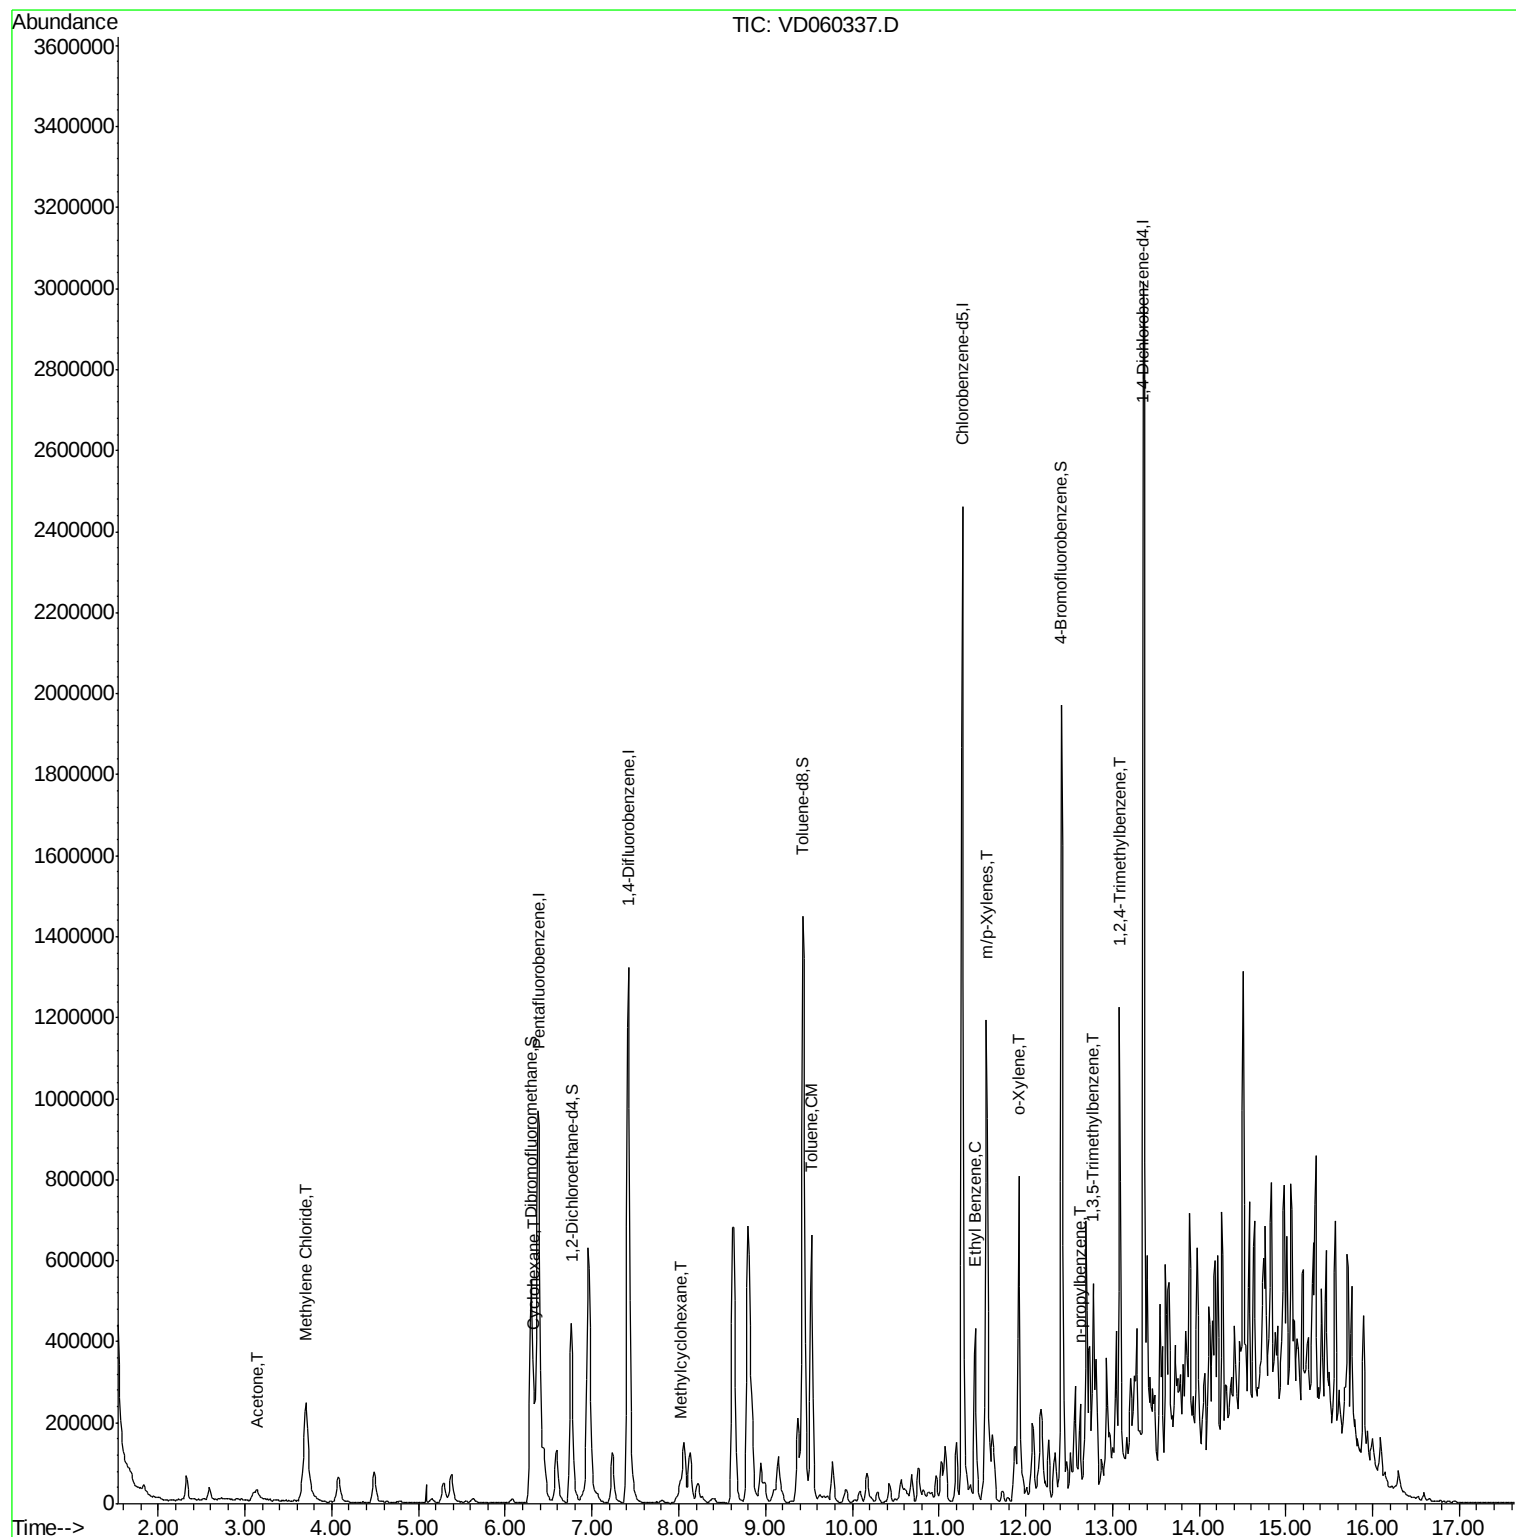

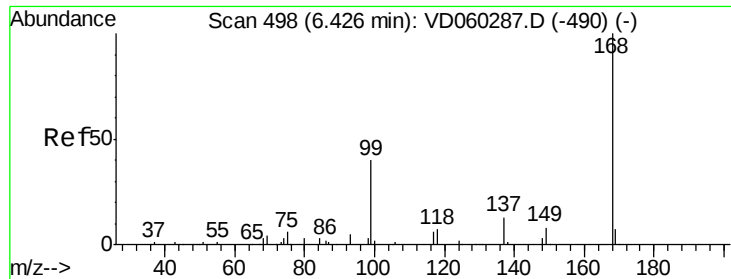

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 6.39 min Scan# 494

Delta R.T. -0.04 min

Lab File: VD060337.D

Acq: 12 Nov 2018 15:05

Instrument :

MSVOA_D

ClientSampleId :


DUP

Tot Ion:168 Resp: 944779

Ion Ratio Lower Upper

168 100

99 47.8 39.8 59.8

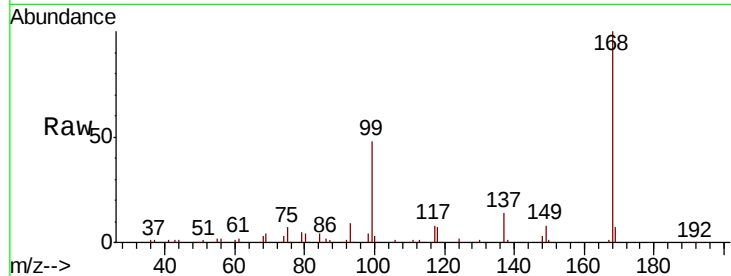

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

6.39

400000

300000

200000

100000



0

Time-->

6.20

6.40

6.60



#16

Acetone

Concen: 50.089 ug/l

RT: 3.14 min Scan# 164

Delta R.T. -0.03 min

Lab File: VD060337.D


Acq: 12 Nov 2018 15:05

Tgt Ion: 43 Resp: 58776

Ion Ratio Lower Upper

43 100

58 22.6 16.9 25.3



Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

15000

10000

5000


0


Time-->

3.00

3.10

3.20







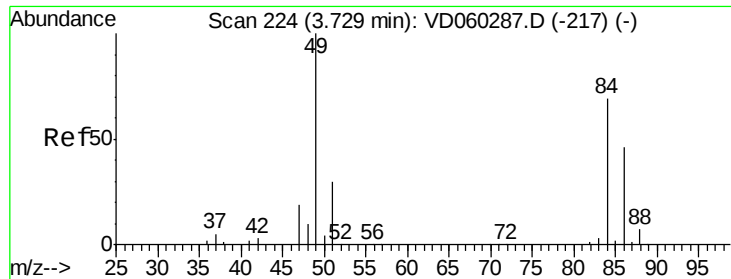

#20
Methylene Chloride
Concen: 9.685 ug/l
RT: 3.69 min Scan# 220
Delta R.T. -0.04 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05




Instrument :
MSVOA_D
ClientSampleId :
DUP


Tot Ion: 84 Resp: 100814
Ion Ratio Lower Upper
84 100
49 141.2 115.6 173.4
51 44.7 35.6 53.4
86 62.7 52.3 78.5

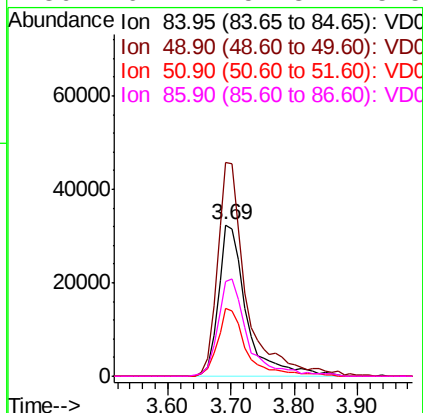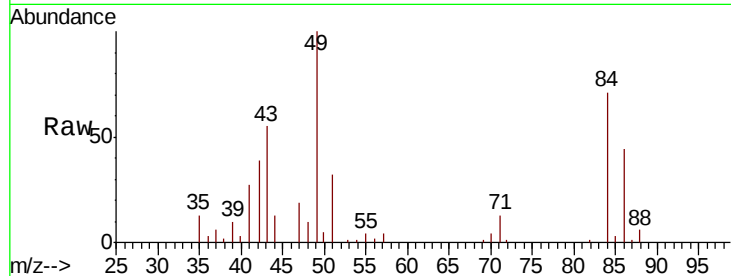

#31
Cyclohexane
Concen: 4.389 ug/l
RT: 6.34 min Scan# 489
Delta R.T. -0.05 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05

Tgt Ion: 56 Resp: 70882
Ion Ratio Lower Upper
56 100
69 24.7 22.2 33.2
84 59.2 63.0 94.4#

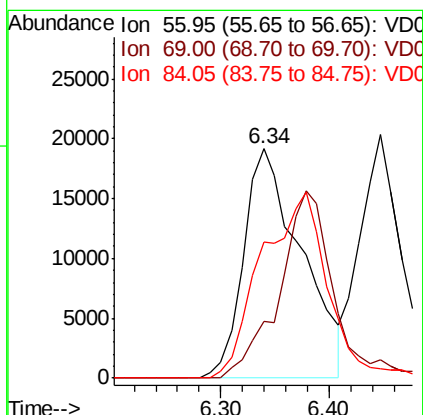

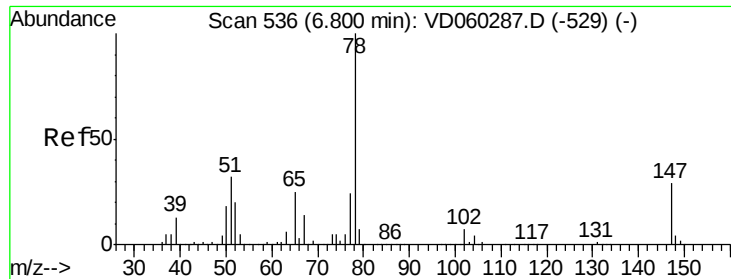

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 6.76 min Scan# 532

Delta R.T. -0.04 min

Lab File: VD060337.D

Acq: 12 Nov 2018 15:05

Instrument :

MSVOA_D

ClientSampleId :


DUP

Tot Ion: 65 Resp: 365456

Ion Ratio Lower Upper




65 100

67 52.7 0.0 109.8

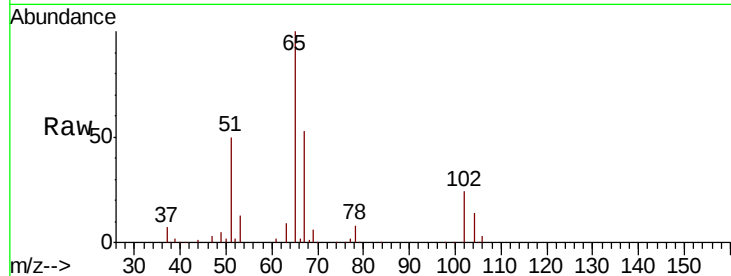

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

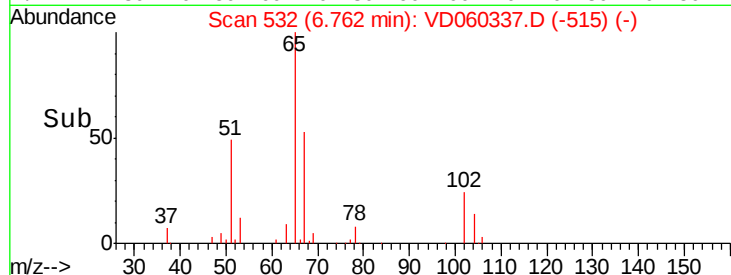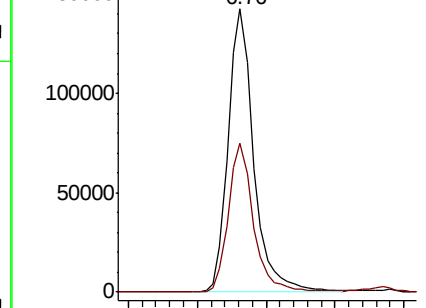

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 7.42 min Scan# 599

Delta R.T. -0.04 min

Lab File: VD060337.D

Acq: 12 Nov 2018 15:05


Tgt Ion: 114 Resp: 1409173

Ion Ratio Lower Upper

114 100

63 18.8 0.0 34.0



88 17.9 0.0 35.4




Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): VDC

Ion 87.90 (87.60 to 88.60): VDC

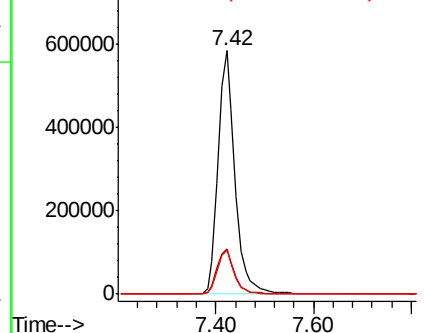

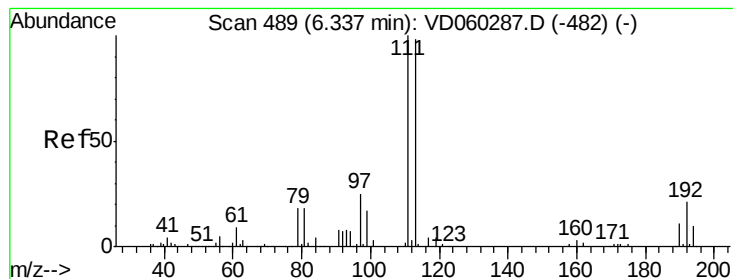

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 6.30 min Scan# 485

Delta R.T. -0.04 min

Lab File: VD060337.D

Acq: 12 Nov 2018 15:05

Instrument :

MSVOA_D

ClientSampleId :

DUP


Tot Ion:113 Resp: 430215

Ion Ratio Lower Upper

113 100

111 104.9 81.6 122.4




192 20.8 16.5 24.7

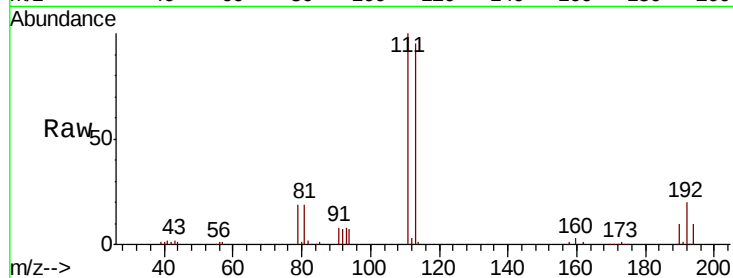

Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

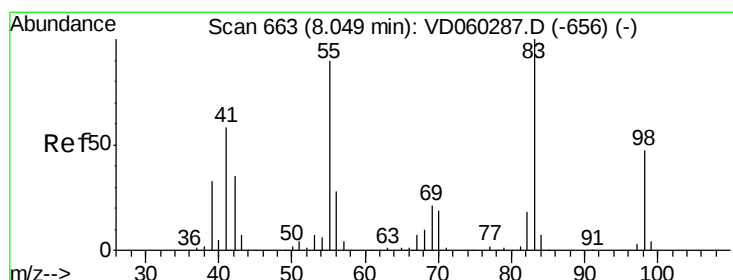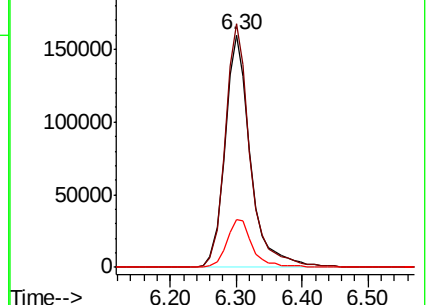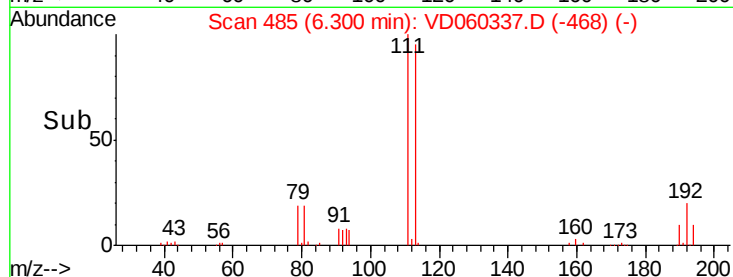

#39

Methylcyclohexane

Concen: 1.644 ug/l

RT: 8.01 min Scan# 659

Delta R.T. -0.04 min

Lab File: VD060337.D

Acq: 12 Nov 2018 15:05


Tgt Ion: 83 Resp: 26328

Ion Ratio Lower Upper

83 100

55 78.7 71.2 106.8



98 36.3 38.4 57.6#

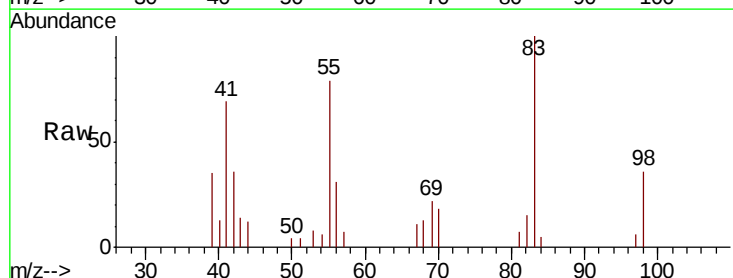


Abundance Ion 83.05 (82.75 to 83.75): V

Ion 55.00 (54.70 to 55.70): V

Ion 98.05 (97.75 to 98.75): V

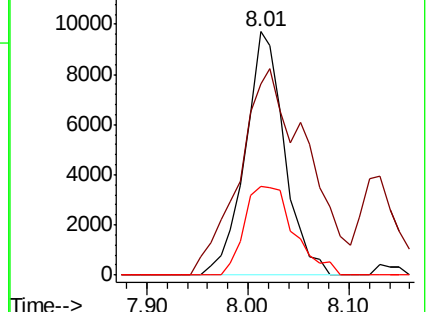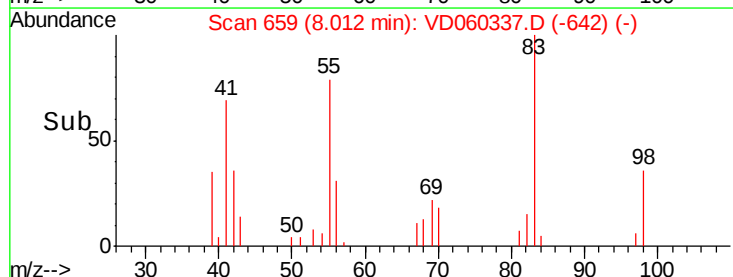

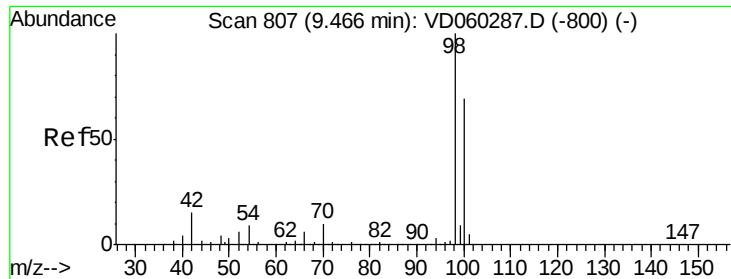

#50

Toluene-d8

Concen: N.D. ug/l

RT: 9.43 min Scan# 803

Delta R.T. -0.04 min

Lab File: VD060337.D

Acq: 12 Nov 2018 15:05

Instrument :

MSVOA_D

ClientSampleId :





DUP

Tot Ion: 98 Resp: 1166622

Ion Ratio Lower Upper

98 100

100 69.9 55.2 82.8

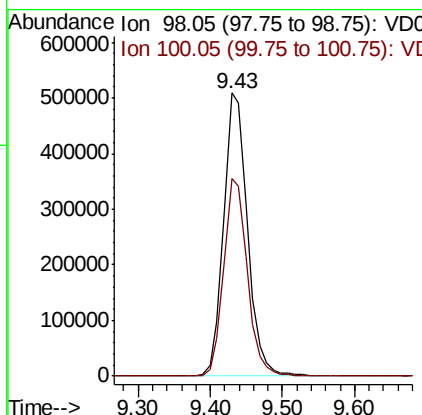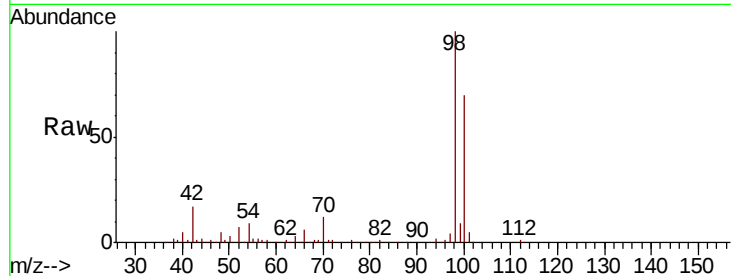

#52

Toluene

Concen: 15.193 ug/l

RT: 9.53 min Scan# 813

Delta R.T. -0.04 min

Lab File: VD060337.D




Acq: 12 Nov 2018 15:05


Tgt Ion: 92 Resp: 344887

Ion Ratio Lower Upper

92 100

91 170.4 131.9 197.9


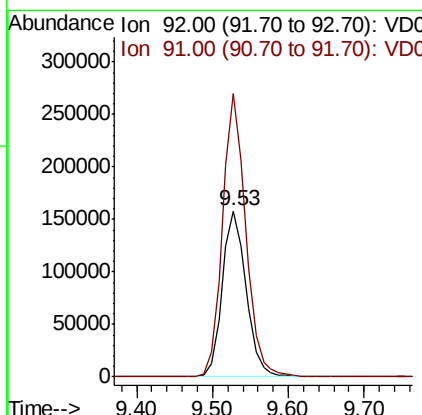




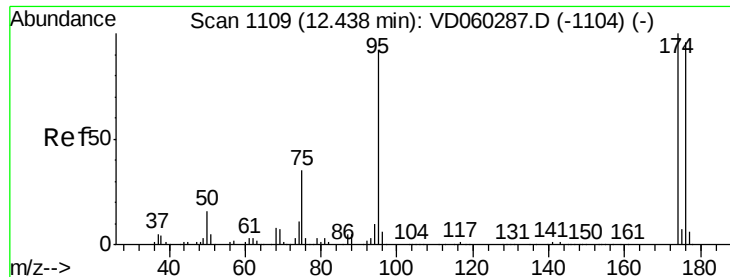

#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.41 min Scan# 1106
Delta R.T. -0.03 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05




Instrument :
MSVOA_D
ClientSampled :
DUP


Tot Ion: 95 Resp: 546534
Ion Ratio Lower Upper
95 100
174 84.8 0.0 160.8
176 78.6 0.0 154.6

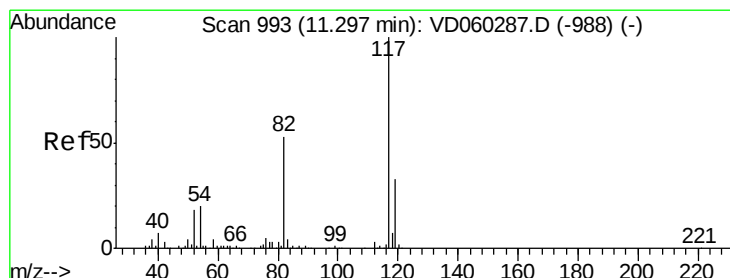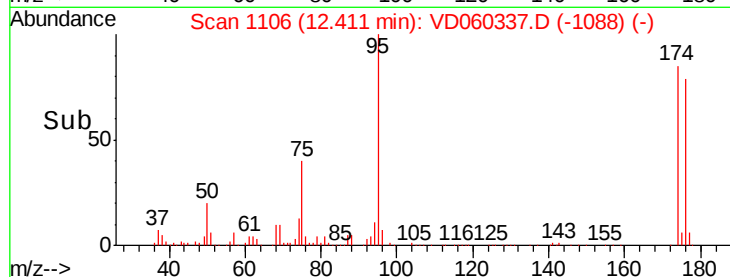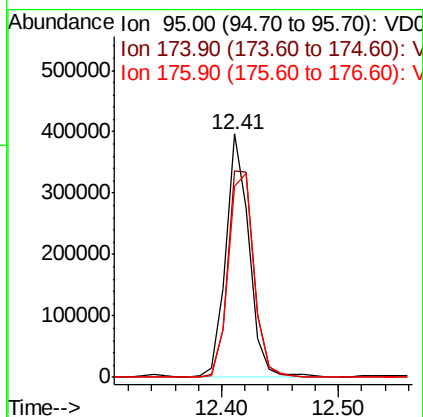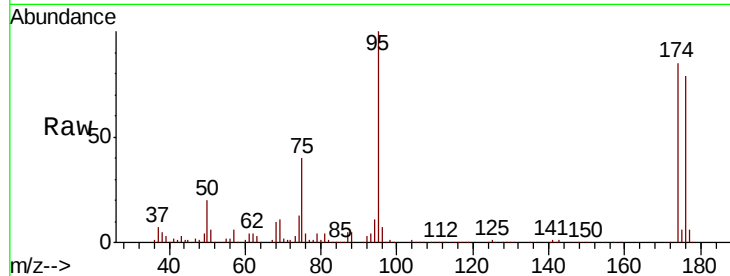

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.27 min Scan# 990
Delta R.T. -0.03 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05

Tgt Ion: 117 Resp: 1325589
Ion Ratio Lower Upper
117 100
82 53.0 43.7 65.5
119 33.1 26.1 39.1


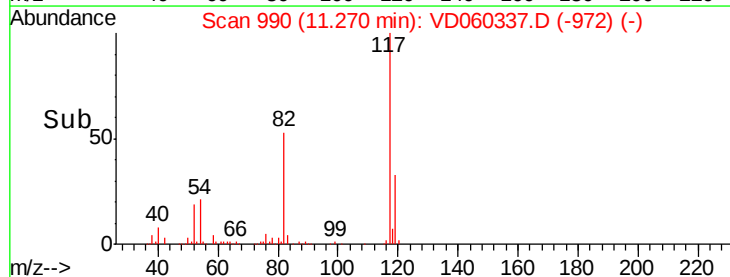
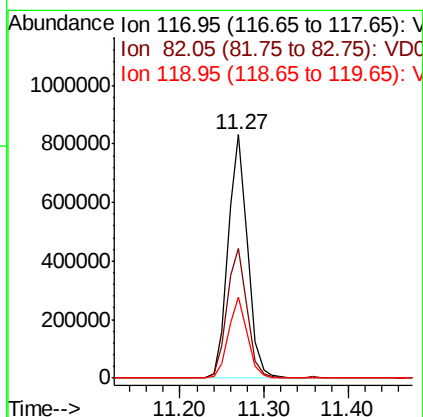
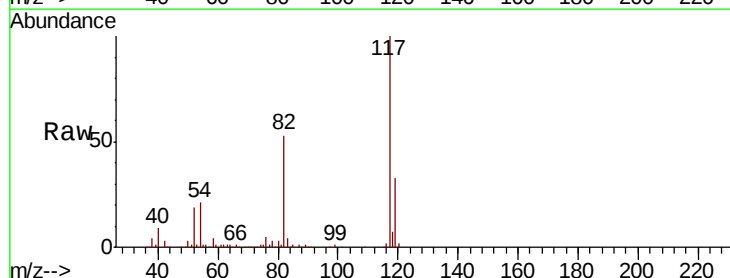


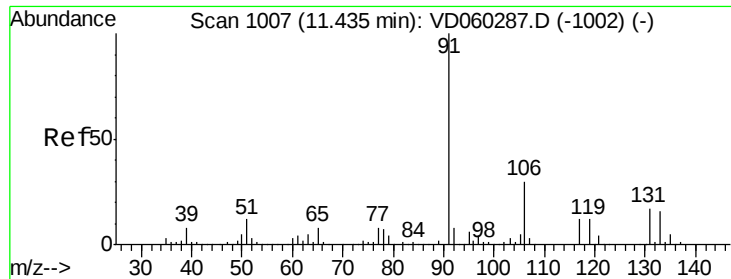

#67
Ethyl Benzene
Concen: 5.443 ug/l
RT: 11.42 min Scan# 1005
Delta R.T. -0.02 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05




Instrument :
MSVOA_D
ClientSampled :
DUP


Tot Ion: 91 Resp: 267422
Ion Ratio Lower Upper
91 100
106 28.4 24.6 36.8

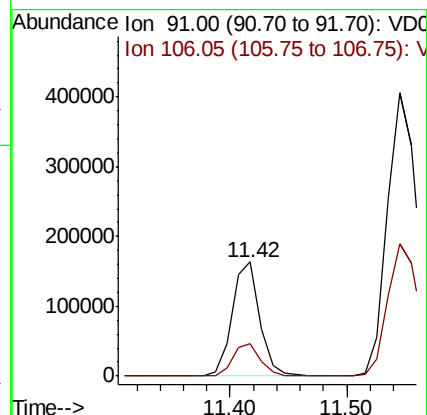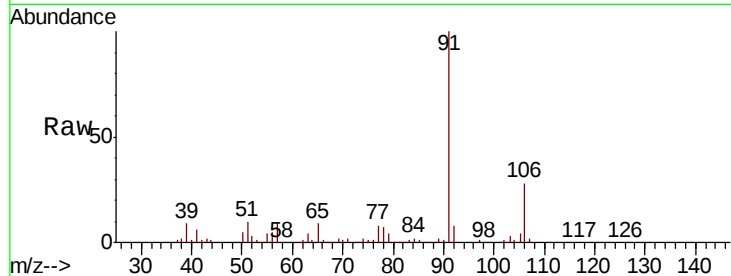

#68
m/p-Xylenes
Concen: 19.731 ug/l
RT: 11.55 min Scan# 1018
Delta R.T. -0.03 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05

Tgt Ion: 106 Resp: 357603
Ion Ratio Lower Upper
106 100
91 214.7 159.4 239.2



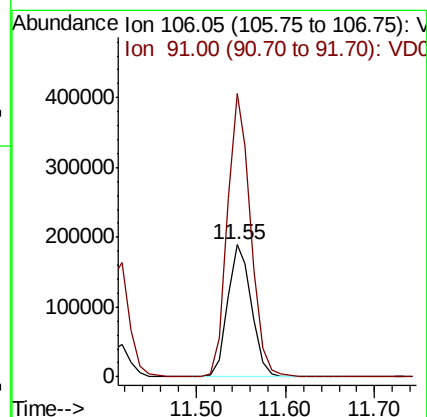



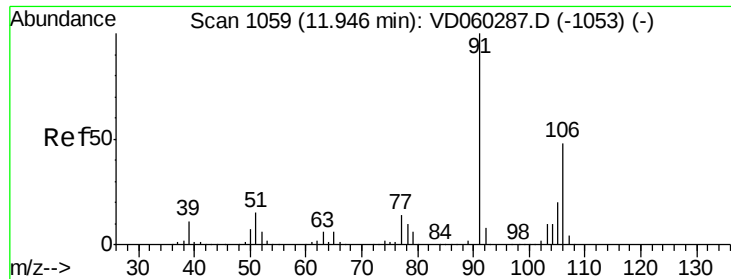

#69
o-Xylene
Concen: 9.962 ug/l
RT: 11.92 min Scan# 1056
Delta R.T. -0.03 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05




Instrument :
MSVOA_D
ClientSampled :
DUP


Tot Ion:106 Resp: 174439
Ion Ratio Lower Upper
106 100
91 224.2 109.2 327.6

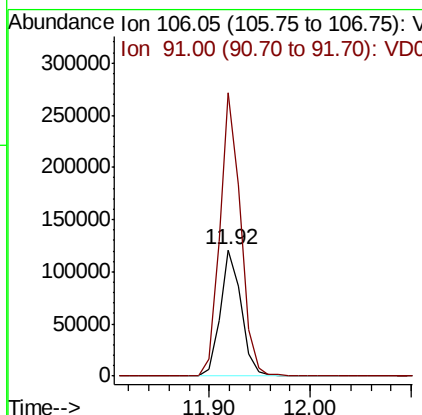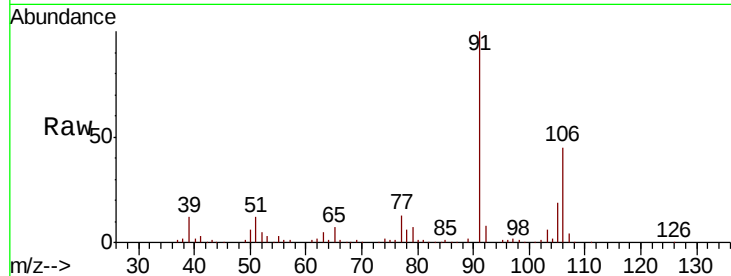

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.37 min Scan# 1203
Delta R.T. -0.02 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05

Tgt Ion:152 Resp: 769826
Ion Ratio Lower Upper
152 100
115 45.7 24.1 72.3
150 155.9 0.0 310.6


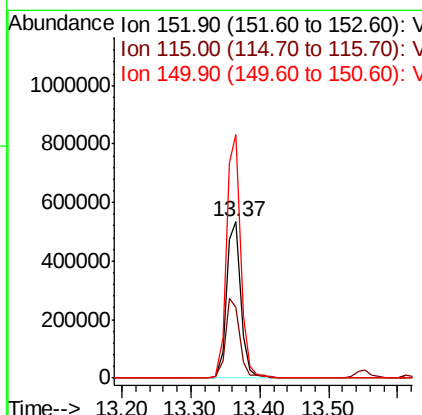




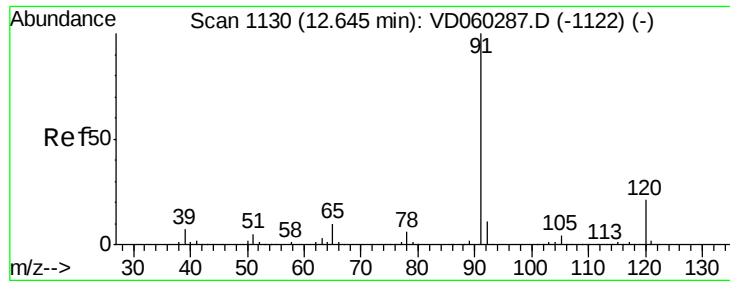

#78
n-propylbenzene
Concen: 1.983 ug/l
RT: 12.63 min Scan# 1128
Delta R.T. -0.02 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05




Instrument :
MSVOA_D
ClientSampled :
DUP


Tot Ion: 91 Resp: 138827
Ion Ratio Lower Upper
91 100
120 20.2 10.4 31.4

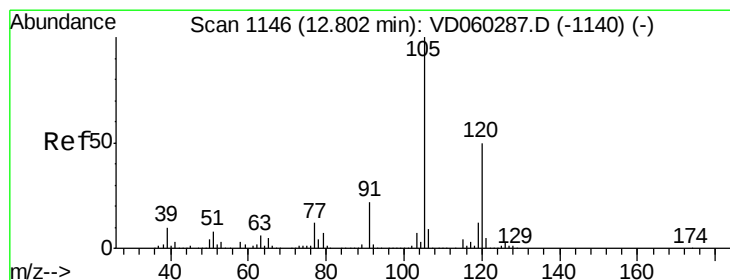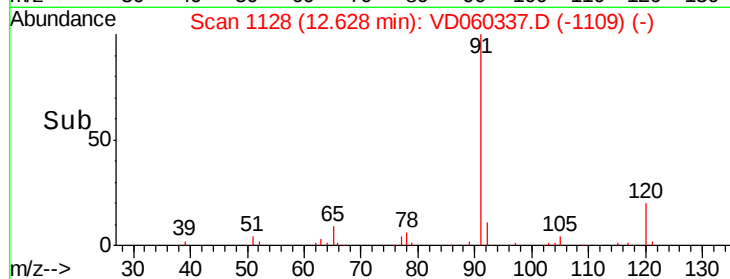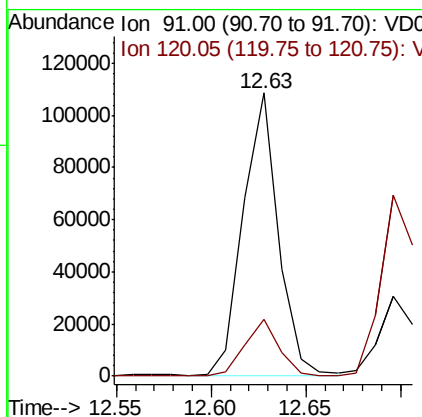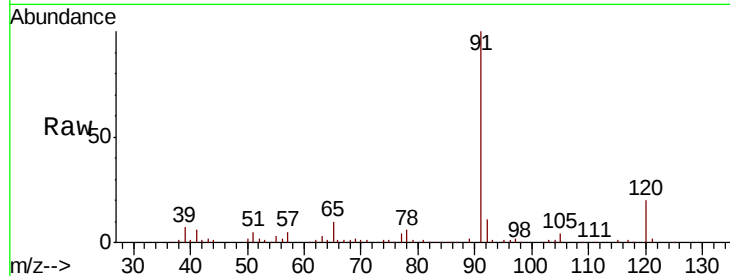

#80
1,3,5-Trimethylbenzene
Concen: 4.328 ug/l
RT: 12.79 min Scan# 1144
Delta R.T. -0.02 min
Lab File: VD060337.D
Acq: 12 Nov 2018 15:05

Tgt Ion:105 Resp: 188630
Ion Ratio Lower Upper
105 100
120 50.8 24.4 73.4

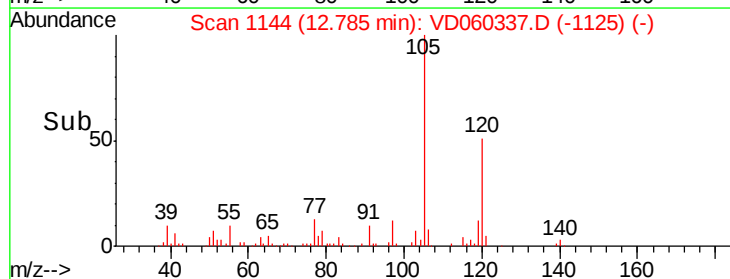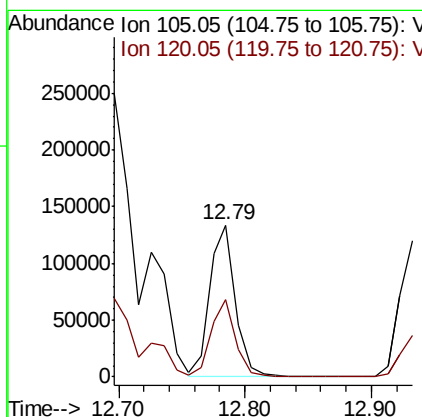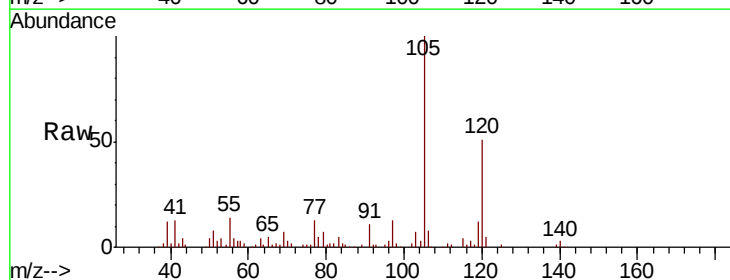

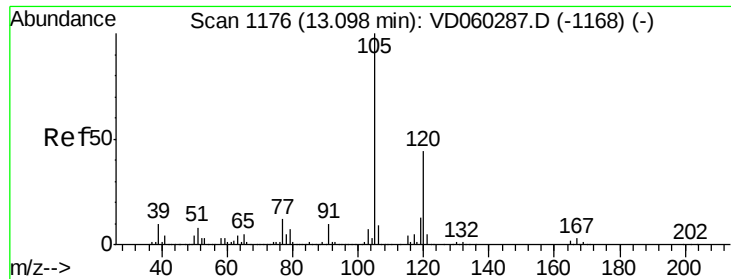

#84
 1,2,4-Trimethylbenzene
 Concen: 10.533 ug/l
 RT: 13.08 min Scan# 1174
 Delta R.T. -0.02 min
 Lab File: VD060337.D
 Acq: 12 Nov 2018 15:05

Instrument :
 MSVOA_D
 ClientSampleId :
 DUP

Tot Ion:105 Resp: 458538
 Ion Ratio Lower Upper
 105 100
 120 43.7 21.9 65.8

