


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111218\
Data File : VD060328.D
Acq On : 12 Nov 2018 9:31
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Title : SW846 8260
Last Update : Tue Nov 06 13:56:04 2018

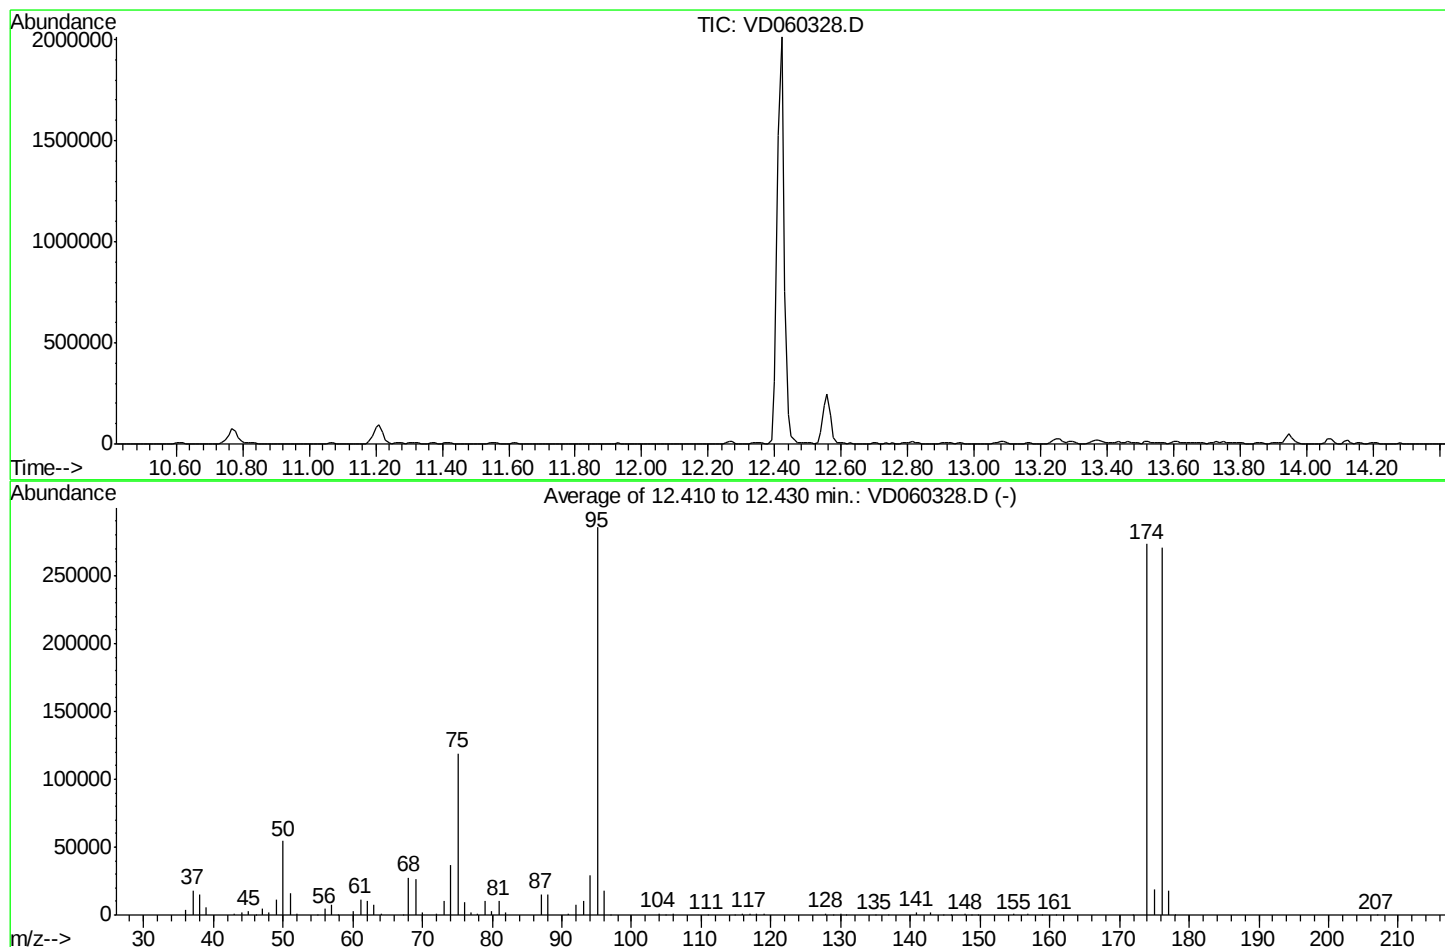

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	54328	PASS
75	95	30	60	41.7	119002	PASS
95	95	100	100	100.0	285554	PASS
96	95	5	9	6.3	17932	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	95.6	273066	PASS
175	174	5	9	7.0	19085	PASS
176	174	95	101	99.2	270848	PASS
177	176	5	9	6.7	18037	PASS