




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
 Data File : VD077540.D
 Acq On : 13 Nov 2023 11:16
 Operator : JC/SY
 Sample : 05296-03
 Misc : 5.59G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH3R3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:41:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 10 02:07:44 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

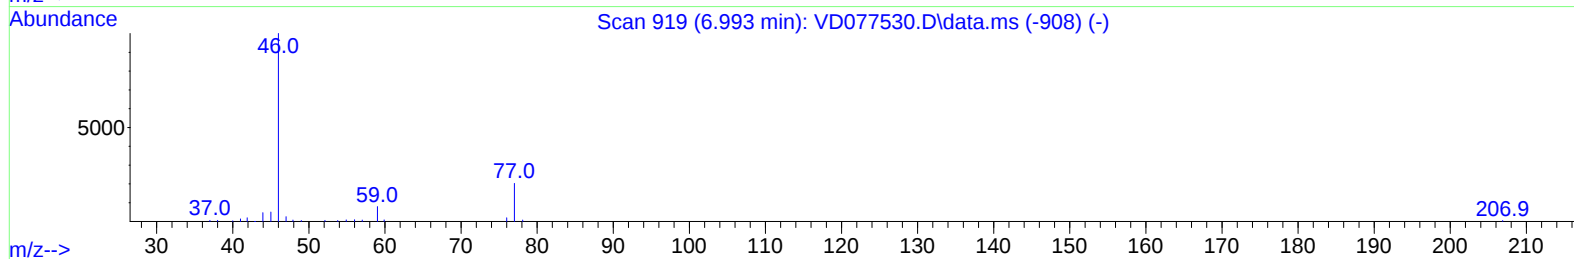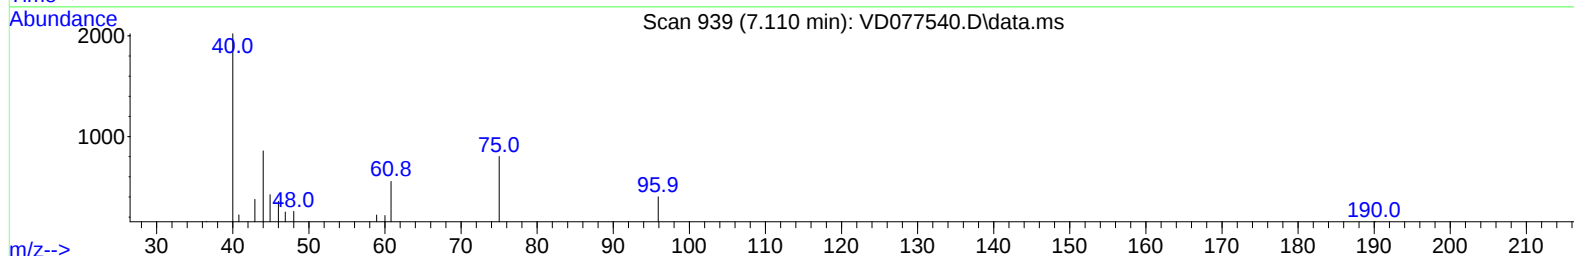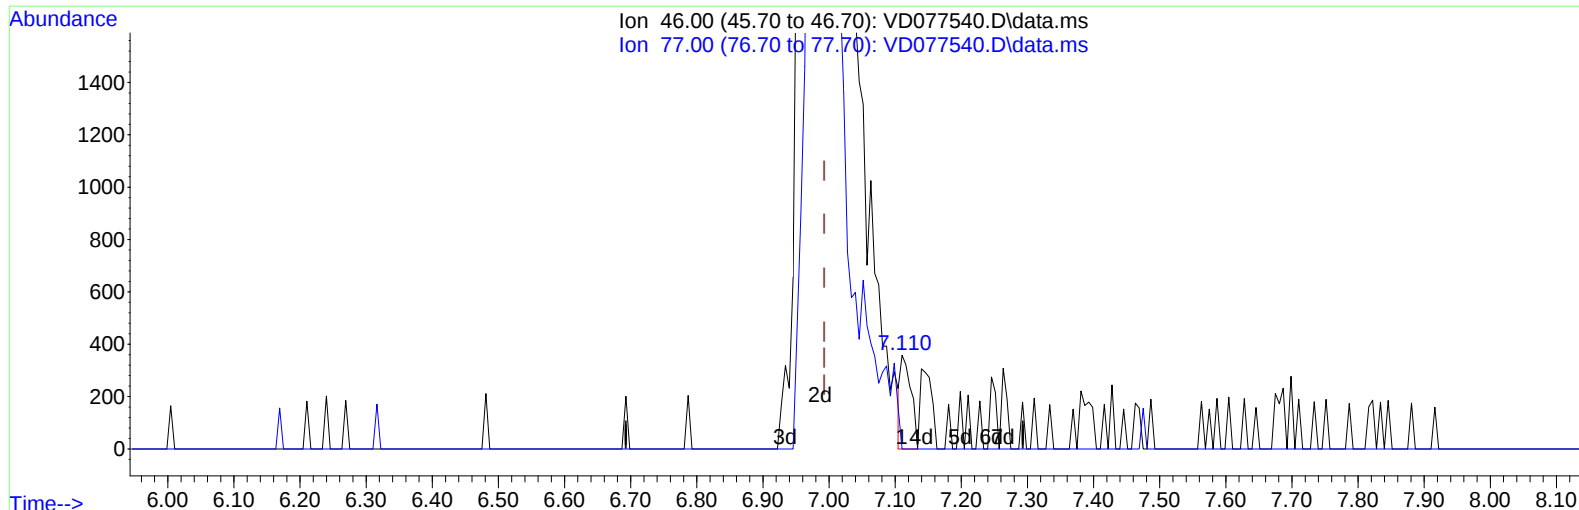

TIC: VD077540.D\data.ms

(21) 2-Butanone-d5 (S)

7.110min (+ 0.117) 0.17 ug/L

response	391	
Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.40	18.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
Data File : VD077540.D
Acq On : 13 Nov 2023 11:16
Operator : JC/SY
Sample : 05296-03
Misc : 5.59G/10ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH3R3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

Quant Time: Nov 16 00:41:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 10 02:07:44 2023
Response via : Initial Calibration

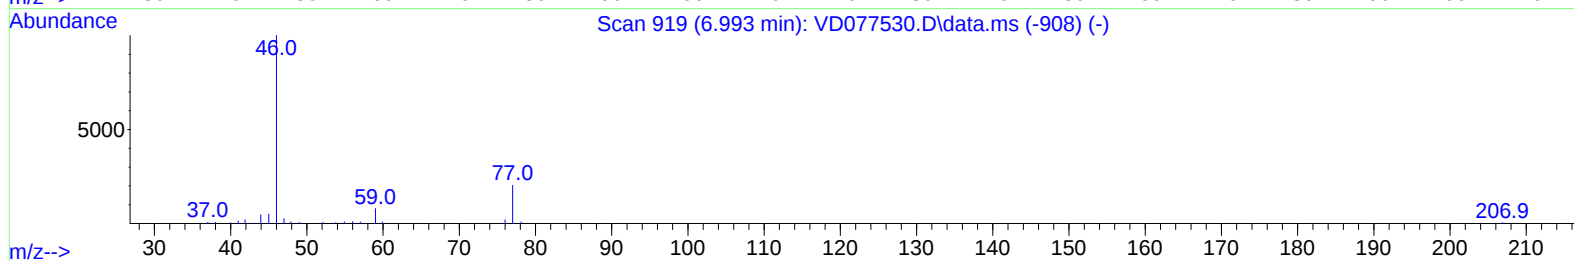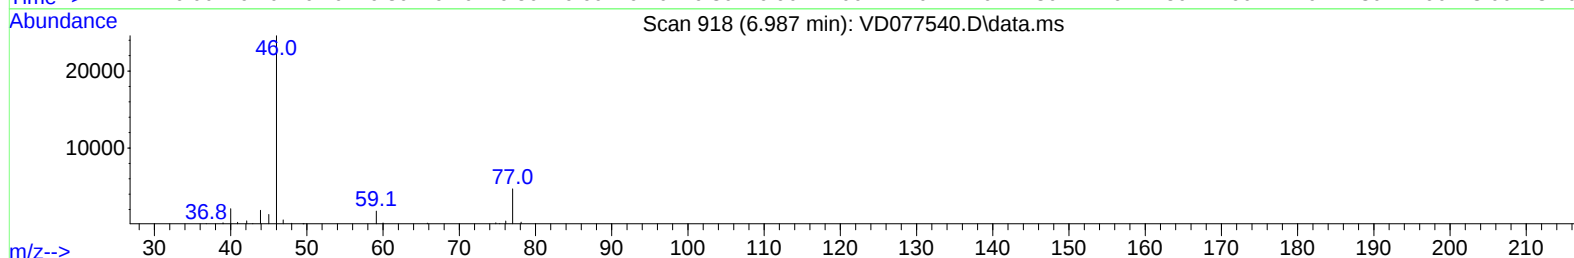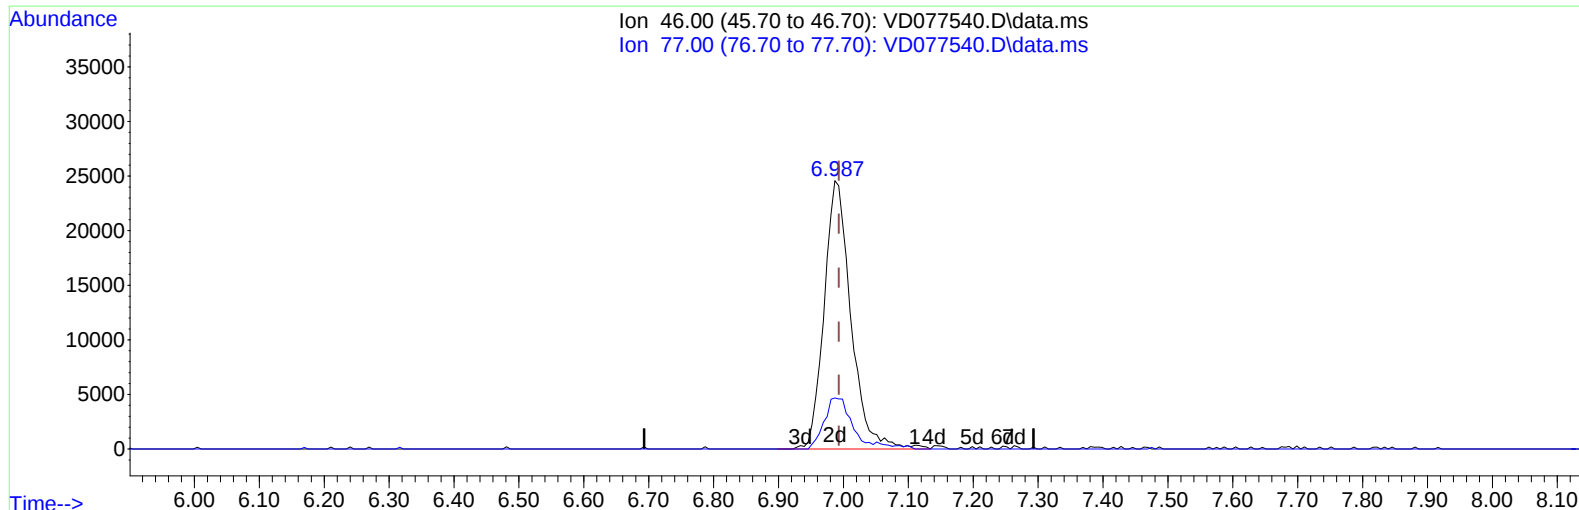

TIC: VD077540.D\data.ms

(21) 2-Butanone-d5 (S)

6.987min (-0.006) 30.32 ug/L m

response 70569

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.40	0.10#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
 Data File : VD077540.D
 Acq On : 13 Nov 2023 11:16
 Operator : JC/SY
 Sample : 05296-03
 Misc : 5.59G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH3R3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:41:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 10 02:07:44 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

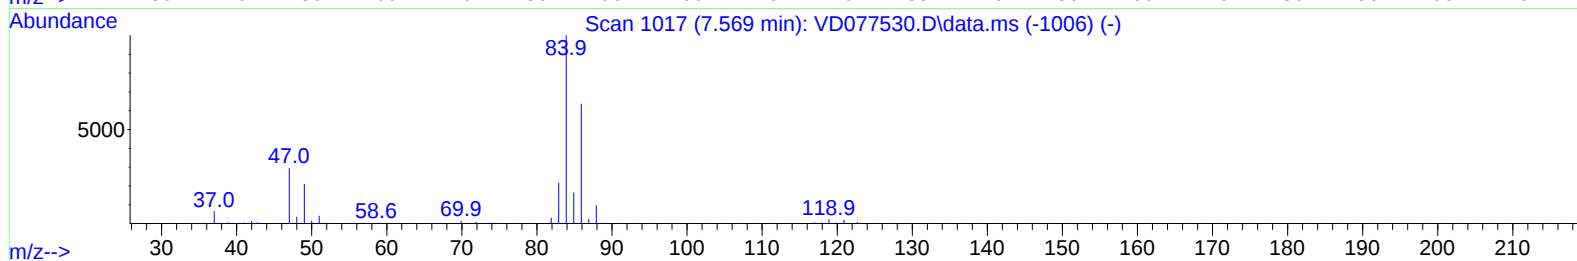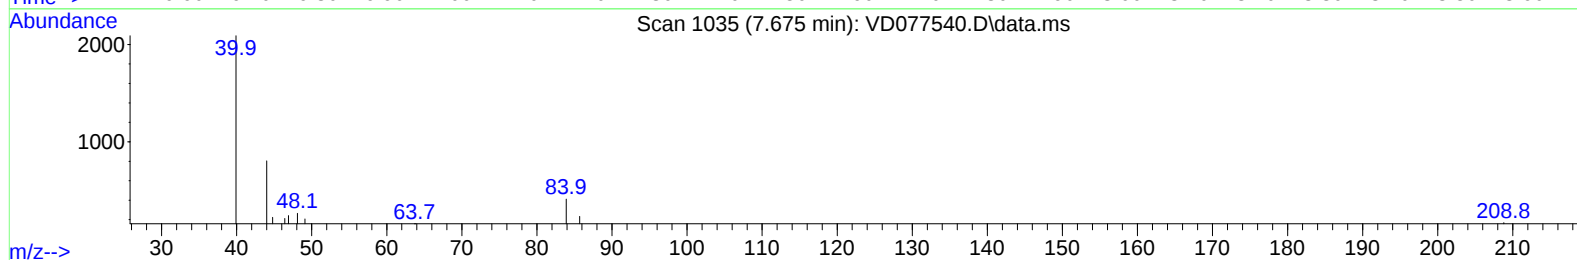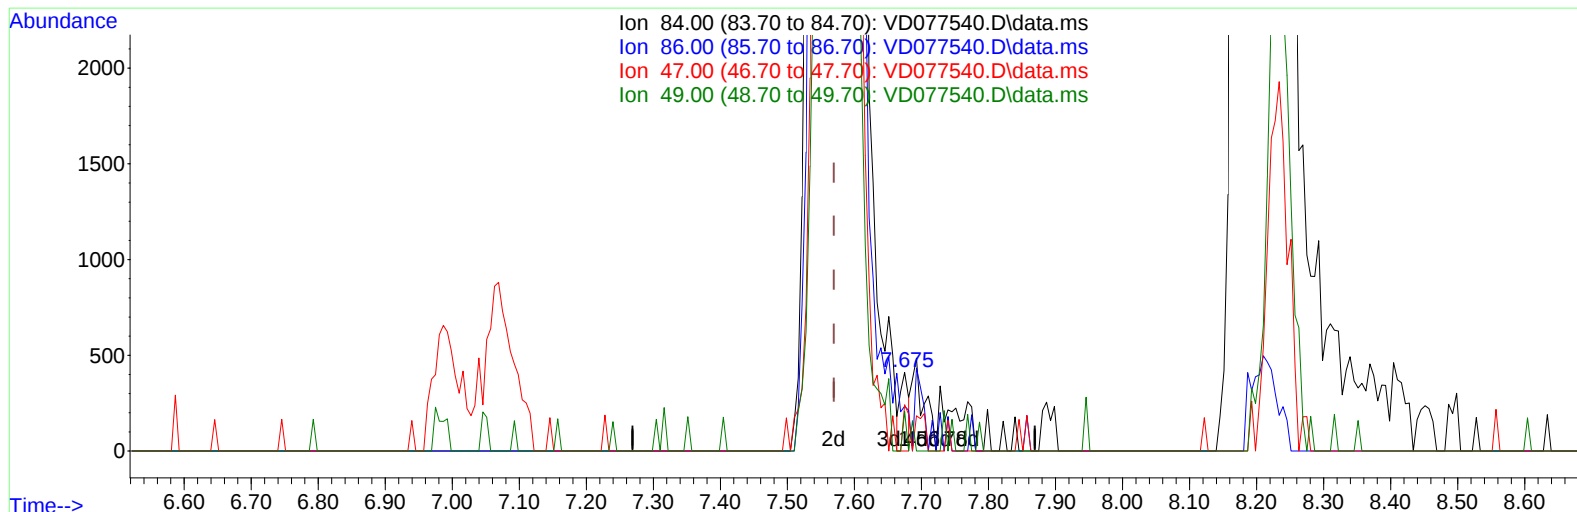

TIC: VD077540.D\data.ms

(24) Chloroform-d (S)

7.675min (+ 0.106) 0.02 ug/L

response	353	
Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	44.76
47.00	50.40	43.34
49.00	28.50	20.68


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
 Data File : VD077540.D
 Acq On : 13 Nov 2023 11:16
 Operator : JC/SY
 Sample : 05296-03
 Misc : 5.59G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH3R3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:41:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 10 02:07:44 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

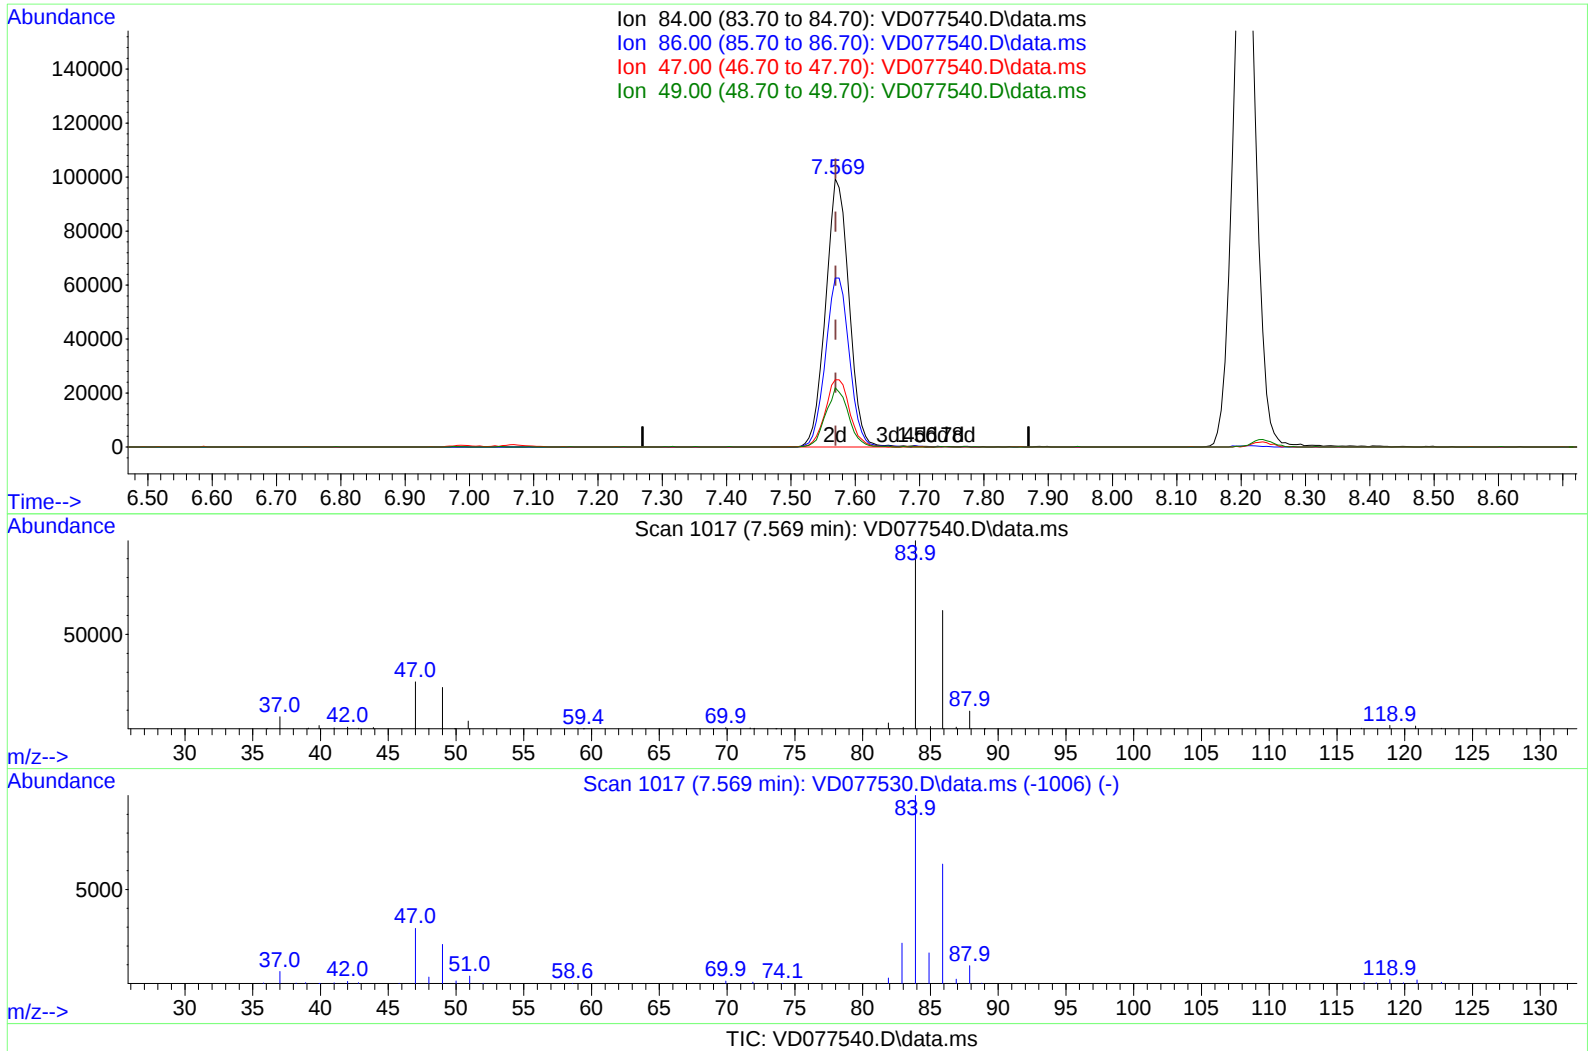

(24) Chloroform-d (S)

7.569min (-0.000) 16.49 ug/L m

response 251762

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	0.06#
47.00	50.40	0.06#
49.00	28.50	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
 Data File : VD077540.D
 Acq On : 13 Nov 2023 11:16
 Operator : JC/SY
 Sample : 05296-03
 Misc : 5.59G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH3R3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:41:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 10 02:07:44 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/17/2023
 Supervised By :Semsettin Yesilyurt 11/17/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	528377	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.586	117	446553	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	178411	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.287	65	204791	15.236	ug/L	0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	60.960%	
7) Chloroethane-d5	2.816	69	170734	16.169	ug/L	0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	64.680%	
11) 1,1-Dichloroethene-d2	3.928	65	66019	15.884	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	63.520%	
21) 2-Butanone-d5	6.987	46	70569m	30.325	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	60.640%	
24) Chloroform-d	7.569	84	251762m	16.494	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	65.960%	
26) 1,2-Dichloroethane-d4	8.234	65	137227	16.902	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	67.600%#	
32) Benzene-d6	8.204	84	537772	18.555	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	74.200%	
36) 1,2-Dichloropropane-d6	9.210	67	175582	18.599	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	74.400%	
41) Toluene-d8	10.269	98	465413	17.771	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	71.080%	
43) trans-1,3-Dichloroprop...	10.528	79	70834	17.402	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	69.600%	
47) 2-Hexanone-d5	10.881	63	52825	31.279	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	62.560%	
56) 1,1,2,2-Tetrachloroeth...	12.657	84	97131	15.529	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	62.120%	
66) 1,2-Dichlorobenzene-d4	13.816	152	110430	17.399	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	69.600%#	
Target Compounds						
					Qvalue	
13) Acetone	4.022	43	7634	3.121	ug/L	67
16) Methylene chloride	4.810	84	19811	2.221	ug/L	95
25) Chloroform	7.604	83	6083	0.418	ug/L	97
34) Trichloroethene	9.034	95	3125	0.407	ug/L	87
46) Tetrachloroethene	10.816	164	88070	15.599	ug/L	98
53) m,p-Xylene	11.792	106	6719	0.516	ug/L	99
54) o-Xylene	12.122	106	3813	0.306	ug/L	92
70) 1,2,4-trichlorobenzene	15.098	180	8197	1.206	ug/L #	94
72) 1,2,3-Trichlorobenzene	15.527	180	9353	1.615	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
Data File : VD077540.D
Acq On : 13 Nov 2023 11:16
Operator : JC/SY
Sample : 05296-03
Misc : 5.59G/10ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH3R3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

Quant Time: Nov 16 00:41:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 10 02:07:44 2023
Response via : Initial Calibration

