
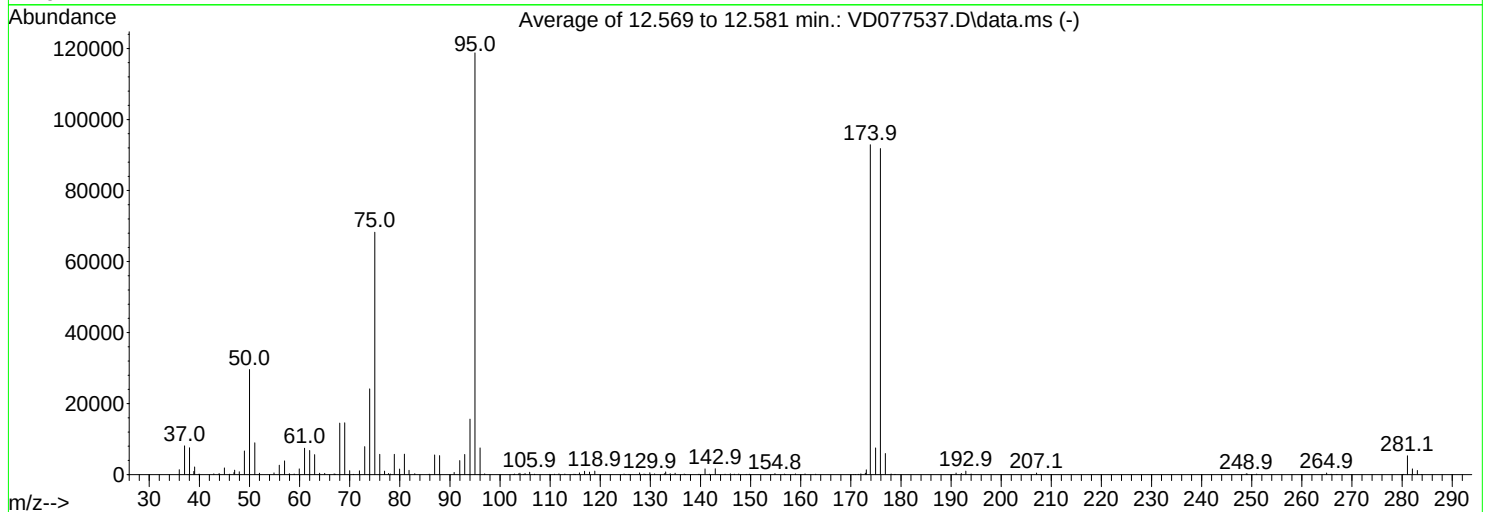


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111323\
Data File : VD077537.D
Acq On : 13 Nov 2023 08:17
Operator : JC/SY
Sample : BFB176
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB176

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Title : SFAM01.0
Last Update : Fri Nov 10 02:07:44 2023

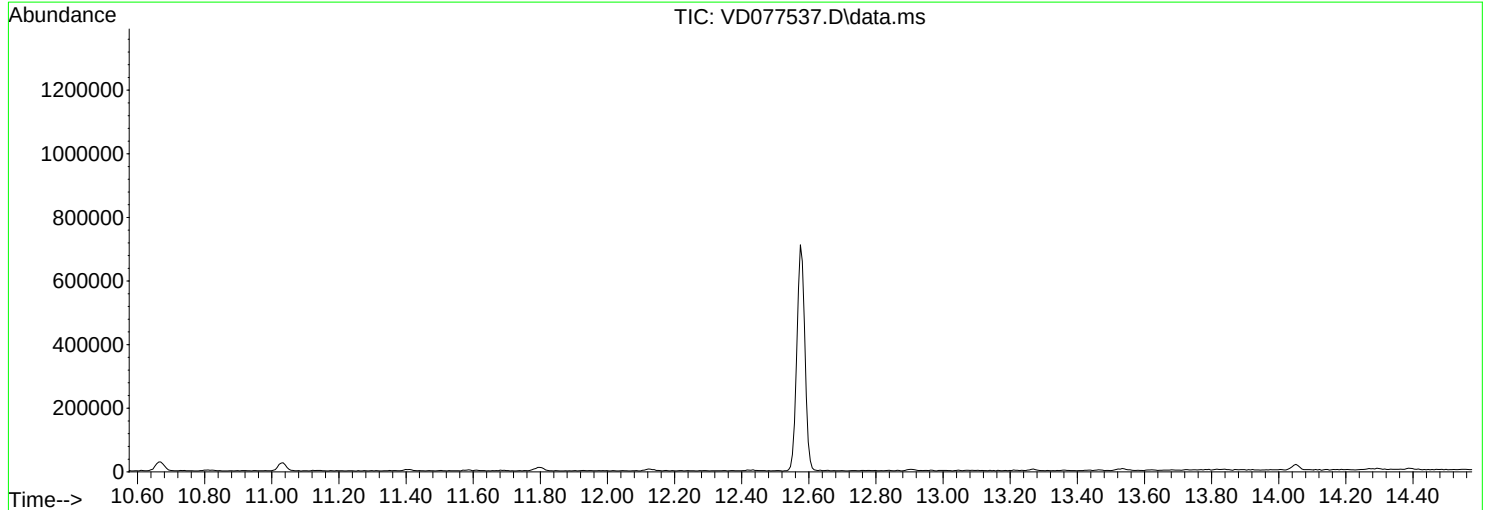

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	29627	PASS
75	95	30	80	57.5	68267	PASS
95	95	100	100	100.0	118779	PASS
96	95	5	9	6.4	7543	PASS
173	174	0.00	2	1.5	1365	PASS
174	95	50	120	78.2	92931	PASS
175	174	5	9	8.1	7511	PASS
176	174	95	105	98.8	91845	PASS
177	176	5	10	6.5	5929	PASS

m/z	Abundance
40.00	2124.0
41.20	231.0
43.90	1106.0
53.30	158.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176

m/z	Abundance
36.00	1572.0
37.00	7480.0
38.10	6544.0
38.90	2669.0
40.00	2292.0
41.00	282.0
43.00	235.0
44.00	1387.0
45.00	1757.0
46.00	273.0
46.90	1793.0
48.00	824.0
49.00	5803.0
50.00	27144.0
51.10	9206.0
52.00	321.0
54.90	505.0
56.00	2561.0
57.00	3347.0
57.90	371.0
59.90	1300.0
61.00	6441.0
62.00	6893.0
63.00	5113.0
64.10	377.0
65.00	400.0
66.90	329.0
68.00	13179.0
69.00	13784.0
70.00	1180.0
72.00	1015.0
73.00	7362.0
74.00	21520.0
75.00	60864.0
76.00	5959.0
77.00	1252.0
77.70	380.0
78.90	4854.0
79.90	1408.0
80.90	5532.0
81.90	1210.0
83.00	219.0
85.90	197.0
87.00	5118.0
87.90	5468.0
90.80	455.0
91.90	3311.0
92.90	4954.0
94.00	14235.0
95.00	105552.0
96.00	6908.0
96.90	176.0
102.70	209.0
104.00	547.0
104.90	235.0
106.00	570.0
110.80	188.0
111.90	173.0
113.00	368.0
114.80	178.0
116.00	337.0
116.80	795.0
117.90	799.0
119.10	707.0
124.70	219.0
127.80	303.0
128.70	192.0
130.00	391.0
130.90	153.0
133.10	525.0
135.00	313.0
136.70	237.0
140.90	1481.0
141.90	206.0
142.90	1801.0
145.00	153.0
146.00	178.0
146.80	167.0
147.70	170.0
154.90	326.0
156.70	285.0
161.00	177.0
163.00	212.0
170.90	213.0
172.90	1239.0
173.90	78432.0
174.90	7089.0
175.90	78192.0
176.90	5036.0
178.00	267.0
191.00	258.0
192.00	250.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176

193.00	761.0
207.00	228.0
248.90	375.0
251.00	266.0
264.90	390.0
281.10	3971.0
282.00	1110.0
283.00	895.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176

m/z	Abundance
36.00	1327.0
37.10	8853.0
38.00	8611.0
39.10	3600.0
39.90	2405.0
42.80	291.0
44.10	1664.0
45.00	1940.0
46.10	160.0
47.10	1692.0
47.90	791.0
49.00	7897.0
50.00	31696.0
51.00	8654.0
52.00	492.0
54.90	598.0
56.00	2966.0
57.00	4645.0
58.00	254.0
58.90	322.0
60.00	2141.0
61.00	8066.0
62.00	7379.0
63.00	5907.0
63.90	458.0
65.00	446.0
66.90	355.0
68.00	15327.0
69.00	16329.0
70.00	920.0
71.90	1166.0
73.00	8091.0
74.00	27456.0
75.00	75264.0
76.00	6081.0
76.90	644.0
77.80	586.0
78.90	6461.0
80.00	1448.0
80.90	6553.0
81.80	1075.0
83.00	331.0
85.80	187.0
86.90	6170.0
88.00	6155.0
90.90	736.0
91.90	4725.0
93.00	6530.0
94.00	17192.0
95.00	131840.0
96.00	8407.0
96.90	253.0
102.90	220.0
103.90	632.0
105.00	492.0
105.90	836.0
106.90	165.0
109.90	231.0
111.70	374.0
115.80	580.0
116.80	1056.0
117.80	779.0
118.90	1191.0
124.80	365.0
125.70	294.0
127.90	501.0
128.80	359.0
130.00	613.0
130.90	255.0
133.00	943.0
134.00	306.0
134.90	517.0
136.80	385.0
139.80	170.0
140.90	1716.0
141.70	210.0
143.00	1586.0
144.80	194.0
146.00	300.0
146.70	203.0
149.70	230.0
154.80	360.0
156.80	257.0
159.00	287.0
160.80	344.0
170.60	179.0
172.00	625.0
173.10	2041.0
173.90	103656.0
174.90	7994.0
175.90	98888.0
176.90	6933.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176

191.00	586.0
192.10	386.0
192.90	1287.0
194.00	277.0
207.10	446.0
207.90	259.0
248.90	447.0
265.00	491.0
265.80	164.0
281.10	5511.0
282.10	1995.0
283.10	1105.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176

m/z	Abundance
36.00	1279.0
37.00	8055.0
38.10	7536.0
39.00	2930.0
39.90	2238.0
41.00	213.0
42.80	152.0
44.10	1263.0
45.00	1995.0
47.00	2089.0
47.90	798.0
49.00	6338.0
50.00	30040.0
51.00	9065.0
52.00	475.0
55.00	361.0
55.90	2392.0
57.00	3692.0
58.00	244.0
58.90	160.0
60.00	1432.0
61.00	7770.0
62.00	6107.0
63.00	5857.0
64.00	441.0
65.00	251.0
67.10	349.0
68.00	14984.0
69.00	13738.0
70.00	1347.0
70.80	224.0
71.90	1051.0
73.00	8234.0
74.00	23520.0
75.00	68672.0
76.00	5150.0
76.90	1071.0
78.10	530.0
78.90	5877.0
80.00	1851.0
80.90	5260.0
81.90	1380.0
83.00	211.0
87.00	5378.0
87.90	4517.0
90.80	661.0
92.00	3915.0
93.00	5622.0
94.00	15522.0
95.00	118944.0
96.00	7315.0
97.00	220.0
102.90	349.0
103.70	694.0
104.70	266.0
105.10	176.0
105.80	561.0
106.90	233.0
110.90	285.0
111.70	198.0
112.90	172.0
114.70	278.0
115.00	273.0
115.80	553.0
116.90	1034.0
117.90	529.0
118.80	1054.0
125.10	175.0
125.90	180.0
127.90	649.0
129.00	222.0
129.80	648.0
130.80	250.0
132.80	872.0
133.10	841.0
133.90	489.0
135.00	371.0
137.00	184.0
139.60	203.0
140.90	1652.0
142.90	1662.0
145.80	194.0
147.60	343.0
149.10	239.0
149.80	177.0
154.80	284.0
157.00	180.0
158.90	375.0
160.90	174.0
163.00	217.0
171.50	319.0
173.10	2055.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176

173.90	96704.0
175.00	7450.0
175.90	98456.0
176.90	5817.0
178.10	226.0
178.80	218.0
191.00	539.0
192.00	279.0
193.00	985.0
194.00	259.0
207.00	638.0
249.10	579.0
251.00	230.0
265.00	515.0
265.90	204.0
267.00	259.0
280.20	237.0
281.00	6544.0
282.10	1733.0
283.00	1505.0
283.90	160.0

Instrument :
MSVOA_D
ClientSampleId :
BFB176