
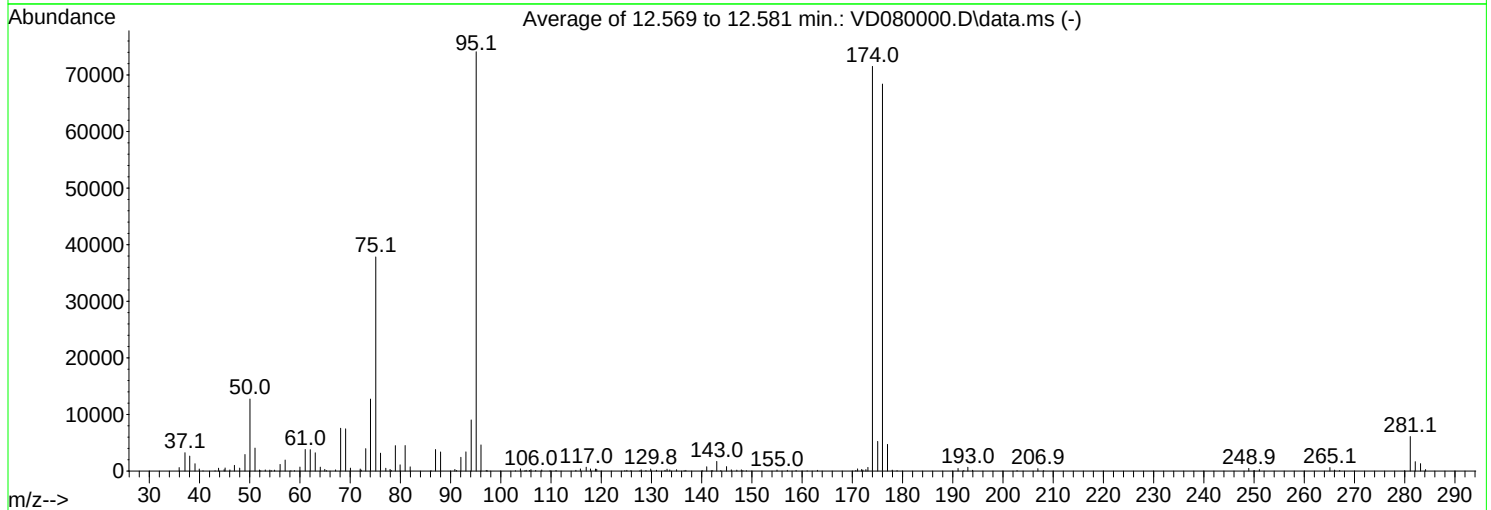


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111324\
Data File : VD080000.D
Acq On : 13 Nov 2024 09:39
Operator : RP/MD
Sample : BFB837
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB837

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM111224SMA.M
Title : SFAM01.0
Last Update : Wed Nov 13 03:23:57 2024

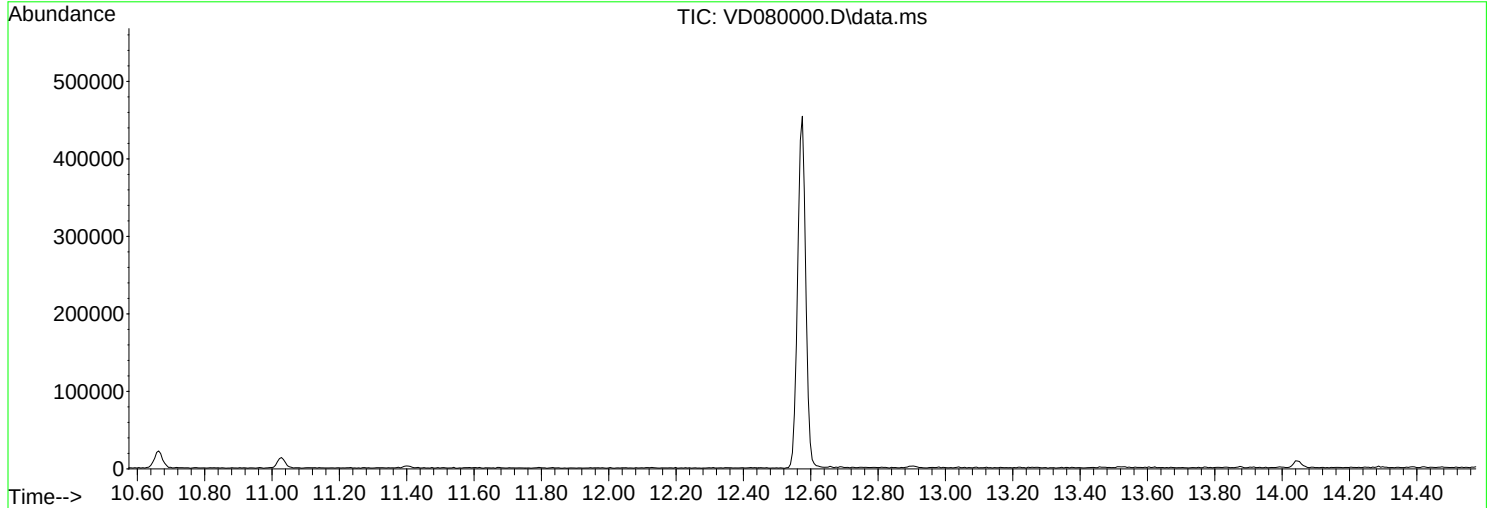

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	12735	PASS
75	95	30	80	51.1	37840	PASS
95	95	100	100	100.0	74104	PASS
96	95	5	9	6.2	4620	PASS
173	174	0.00	2	0.9	659	PASS
174	95	50	120	96.5	71515	PASS
175	174	5	9	7.3	5240	PASS
176	174	95	105	95.6	68397	PASS
177	176	5	10	6.9	4722	PASS

m/z	Abundance
39.90	557.0
43.80	251.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837

m/z	Abundance
36.00	534.0
37.10	3524.0
38.10	2934.0
39.10	1259.0
40.10	1021.0
43.90	744.0
44.90	738.0
46.00	359.0
46.90	1010.0
48.00	625.0
49.00	3209.0
50.10	14084.0
51.00	4610.0
52.00	417.0
53.10	199.0
54.00	173.0
54.90	256.0
56.00	1162.0
57.00	1903.0
60.00	765.0
61.00	4754.0
62.00	4278.0
63.10	3539.0
64.00	719.0
65.00	295.0
67.20	278.0
68.10	8771.0
69.10	8828.0
70.10	524.0
72.00	522.0
73.10	4671.0
74.10	12717.0
75.10	40232.0
76.10	3516.0
77.10	606.0
78.00	594.0
79.00	4697.0
80.00	919.0
80.90	4316.0
82.00	702.0
86.10	173.0
87.00	3661.0
88.00	3952.0
90.90	337.0
92.00	2456.0
93.00	3457.0
94.10	8961.0
95.10	76664.0
96.10	4780.0
97.10	359.0
104.00	367.0
104.80	175.0
106.00	298.0
108.20	164.0
109.80	156.0
115.90	486.0
116.90	660.0
118.00	243.0
118.80	584.0
128.00	395.0
129.80	367.0
131.10	205.0
133.10	484.0
135.00	282.0
136.80	209.0
141.00	737.0
143.00	1715.0
145.10	787.0
145.90	246.0
148.20	240.0
155.00	227.0
158.90	199.0
170.70	320.0
171.10	243.0
172.10	551.0
174.00	72128.0
175.00	5661.0
176.00	70040.0
177.00	5202.0
191.10	441.0
192.20	155.0
192.90	731.0
207.00	295.0
249.00	341.0
250.00	186.0
251.10	255.0
265.10	614.0
266.00	193.0
267.10	183.0
281.10	4810.0
282.10	1361.0
283.20	929.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837

284.30

234.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837

m/z	Abundance
36.00	808.0
37.10	3312.0
38.10	2788.0
39.10	1442.0
40.10	722.0
40.70	165.0
43.10	162.0
43.80	944.0
45.10	948.0
46.10	270.0
47.00	1257.0
48.10	583.0
49.10	3239.0
50.10	13602.0
51.10	4529.0
51.90	181.0
52.20	159.0
53.20	238.0
54.10	180.0
55.00	261.0
56.10	1268.0
57.10	2121.0
58.20	184.0
60.00	615.0
61.10	3629.0
62.10	3928.0
63.00	3396.0
64.00	829.0
64.90	230.0
65.30	227.0
67.00	180.0
68.10	7613.0
69.10	7556.0
70.00	798.0
72.00	577.0
73.10	3942.0
74.00	14613.0
75.10	41544.0
76.10	3363.0
77.00	619.0
78.20	300.0
79.00	4908.0
79.90	1413.0
81.00	5010.0
81.90	937.0
87.00	4235.0
88.00	3119.0
90.80	280.0
91.20	331.0
92.10	2826.0
93.00	3940.0
94.10	10011.0
95.10	83224.0
96.00	5179.0
97.30	177.0
102.90	169.0
103.90	483.0
105.00	169.0
105.70	344.0
106.90	181.0
108.10	238.0
111.00	349.0
114.90	203.0
115.80	406.0
117.00	823.0
117.80	599.0
119.10	967.0
124.70	206.0
125.10	235.0
125.90	175.0
127.90	295.0
128.90	311.0
129.90	281.0
130.90	251.0
132.70	407.0
133.60	244.0
135.00	309.0
136.50	218.0
141.00	936.0
141.90	224.0
143.00	1879.0
143.80	230.0
144.90	668.0
145.90	174.0
147.00	304.0
147.90	291.0
148.90	194.0
157.00	161.0
158.70	171.0
161.00	169.0
163.10	265.0
171.00	464.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837

171.80	257.0
173.10	1978.0
174.00	79000.0
175.10	5770.0
176.00	74784.0
177.00	5414.0
178.00	345.0
191.00	486.0
192.20	163.0
193.00	800.0
194.00	241.0
202.80	162.0
207.00	523.0
249.00	649.0
250.00	171.0
251.00	196.0
265.20	533.0
281.10	6708.0
282.10	2004.0
283.10	1671.0
284.10	267.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837

m/z	Abundance
35.90	505.0
37.10	2916.0
38.00	2219.0
39.10	1199.0
40.00	1024.0
43.90	605.0
45.10	718.0
47.00	779.0
47.90	370.0
49.00	2326.0
50.00	10518.0
51.10	3040.0
53.00	182.0
53.90	194.0
54.30	194.0
56.00	1114.0
57.00	1825.0
58.90	246.0
60.00	767.0
61.10	3078.0
62.00	3145.0
63.00	2749.0
64.10	554.0
65.00	381.0
67.10	190.0
68.10	6315.0
69.10	6017.0
70.00	257.0
72.20	519.0
73.10	3282.0
74.10	10840.0
75.10	31744.0
76.00	2600.0
77.20	285.0
77.80	311.0
79.00	3872.0
79.90	968.0
80.90	4217.0
82.00	598.0
87.00	3529.0
88.00	3046.0
90.80	269.0
92.00	2014.0
93.10	2795.0
94.10	8136.0
95.10	62424.0
96.10	3901.0
103.80	359.0
105.10	240.0
106.00	500.0
107.00	181.0
108.10	195.0
115.00	207.0
115.80	267.0
117.10	577.0
117.90	305.0
118.90	528.0
125.10	168.0
127.70	205.0
129.90	436.0
133.10	537.0
133.70	377.0
135.00	156.0
136.90	179.0
140.20	169.0
141.00	618.0
142.20	241.0
143.00	1538.0
144.90	924.0
145.90	254.0
147.00	202.0
147.90	380.0
155.00	334.0
157.10	242.0
163.00	165.0
171.00	459.0
171.90	600.0
172.70	782.0
174.00	63416.0
175.00	4290.0
176.00	60368.0
177.00	3551.0
177.90	178.0
178.90	279.0
191.10	478.0
193.10	472.0
193.90	203.0
202.80	156.0
206.90	496.0
208.10	193.0
248.90	447.0
251.00	372.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837

265.00	723.0
266.10	335.0
267.00	150.0
280.00	157.0
281.10	6795.0
282.10	1617.0
283.10	1357.0
284.10	289.0

Instrument :
MSVOA_D
ClientSampleId :
BFB837