

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD111418\
 Data File : VD060383.D
 Acq On : 14 Nov 2018 17:09
 Operator : JC/SY
 Sample : J5918-03MS
 Misc : 5.02g/5ml/MSVOA D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FDSB-05(25-27)MS

Quant Time: Nov 15 05:42:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 06 13:56:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-6.43
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-7.46
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.30
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.38

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD111418\
Data File : VD060383.D
Acq On : 14 Nov 2018 17:09
Operator : JC/SY
Sample : J5918-03MS
Misc : 5.02g/5ml/MSVOA D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FDSB-05(25-27)MS

Quant Time: Nov 15 05:42:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 06 13:56:04 2018
Response via : Initial Calibration

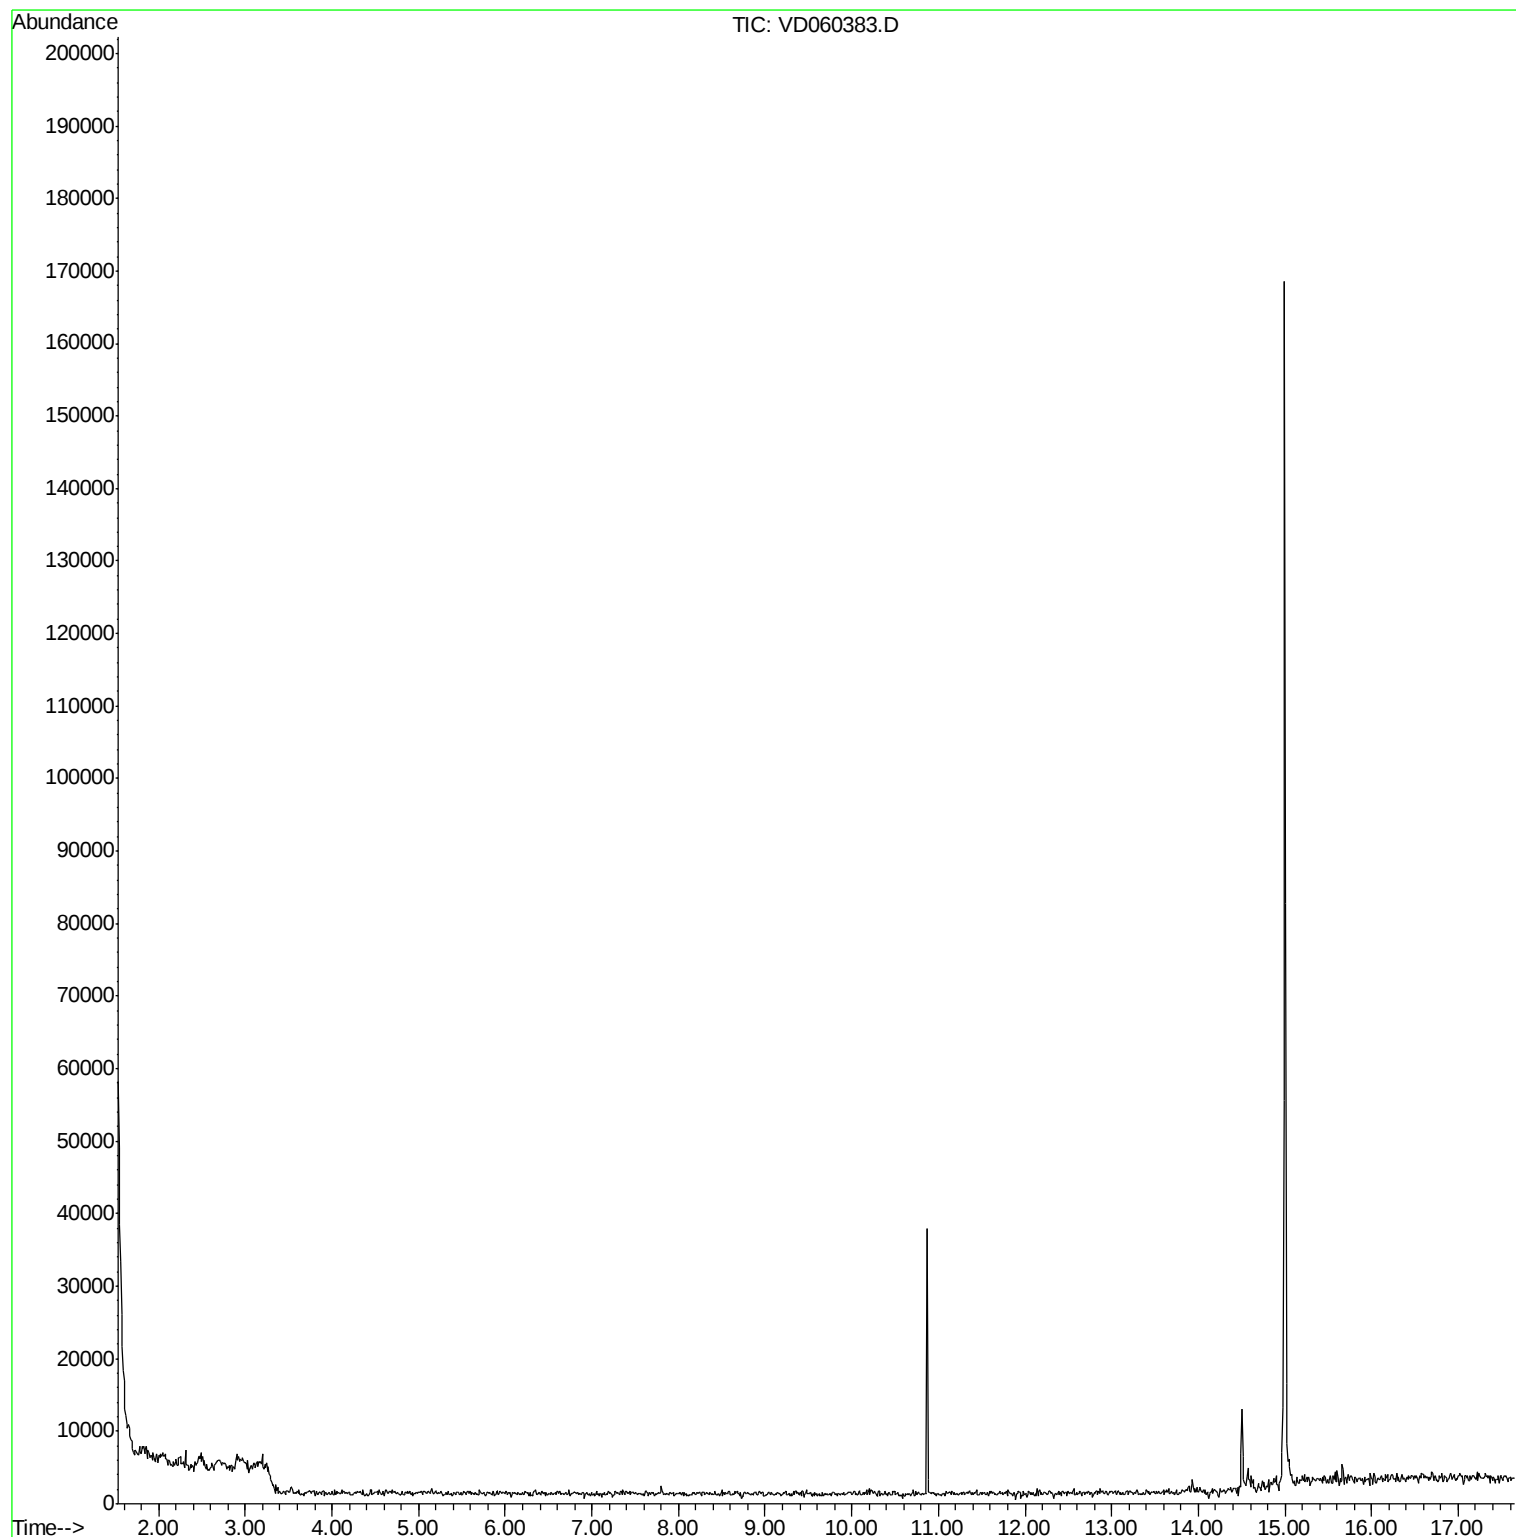

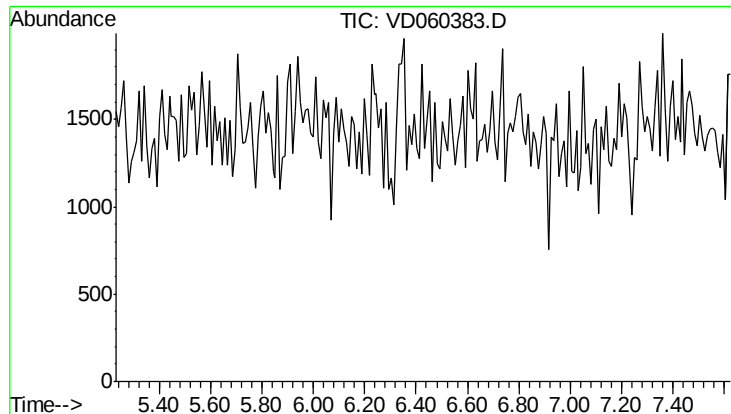

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 6.43 min

Lab File: VD060383.D

Acq: 14 Nov 2018 17:09

Tot Ion: 168

Sig Exp Ratio

168 100



99 49.8

Instrument :

MSVOA_D

ClientSampleId :

FDSB-05(25-27)MS

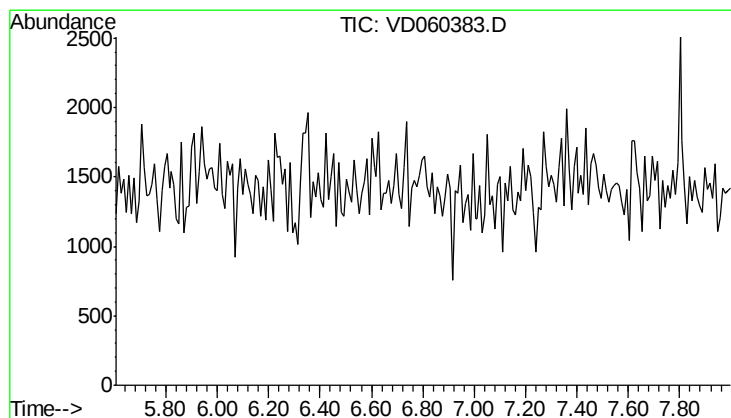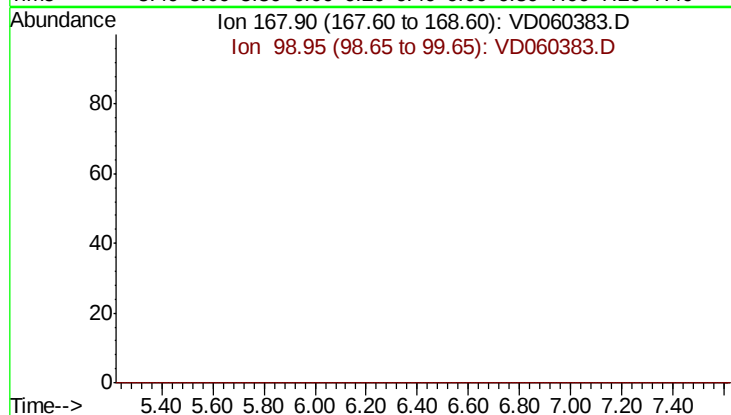

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

Expected RT: 6.80 min

Lab File: VD060383.D


Acq: 14 Nov 2018 17:09


Tgt Ion: 65

Sig Exp Ratio

65 100

67 54.9


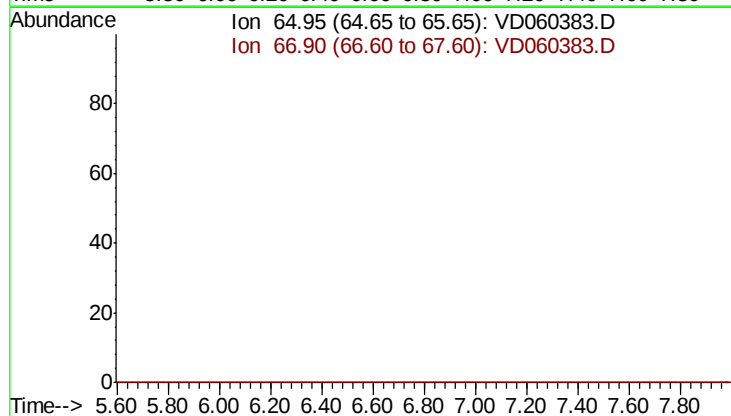


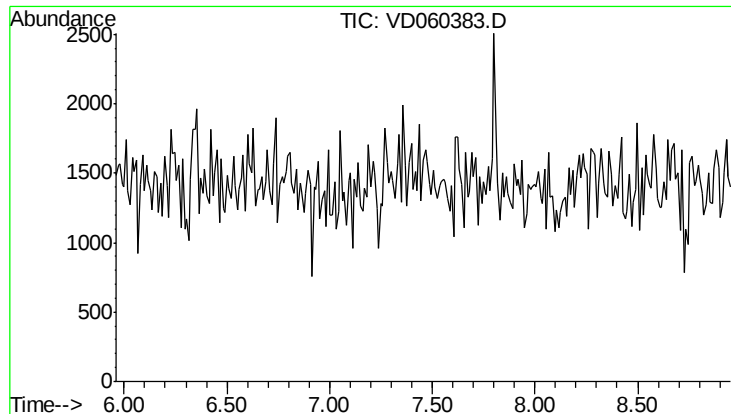

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 7.46 min
 Lab File: VD060383.D
 Acq: 14 Nov 2018 17:09


Instrument :
 MSVOA_D
 ClientSampleId :
 FDSB-05(25-27)MS


Tot Ion: 114
 Sig Exp Ratio
 114 100
 63 17.0
 88 17.7

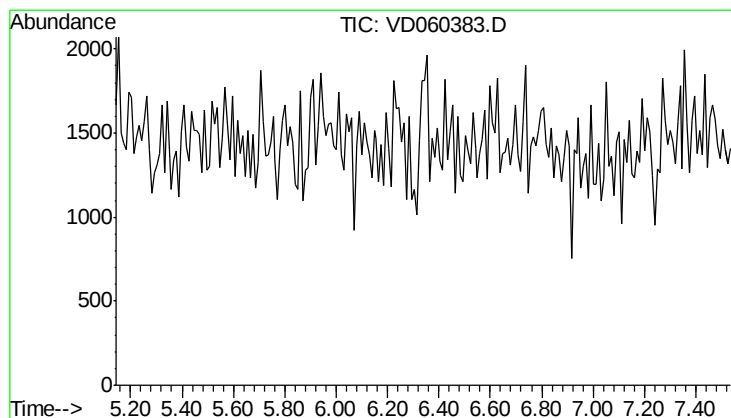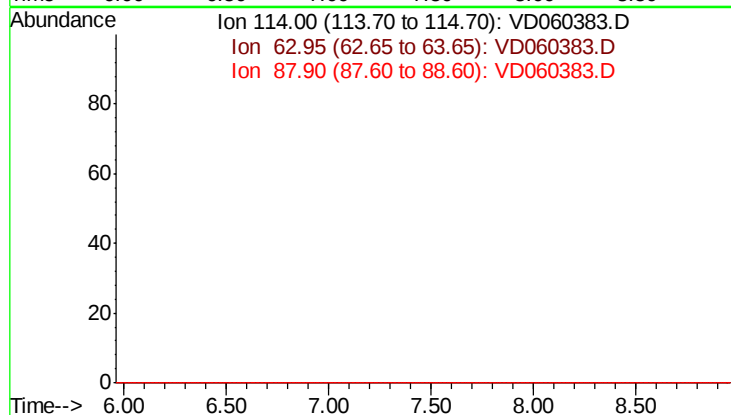

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 6.34 min
 Lab File: VD060383.D
 Acq: 14 Nov 2018 17:09

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 102.0
 192 20.6

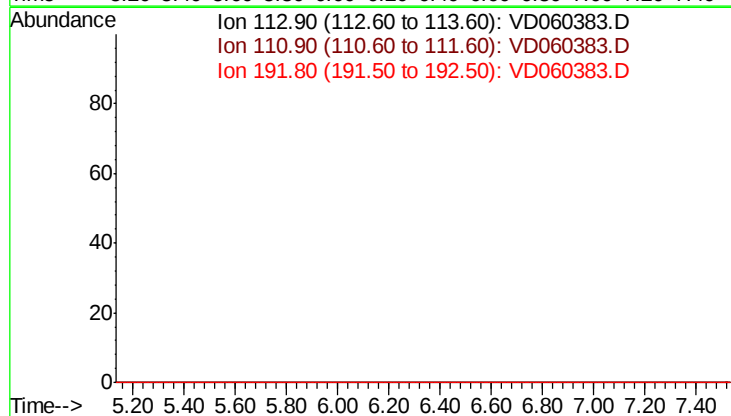


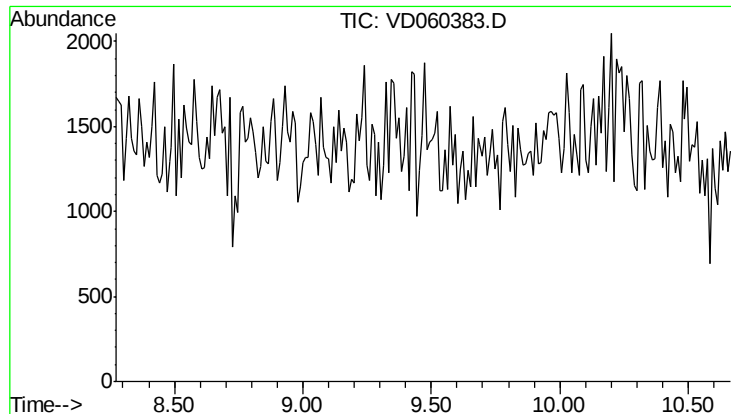


#50
Toluene-d8
Concen: N.D. ug/l
Expected RT: 9.47 min

Lab File: VD060383.D
Acq: 14 Nov 2018 17:09

Instrument :
MSVOA_D
ClientSampleId :
FDSB-05(25-27)MS


Tot Ion:	98
Sig	Exp Ratio
98	100
100	69.0

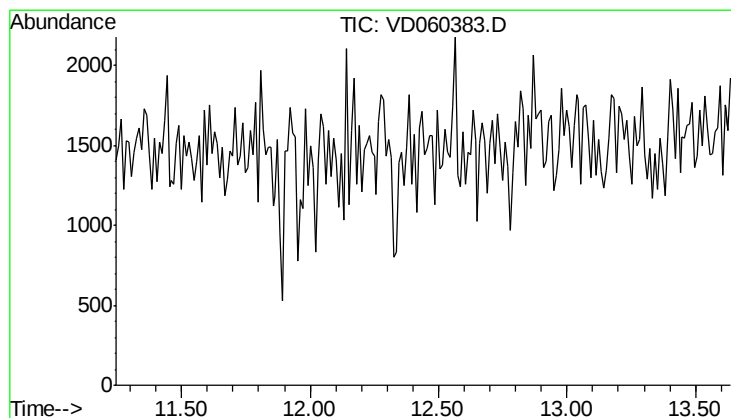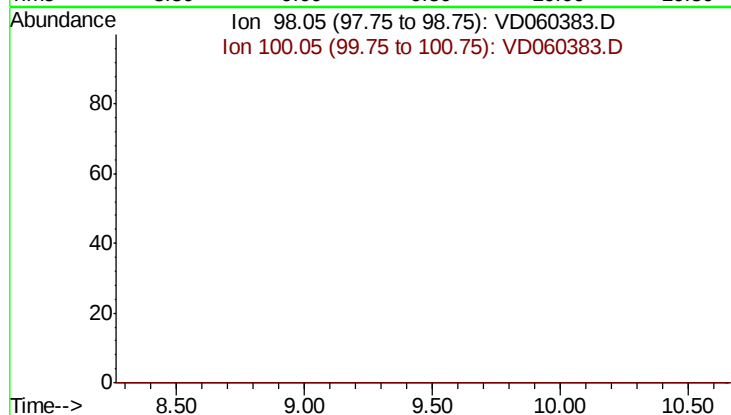


#62
4-Bromofluorobenzene
Concen: N.D. ug/l
Expected RT: 12.44 min

Lab File: VD060383.D
Acq: 14 Nov 2018 17:09

Tgt Ion:	95
Sig	Exp Ratio
95	100
174	80.4
176	77.3


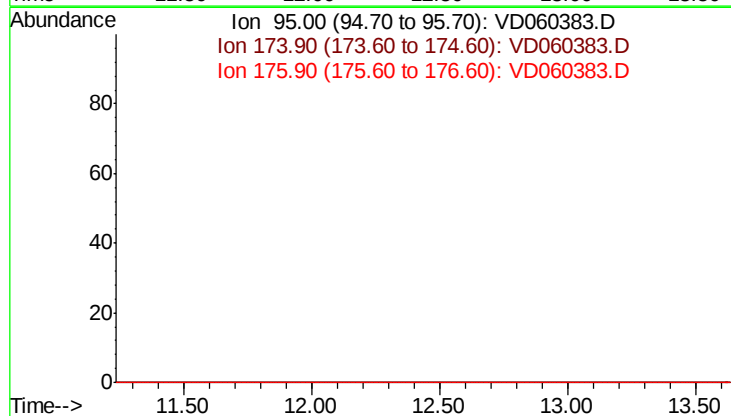


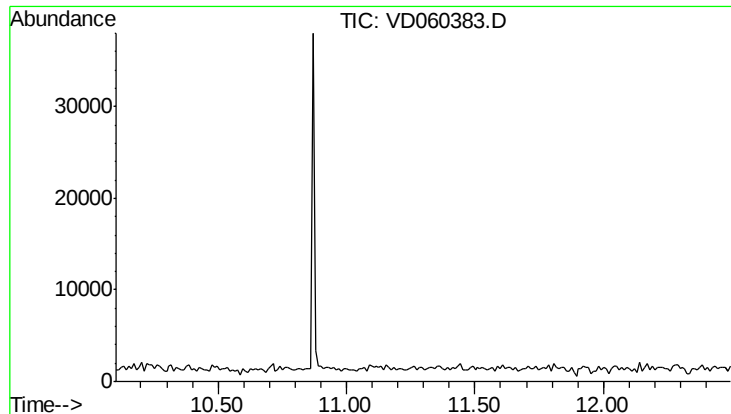

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.30 min
 Lab File: VD060383.D
 Acq: 14 Nov 2018 17:09

Instrument :
 MSVOA_D
 ClientSampleId :
 FDSB-05(25-27)MS

Tot Ion	117
Sig	Exp Ratio
117	100
82	54.6
119	32.6

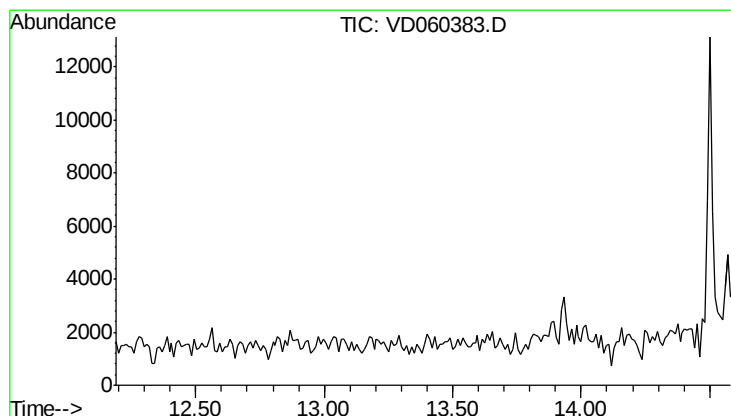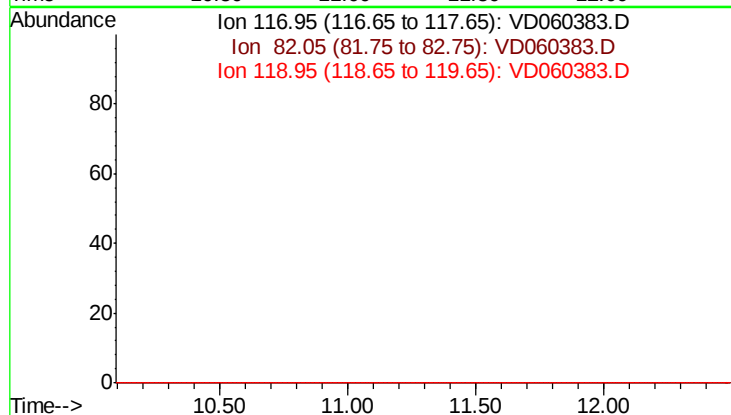

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.38 min
 Lab File: VD060383.D
 Acq: 14 Nov 2018 17:09

Tgt Ion	152
Sig	Exp Ratio
152	100
115	48.2
150	155.3

