


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111418\
Data File : VD060369.D
Acq On : 14 Nov 2018 9:44
Operator : JC/SY
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Title : SW846 8260
Last Update : Tue Nov 06 13:56:04 2018

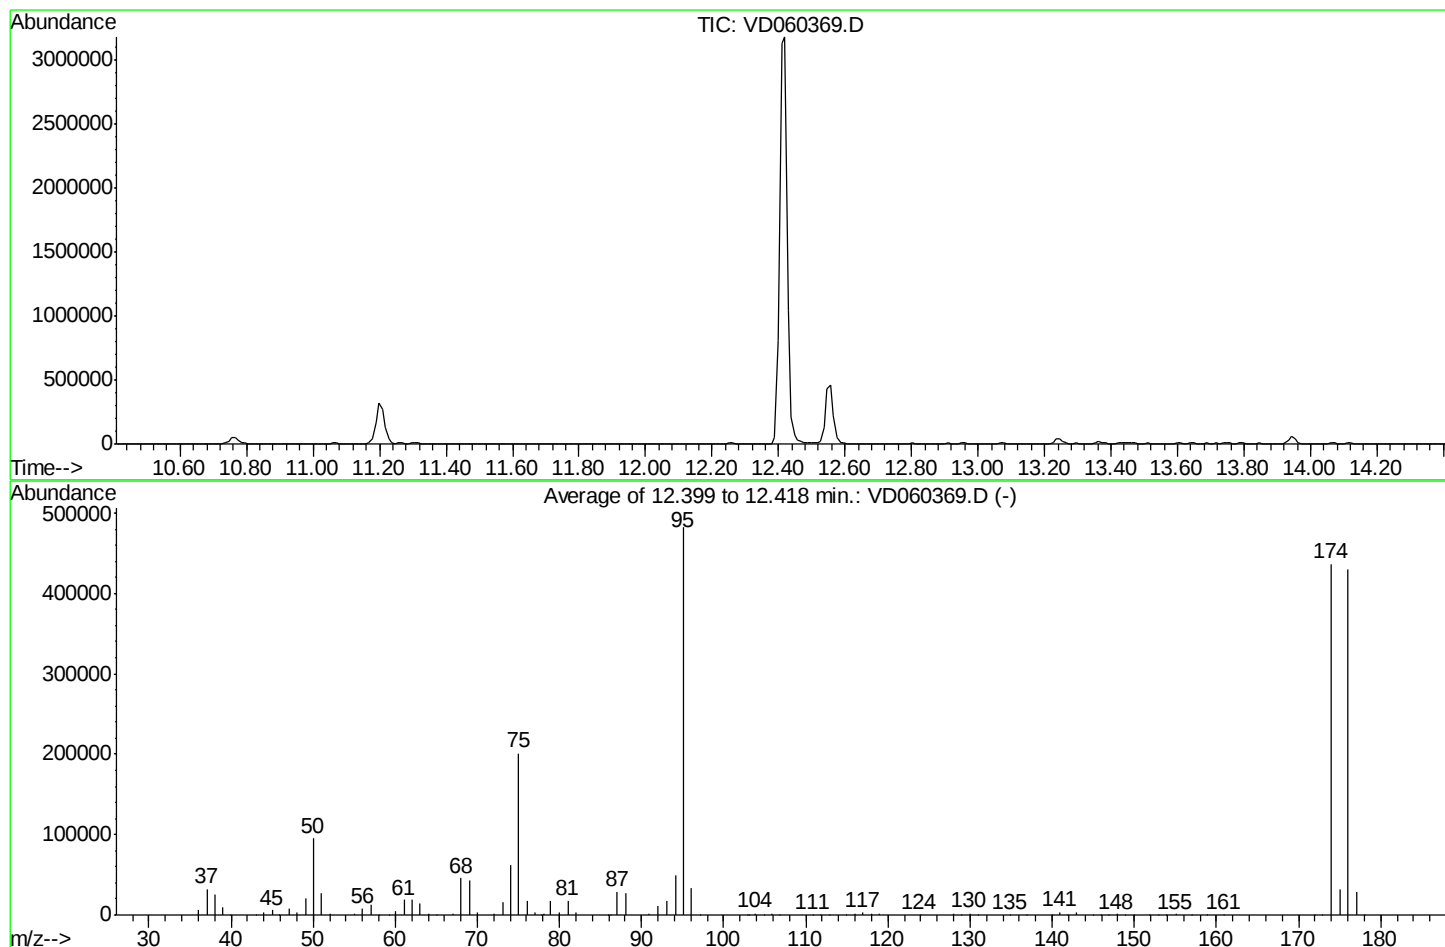

AutoFind: Scans 1105, 1106, 1107; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	94829	PASS
75	95	30	60	41.8	201450	PASS
95	95	100	100	100.0	482197	PASS
96	95	5	9	6.8	32859	PASS
173	174	0.00	2	0.1	231	PASS
174	95	50	100	90.6	436965	PASS
175	174	5	9	7.4	32409	PASS
176	174	95	101	98.5	430405	PASS
177	176	5	9	6.5	28023	PASS