
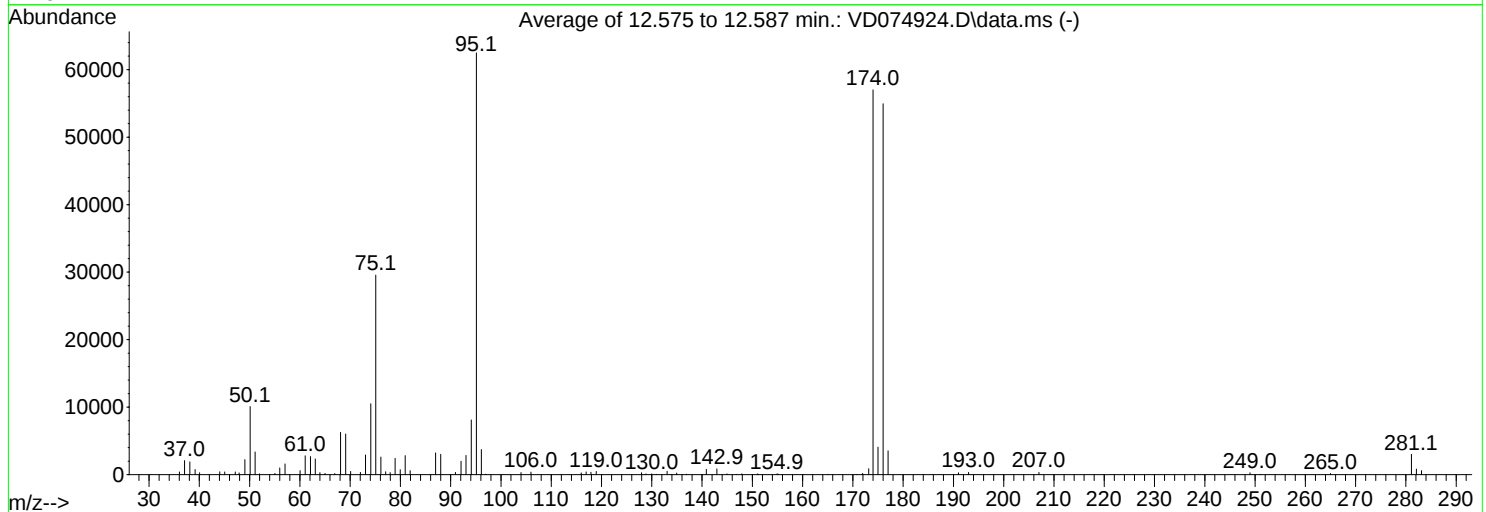


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111422\
 Data File : VD074924.D
 Acq On : 14 Nov 2022 09:50
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
 Title : SW846 8260
 Last Update : Mon Nov 14 00:51:58 2022

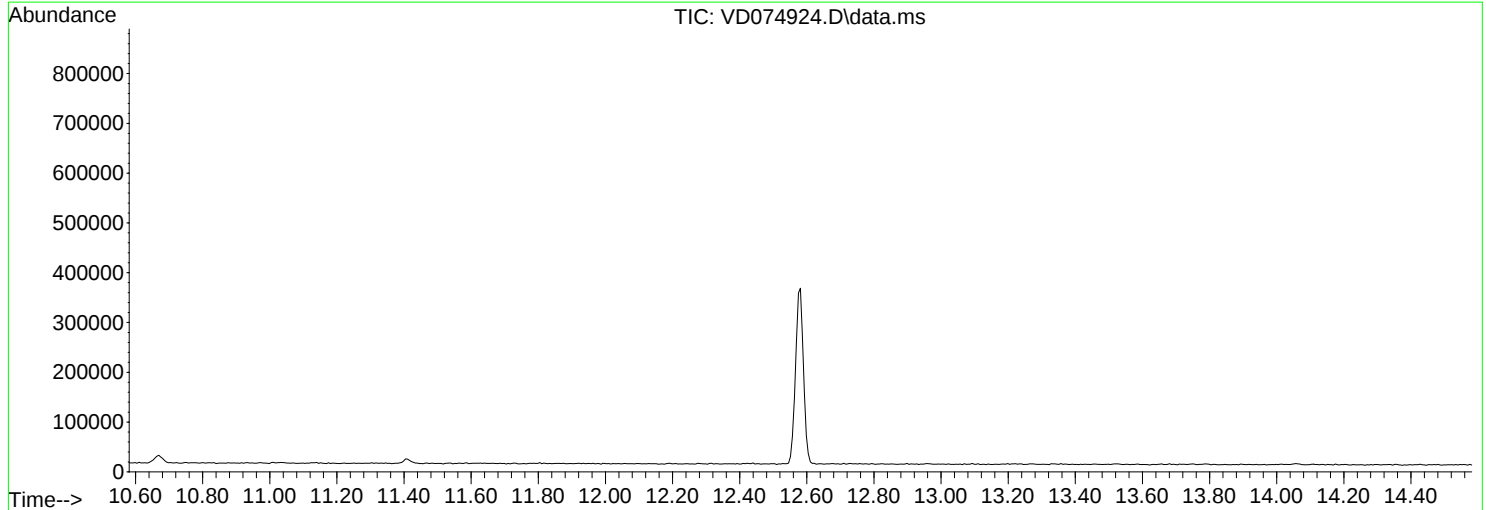

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	10109	PASS
75	95	30	60	47.3	29555	PASS
95	95	100	100	100.0	62488	PASS
96	95	5	9	6.0	3721	PASS
173	174	0.00	2	1.5	878	PASS
174	95	50	100	91.2	57013	PASS
175	174	5	9	7.2	4088	PASS
176	174	95	101	96.4	54936	PASS
177	176	5	9	6.5	3547	PASS