


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111519\
Data File : VD064216.D
Acq On : 15 Nov 2019 08:44
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Title : SW846 8260
Last Update : Tue Nov 12 02:43:24 2019

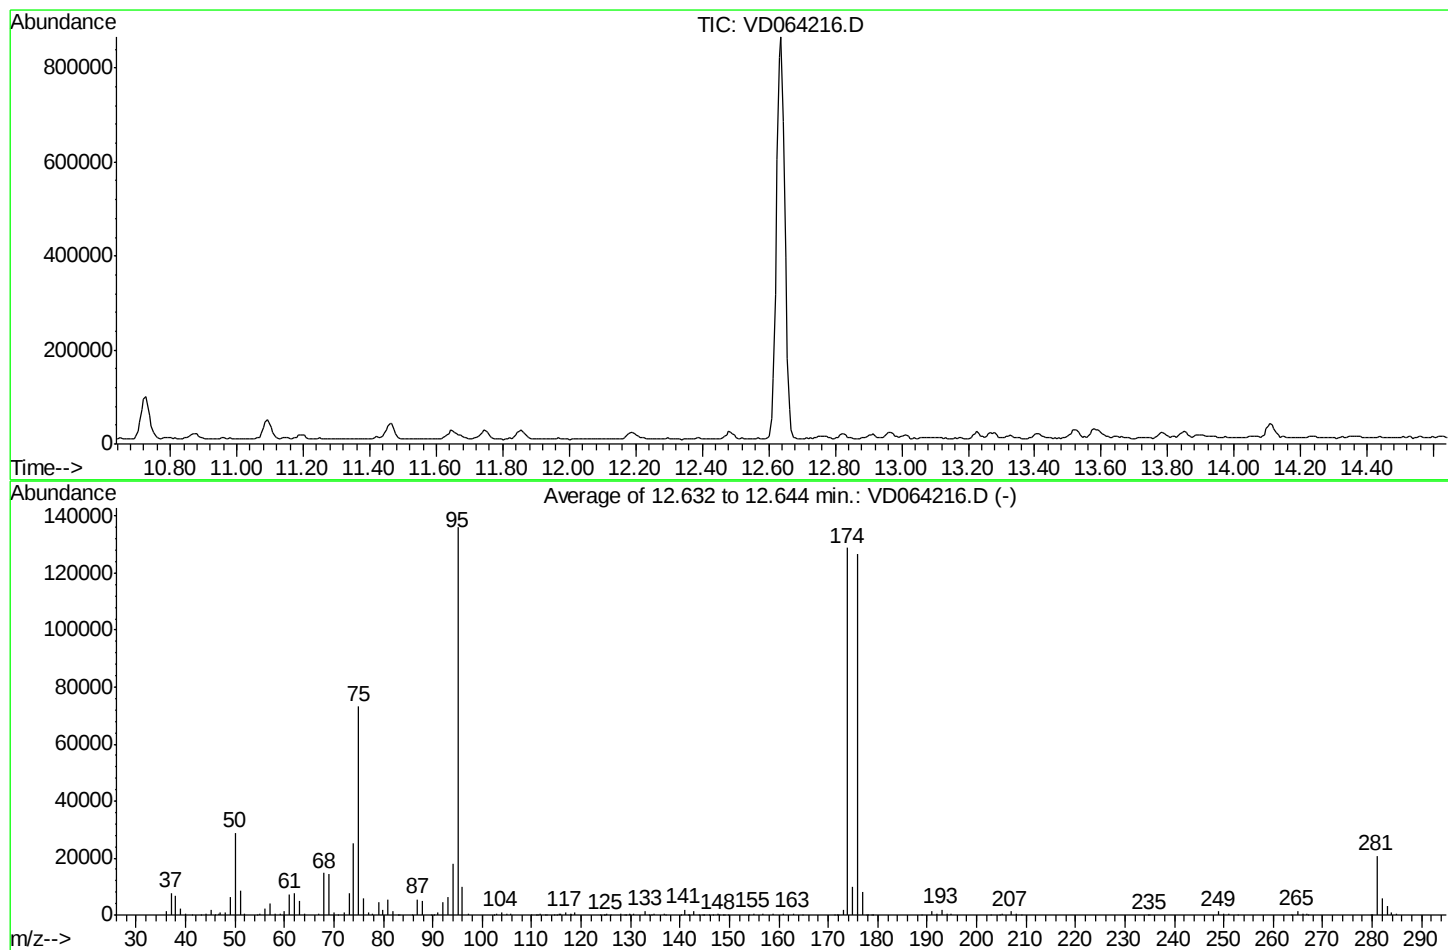

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	28781	PASS
75	95	30	60	53.8	73192	PASS
95	95	100	100	100.0	136090	PASS
96	95	5	9	7.1	9681	PASS
173	174	0.00	2	1.3	1646	PASS
174	95	50	100	94.7	128890	PASS
175	174	5	9	7.5	9695	PASS
176	174	95	101	98.2	126594	PASS
177	176	5	9	6.5	8166	PASS