


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD111519\
Data File : VD064239.D
Acq On : 15 Nov 2019 21:18
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Title : SW846 8260
Last Update : Tue Nov 12 02:43:24 2019

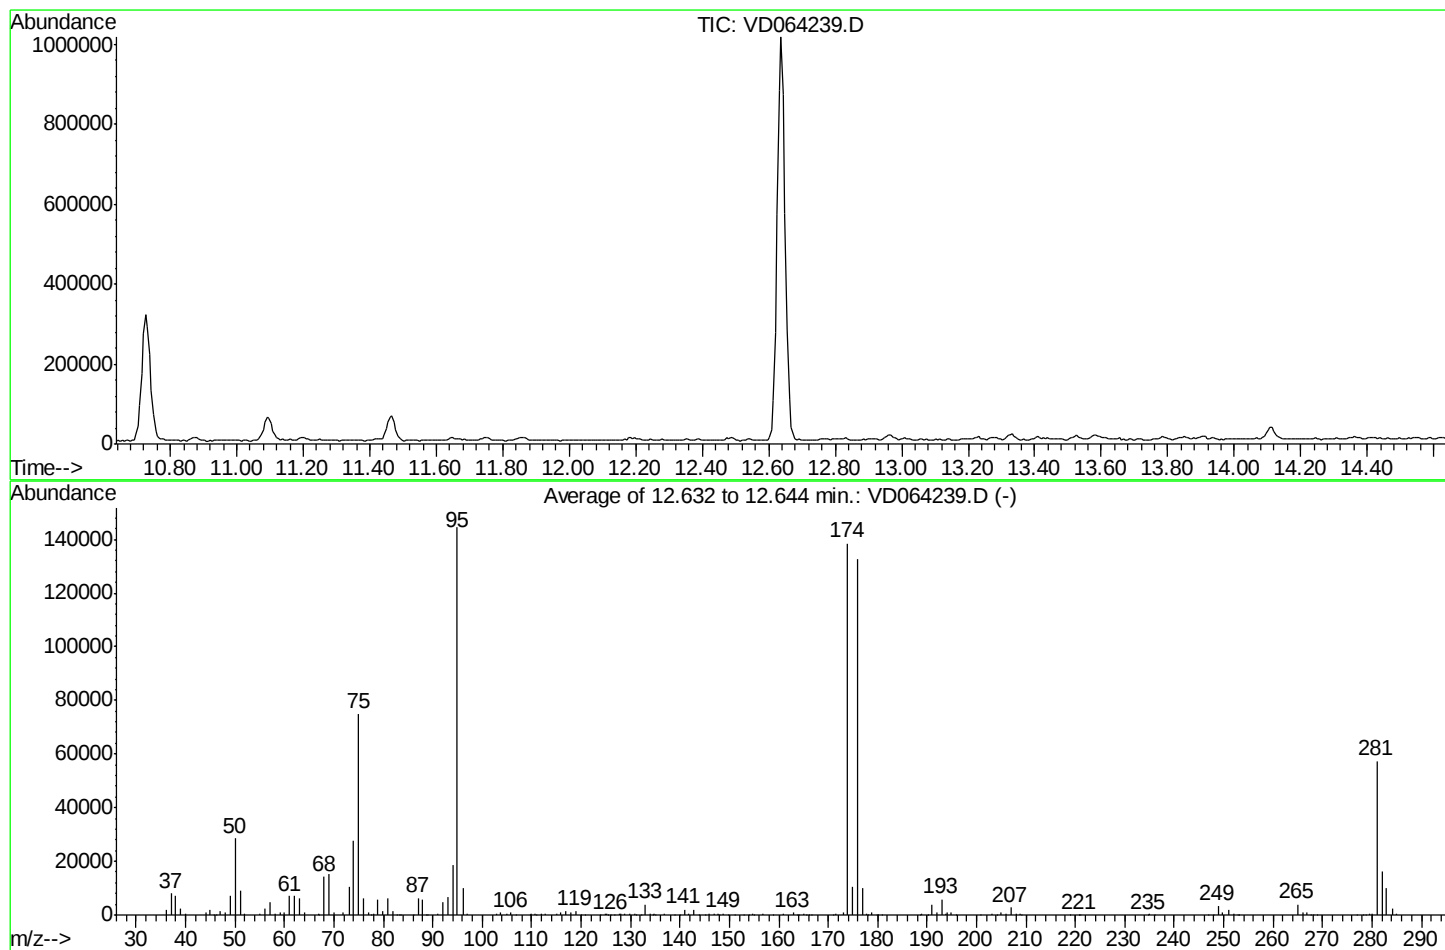

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	28493	PASS
75	95	30	60	51.9	75037	PASS
95	95	100	100	100.0	144490	PASS
96	95	5	9	6.8	9843	PASS
173	174	0.00	2	0.8	1047	PASS
174	95	50	100	95.9	138541	PASS
175	174	5	9	7.7	10715	PASS
176	174	95	101	95.9	132877	PASS
177	176	5	9	7.6	10112	PASS