


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111521\
 Data File : VD071028.D
 Acq On : 15 Nov 2021 14:49
 Operator : VA/SY
 Sample : M4563-01
 Misc : 5.02G/5.00ml/MSVOA_D/SoIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Nov 16 03:21:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 10 03:55:51 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	7.985	168	2169	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	3079	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	2181	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	617	50.000	ug/l	0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	1028	44.515	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	89.020%
35) Dibromofluoromethane	7.908	113	873	50.247	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.500%
50) Toluene-d8	10.332	98	3859	56.715	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	113.440%
62) 4-Bromofluorobenzene	12.620	95	1180	48.165	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.340%
Target Compounds						
					Qvalue	
14) Allyl chloride	4.750	41	55	1.282	ug/l #	28
16) Acetone	4.167	43	199	49.178	ug/l #	40
18) Methyl Acetate	4.750	43	126	6.360	ug/l #	51
23) Vinyl Acetate	6.414	43	54	22.069	ug/l #	72
36) 1,1-Dichloropropene	7.985	75	67	2.437	ug/l #	41
37) Ethyl Acetate	7.491	43	59	4.704	ug/l #	66
38) Carbon Tetrachloride	7.985	117	68	2.686	ug/l #	12
39) Methylcyclohexane	9.344	83	65	1.831	ug/l #	16
41) Methacrylonitrile	7.544	41	172	20.974	ug/l #	12
43) Isopropyl Acetate	8.344	43	63	2.373	ug/l #	47
48) Methyl methacrylate	9.491	41	69	5.299	ug/l #	15
51) 4-Methyl-2-Pentanone	10.244	43	68	5.284	ug/l #	34
55) 1,1,2-Trichloroethane	10.791	97	68	4.965	ug/l #	16
59) 2-Hexanone	11.020	43	68	22.261	ug/l #	22
68) m/p-Xylenes	12.049	106	59	2.142	ug/l #	1
69) o-Xylene	12.049	106	59	2.252	ug/l #	1
74) N-amyl acetate	12.261	43	1465	115.365	ug/l #	57
75) 1,1,2,2-Tetrachloroethane	12.690	83	73	9.541	ug/l #	1
76) 1,2,3-Trichloropropane	12.626	75	239	45.347	ug/l #	1
77) Bromobenzene	12.937	156	53	5.581	ug/l #	63
78) n-propylbenzene	12.820	91	284	5.156	ug/l #	54
79) 2-Chlorotoluene	12.873	91	65	2.070	ug/l #	42
80) 1,3,5-Trimethylbenzene	12.914	105	54	1.475	ug/l #	28
81) trans-1,4-Dichloro-2-b...	12.626	75	239	84.847	ug/l #	18
82) 4-Chlorotoluene	12.949	91	68	2.098	ug/l #	42
83) tert-Butylbenzene	13.220	119	55	1.745	ug/l #	54
84) 1,2,4-Trimethylbenzene	13.390	105	2465	68.774	ug/l #	31
85) sec-Butylbenzene	13.390	105	2465	52.008	ug/l	92
86) p-Isopropyltoluene	13.502	119	857	22.518	ug/l #	64
89) n-Butylbenzene	13.826	91	1321	34.538	ug/l #	54
90) Hexachloroethane	14.090	117	147	19.519	ug/l #	14

(#) = qualifier out of range (m) = manual integration (+) = signals summed






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. 0.006 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49


Instrument :
MSVOA_D
ClientSampleId :

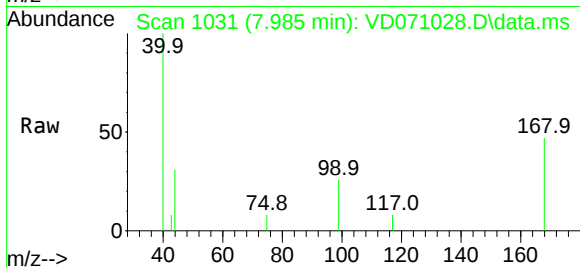



Tgt Ion:168 Resp: 2169
Ion Ratio Lower Upper
168 100
99 55.5 46.6 69.8

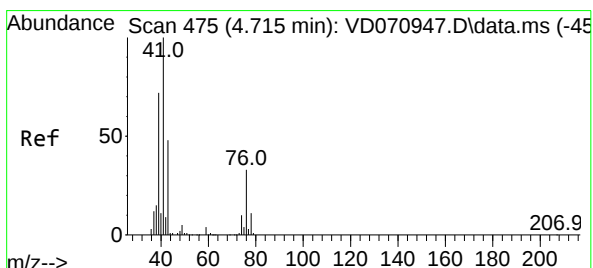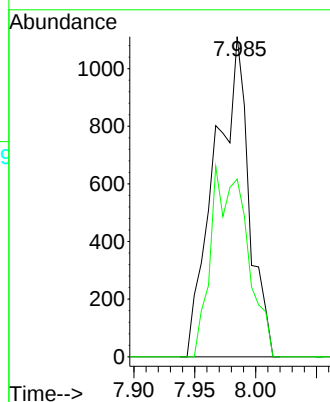


#14
Allyl chloride
Concen: 1.282 ug/l
RT: 4.750 min Scan# 481
Delta R.T. 0.035 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

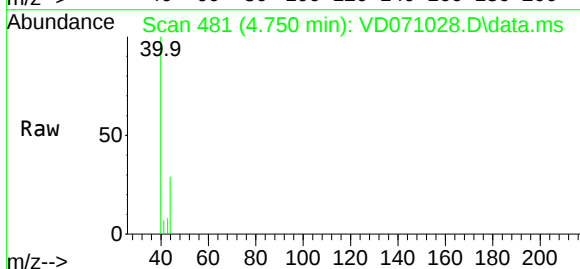

Tgt Ion: 41 Resp: 55
Ion Ratio Lower Upper
41 100
39 0.0 45.6 68.4#
76 0.0 30.2 45.4#



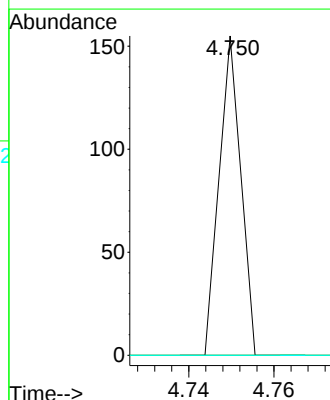
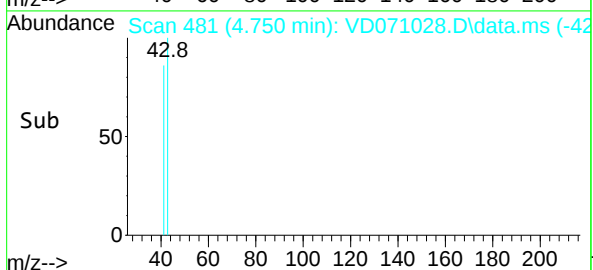




#16
Acetone
Concen: 49.178 ug/l
RT: 4.167 min Scan# 381
Delta R.T. 0.011 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 199
Ion Ratio Lower Upper
43 100
58 0.0 27.8 41.8#

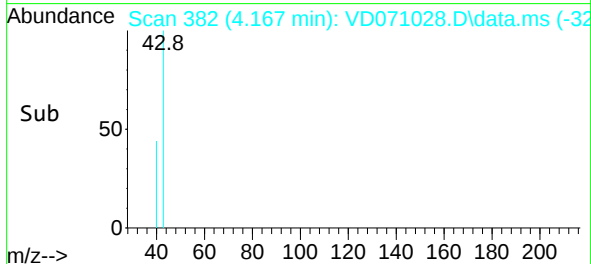

#18
Methyl Acetate
Concen: 6.360 ug/l
RT: 4.750 min Scan# 481
Delta R.T. 0.035 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion: 43 Resp: 126
Ion Ratio Lower Upper
43 100
74 0.0 19.3 28.9#




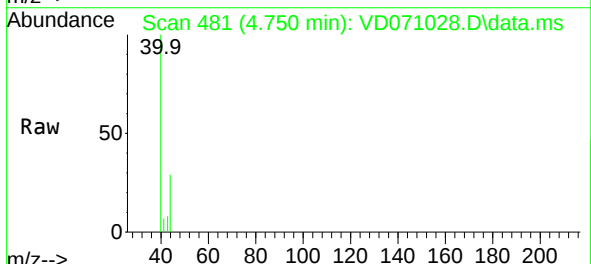




#23
 Vinyl Acetate
 Concen: 22.069 ug/l
 RT: 6.414 min Scan# 70
 Delta R.T. 0.111 min
 Lab File: VD071028.D
 Acq: 15 Nov 2021 14:49




Instrument :
 MSVOA_D
 ClientSampleId :


Tgt Ion: 43 Resp: 54
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.2 12.4#

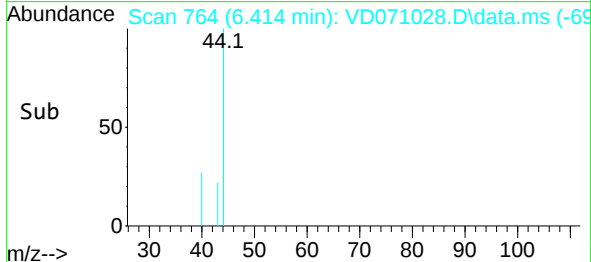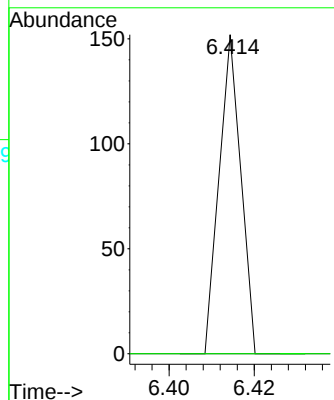

#33
 1,2-Dichloroethane-d4
 Concen: 44.515 ug/l
 RT: 8.326 min Scan# 1089
 Delta R.T. -0.006 min
 Lab File: VD071028.D
 Acq: 15 Nov 2021 14:49

Tgt Ion: 65 Resp: 1028
 Ion Ratio Lower Upper
 65 100
 67 37.2 0.0 112.2

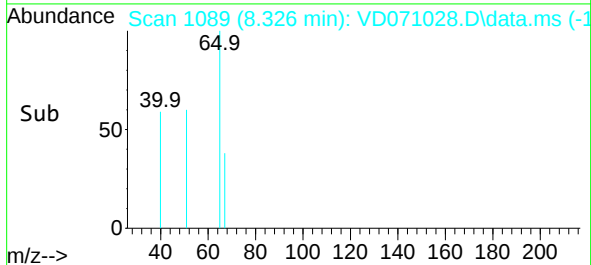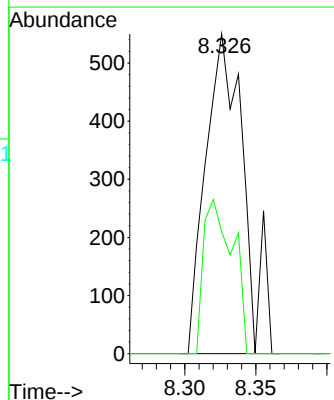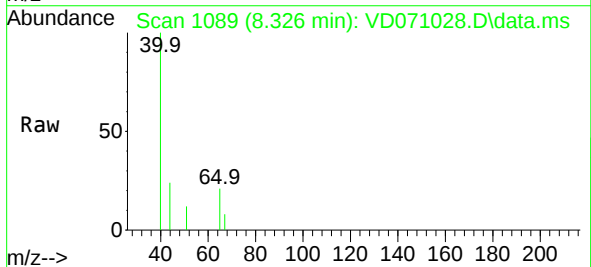



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD071028.D





Acq: 15 Nov 2021 14:49

Instrument :

MSVOA_D

ClientSampleId :

Tgt Ion:114	Resp:	3079
Ion Ratio	Lower	Upper
114	100	
63	12.8	0.0 41.8
88	15.0	0.0 32.8

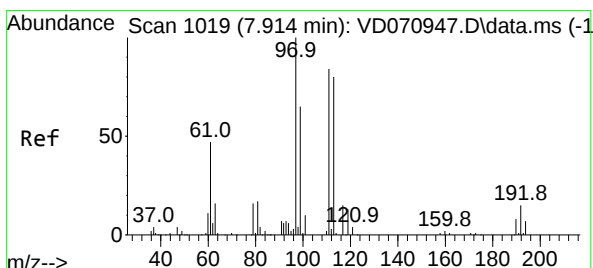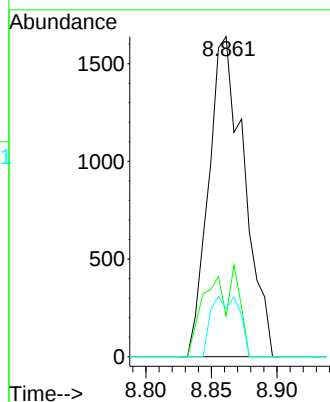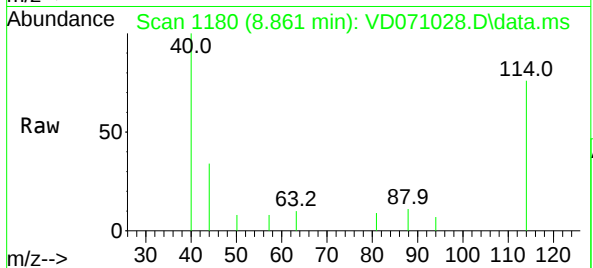

#35

Dibromofluoromethane

Concen: 50.247 ug/l




RT: 7.908 min Scan# 1018


Delta R.T. -0.006 min

Lab File: VD071028.D

Acq: 15 Nov 2021 14:49

Tgt Ion:113	Resp:	873
Ion Ratio	Lower	Upper
113	100	
111	96.0	82.0 123.0
192	0.0	15.2 22.8

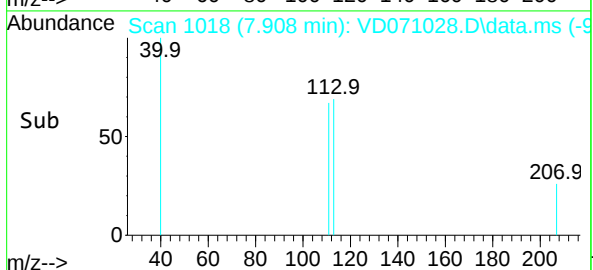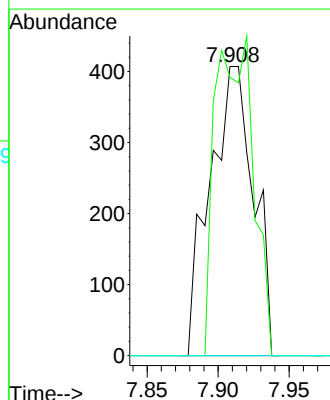



#36

1,1-Dichloropropene

Concen: 2.437 ug/l

RT: 7.985 min Scan# 1

Delta R.T. -0.123 min


Lab File: VD071028.D

Acq: 15 Nov 2021 14:49




Instrument :

MSVOA_D

ClientSampleId :

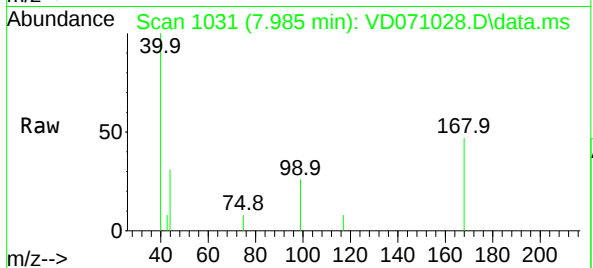

Tgt Ion:	75	Resp:	67
Ion	Ratio	Lower	Upper
75	100		
110	0.0	17.8	53.4#
77	0.0	24.8	37.2#

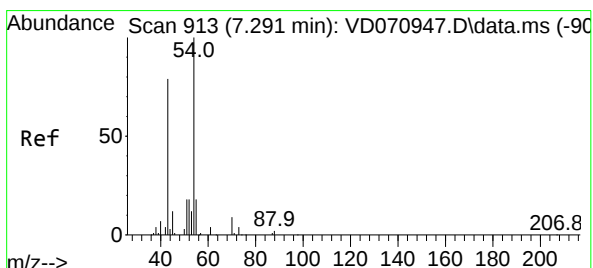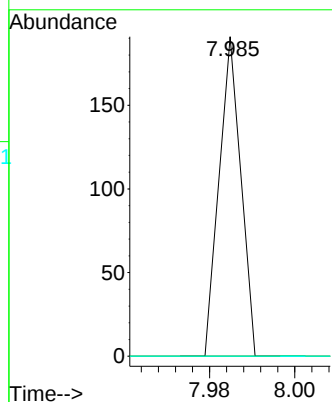

#37

Ethyl Acetate

Concen: 4.704 ug/l




RT: 7.491 min Scan# 947


Delta R.T. 0.200 min

Lab File: VD071028.D

Acq: 15 Nov 2021 14:49


Tgt Ion:	43	Resp:	59
Ion	Ratio	Lower	Upper
43	100		
61	0.0	13.0	19.6#
70	0.0	8.7	13.1#

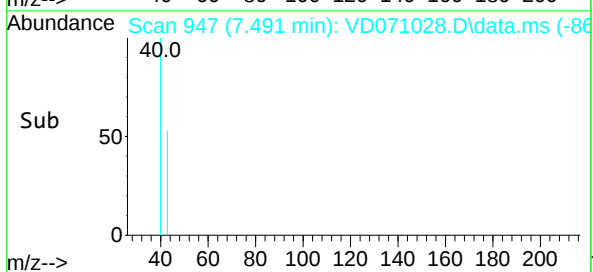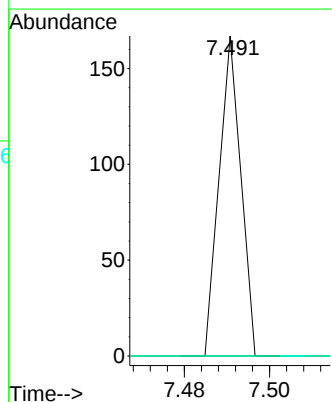






#38
Carbon Tetrachloride
Concen: 2.686 ug/l
RT: 7.985 min Scan# 1050
Delta R.T. -0.112 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Instrument :
MSVOA_D
ClientSampleId :



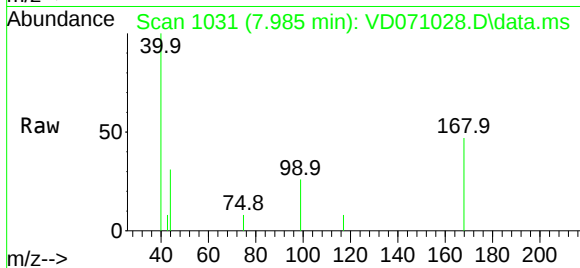



Tgt Ion:117 Resp: 68
Ion Ratio Lower Upper
117 100
119 0.0 75.8 113.6#
121 0.0 23.6 35.4#

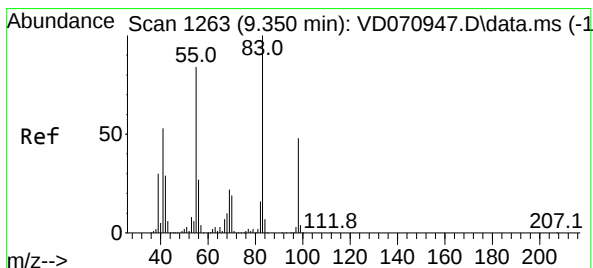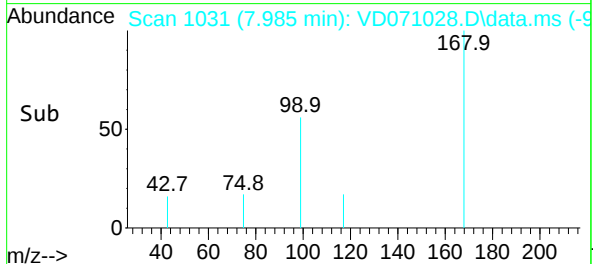

#39
Methylcyclohexane
Concen: 1.831 ug/l
RT: 9.344 min Scan# 1262
Delta R.T. -0.006 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49


Tgt Ion: 83 Resp: 65
Ion Ratio Lower Upper
83 100
55 0.0 65.8 98.8#
98 0.0 38.7 58.1#

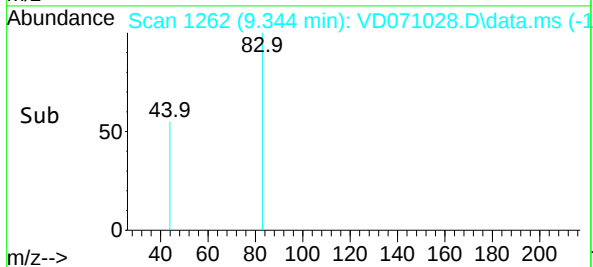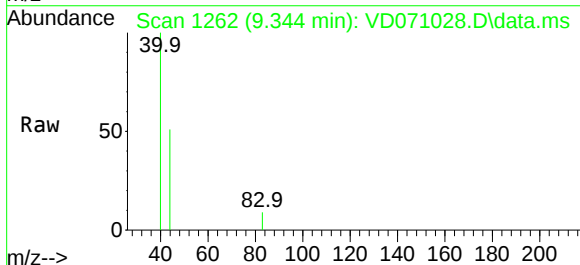






#41
Methacrylonitrile
Concen: 20.974 ug/l
RT: 7.544 min Scan# 91
Delta R.T. 0.030 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Instrument :
MSVOA_D
ClientSampleId :



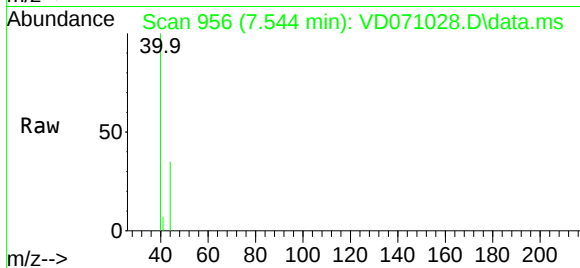



Tgt Ion:	41	Resp:	172
Ion	Ratio	Lower	Upper
41	100		
39	0.0	60.2	90.4#
67	0.0	74.8	112.2#
52	0.0	28.8	43.2#

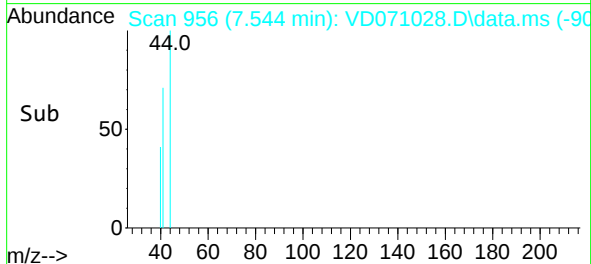

#43
Isopropyl Acetate
Concen: 2.373 ug/l
RT: 8.344 min Scan# 1092
Delta R.T. -0.106 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion:	43	Resp:	63
Ion	Ratio	Lower	Upper
43	100		
61	0.0	28.2	42.4#
87	0.0	10.7	16.1#

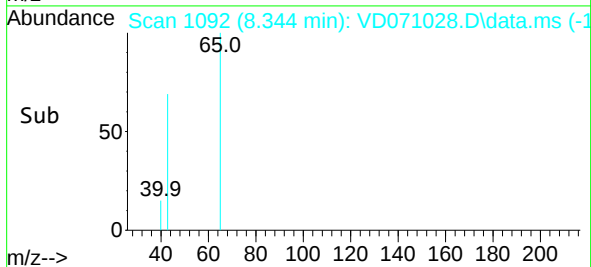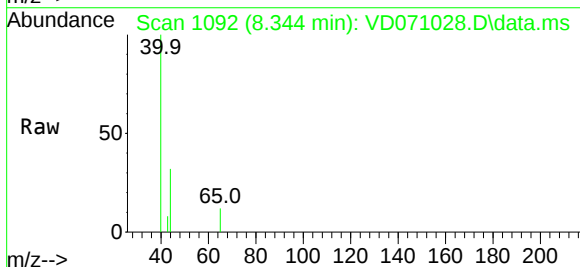



#48

Methyl methacrylate

Concen: 5.299 ug/l

RT: 9.491 min Scan# 11

Delta R.T. 0.041 min

Lab File: VD071028.D

Acq: 15 Nov 2021 14:49

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion: 41 Resp: 69

Ion Ratio Lower Upper

41 100

69 0.0 69.8 104.6#

39 0.0 35.6 53.4#

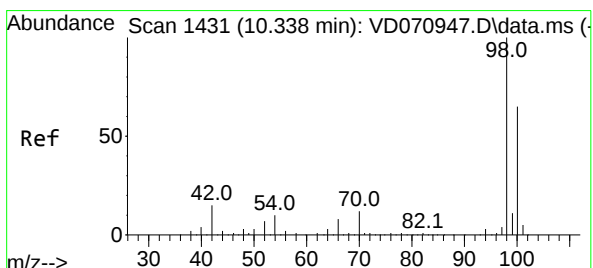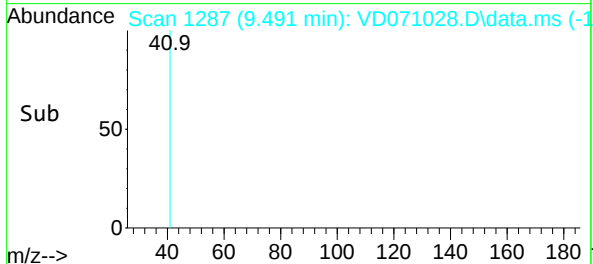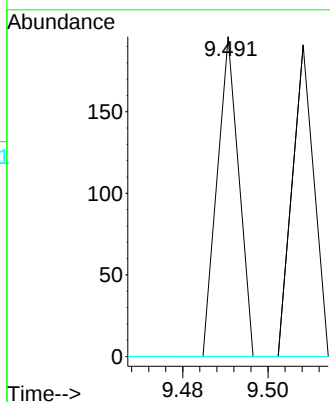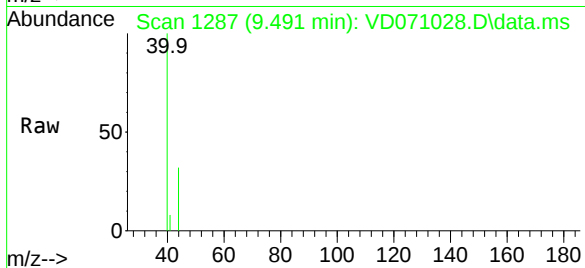

#50

Toluene-d8

Concen: 56.715 ug/l

RT: 10.332 min Scan# 1430

Delta R.T. -0.006 min

Lab File: VD071028.D




Acq: 15 Nov 2021 14:49


Tgt Ion: 98 Resp: 3859

Ion Ratio Lower Upper

98 100


100 62.0 51.8 77.6

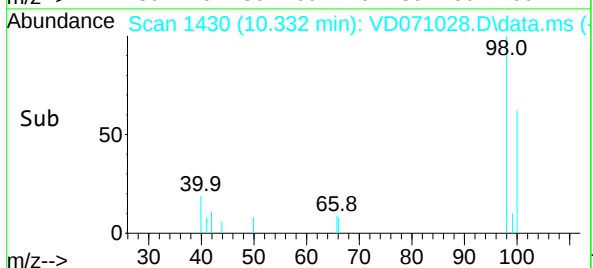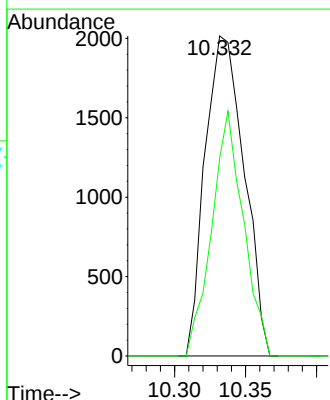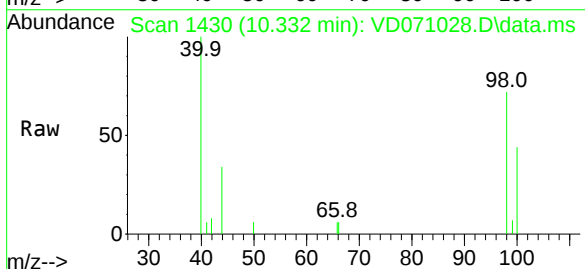






#51
4-Methyl-2-Pentanone
Concen: 5.284 ug/l
RT: 10.244 min Scan# 1411
Delta R.T. 0.024 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Instrument :
MSVOA_D
ClientSampleId :



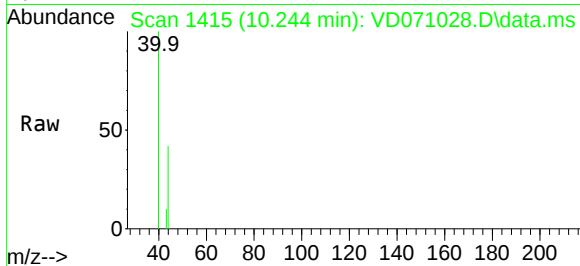



Tgt Ion: 43 Resp: 68
Ion Ratio Lower Upper
43 100
58 0.0 33.1 49.7#

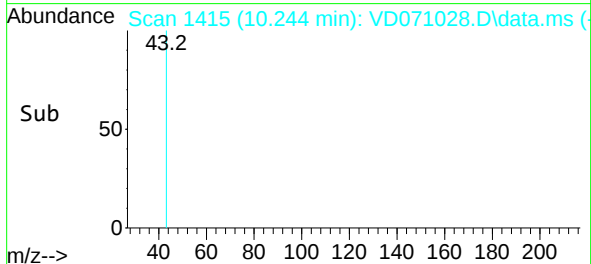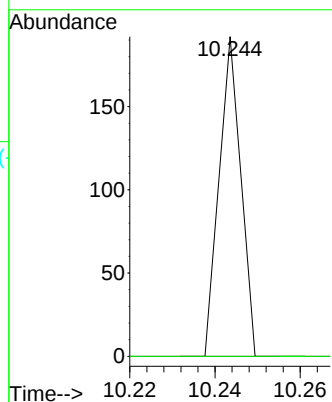

#55
1,1,2-Trichloroethane
Concen: 4.965 ug/l
RT: 10.791 min Scan# 1508
Delta R.T. -0.000 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion: 97 Resp: 68
Ion Ratio Lower Upper
97 100
83 0.0 65.2 97.8#
85 0.0 43.4 65.0#
99 0.0 52.1 78.1#


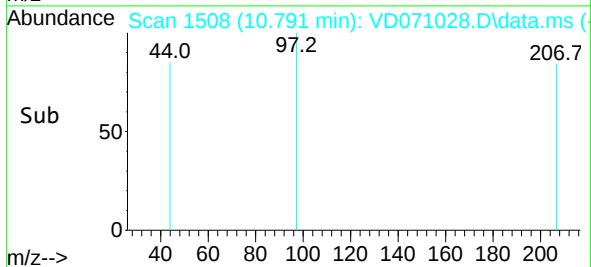

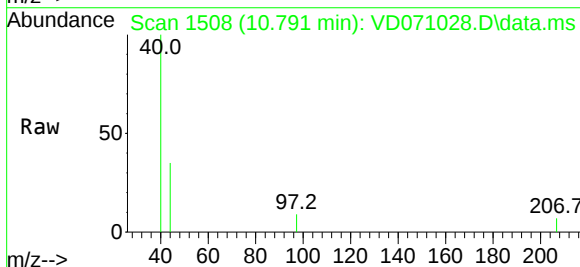




#59
2-Hexanone
Concen: 22.261 ug/l
RT: 11.020 min Scan# 11
Delta R.T. 0.041 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 68
Ion Ratio Lower Upper
43 100
58 0.0 28.7 86.1#

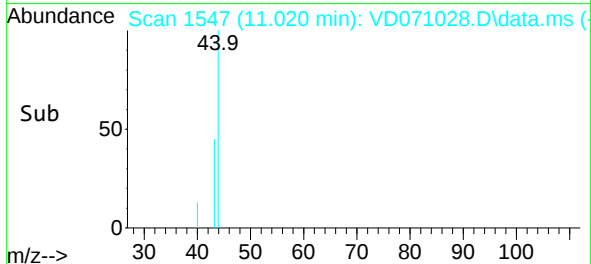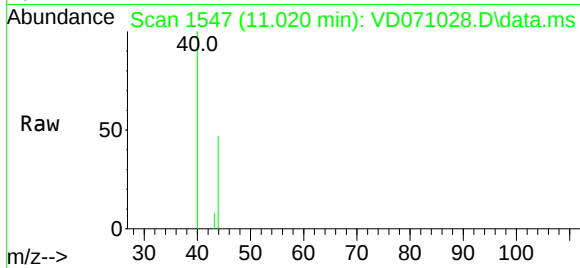

#62
4-Bromofluorobenzene
Concen: 48.165 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion: 95 Resp: 1180
Ion Ratio Lower Upper
95 100
174 46.4 0.0 159.4
176 39.7 0.0 154.0

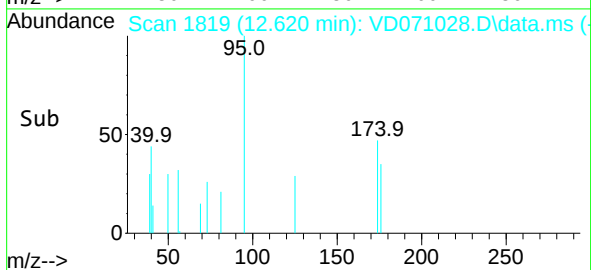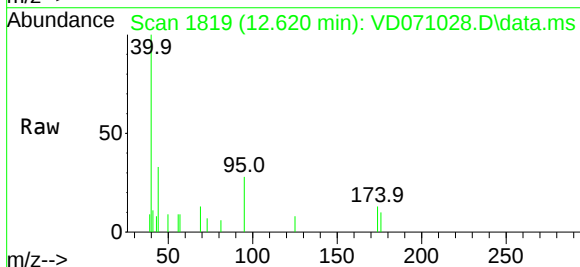



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.643 min Scan# 11

Delta R.T. 0.005 min


Lab File: VD071028.D

Acq: 15 Nov 2021 14:49

Instrument :

MSVOA_D

ClientSampleId :






Tgt Ion:117 Resp: 2181

Ion Ratio Lower Upper

117 100

82 61.7 44.7 67.1

119 38.9 26.2 39.4

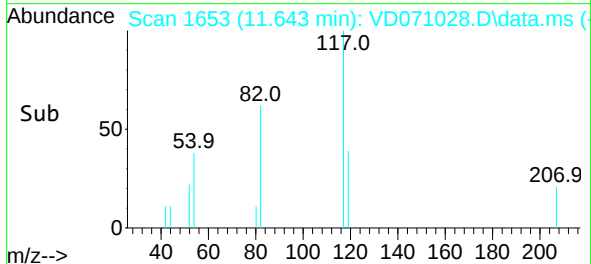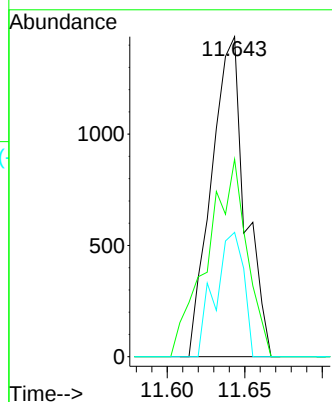

#68

m/p-Xylenes

Concen: 2.142 ug/l

RT: 12.049 min Scan# 1722

Delta R.T. 0.205 min

Lab File: VD071028.D




Acq: 15 Nov 2021 14:49


Tgt Ion:106 Resp: 59

Ion Ratio Lower Upper

106 100

91 0.0 160.1 240.1#


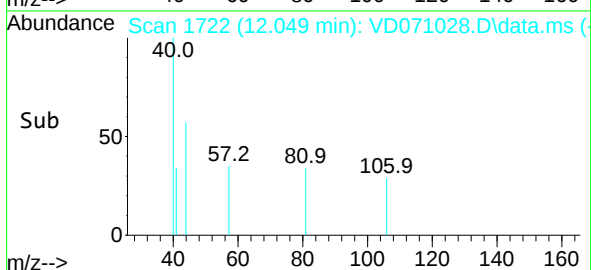






#69
o-Xylene
Concen: 2.252 ug/l
RT: 12.049 min Scan# 11
Delta R.T. -0.124 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:106 Resp: 59
Ion Ratio Lower Upper
106 100
91 0.0 106.3 319.0#

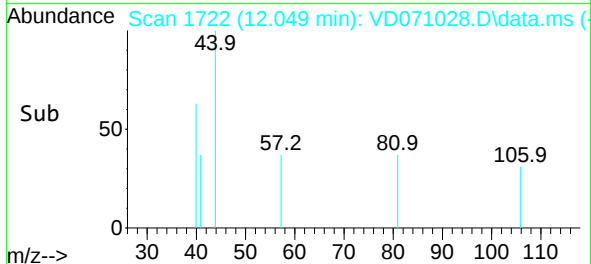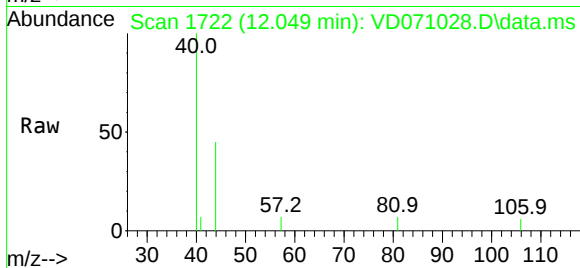

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.012 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49


Tgt Ion:152 Resp: 617
Ion Ratio Lower Upper
152 100
115 36.6 29.8 89.3
150 100.5 0.0 349.2

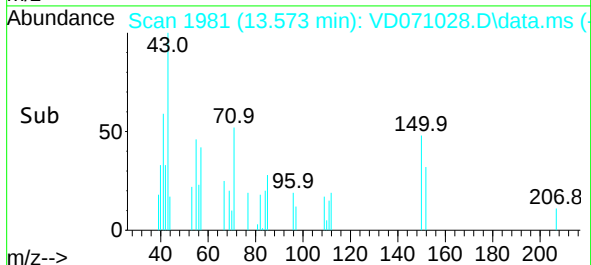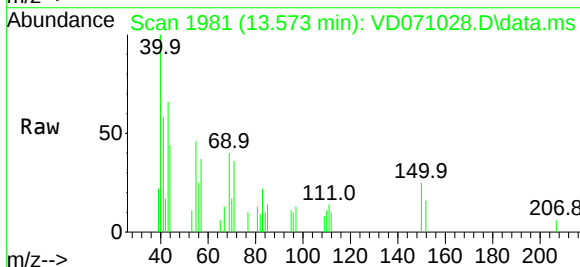



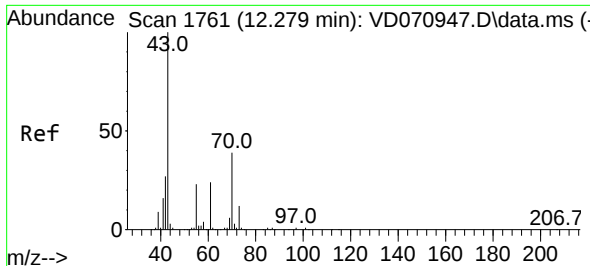


#74
N-amy1 acetate
Concen: 115.365 ug/l
RT: 12.261 min Scan# 1
Delta R.T. -0.018 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Instrument :
MSVOA_D
ClientSampleId :



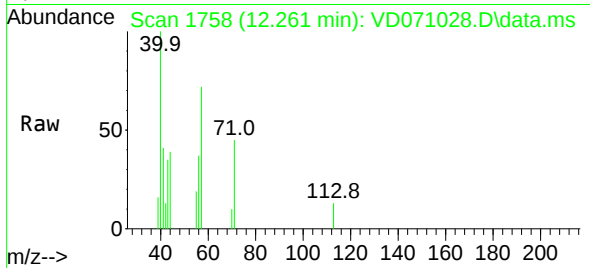



Tgt Ion: 43 Resp: 1465
Ion Ratio Lower Upper
43 100
70 21.7 36.6 55.0#
55 53.0 22.5 33.7#
61 0.0 20.5 30.7#

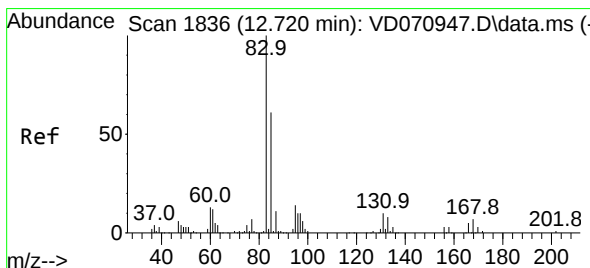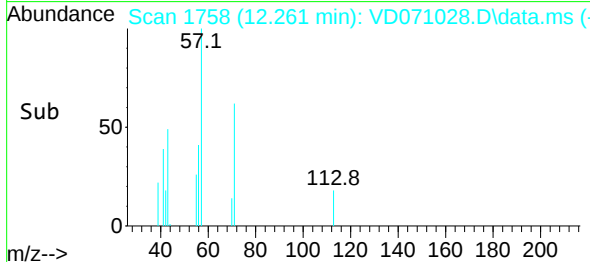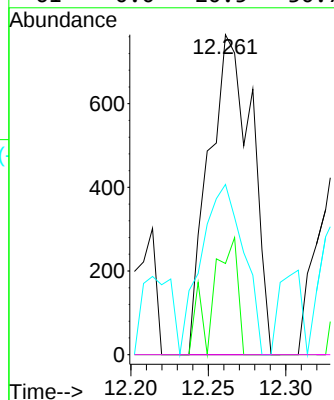

#75
1,1,2,2-Tetrachloroethane
Concen: 9.541 ug/l
RT: 12.690 min Scan# 1831
Delta R.T. -0.030 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion: 83 Resp: 73
Ion Ratio Lower Upper
83 100
131 0.0 4.9 14.7#
85 158.9 32.0 96.2#


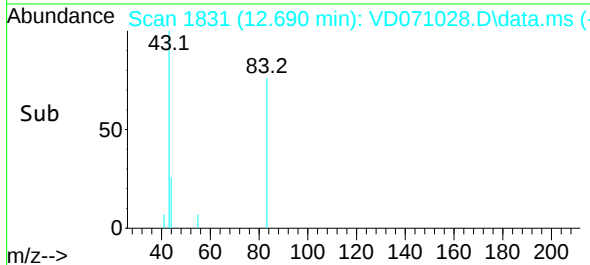
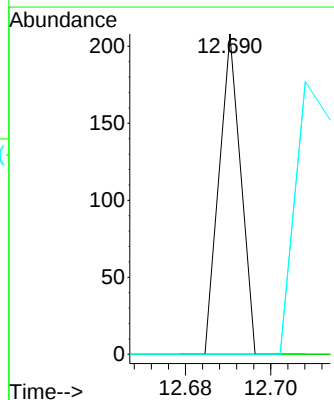
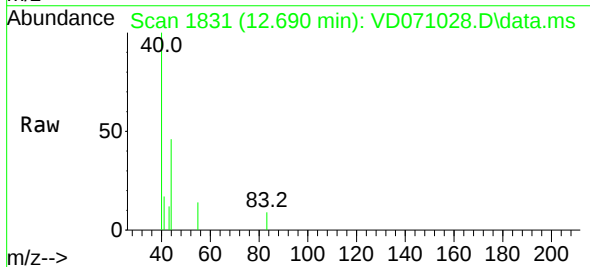




#76
1,2,3-Trichloropropane
Concen: 45.347 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.159 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 75 Resp: 239
Ion Ratio Lower Upper
75 100
77 0.0 158.4 475.3#

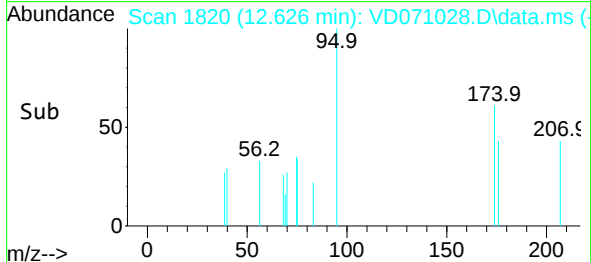

#77
Bromobenzene
Concen: 5.581 ug/l
RT: 12.937 min Scan# 1873
Delta R.T. 0.188 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion:156 Resp: 53
Ion Ratio Lower Upper
156 100
77 200.0 96.6 289.8
158 0.0 49.1 147.4#


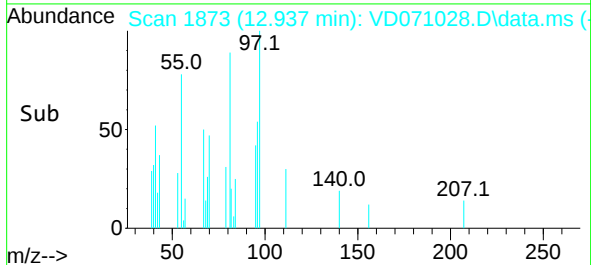

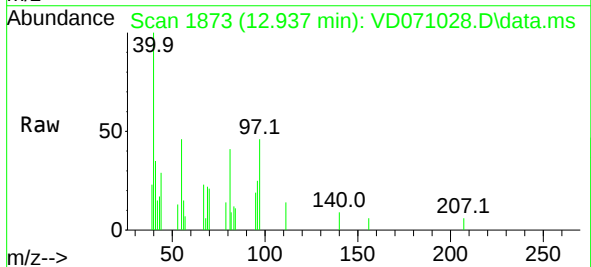




#78
n-propylbenzene
Concen: 5.156 ug/l
RT: 12.820 min Scan# 1853
Delta R.T. 0.012 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 91 Resp: 284
Ion Ratio Lower Upper
91 100
120 0.0 10.9 32.9#

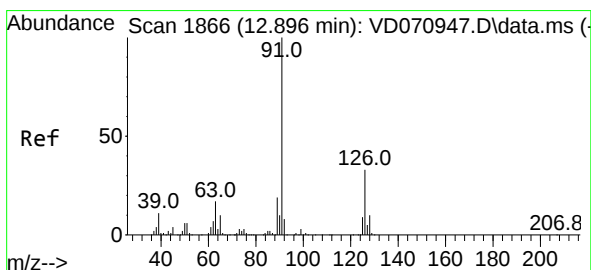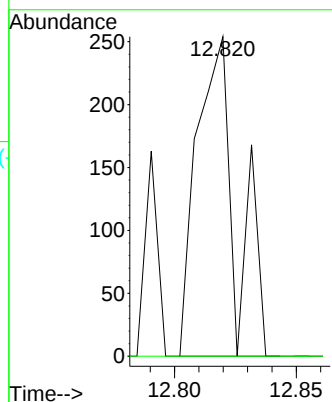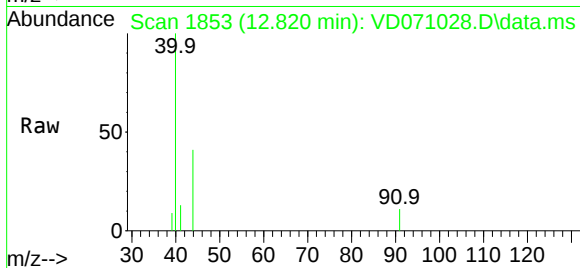

#79
2-Chlorotoluene
Concen: 2.070 ug/l
RT: 12.873 min Scan# 1862
Delta R.T. -0.023 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49


Tgt Ion: 91 Resp: 65
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.7#

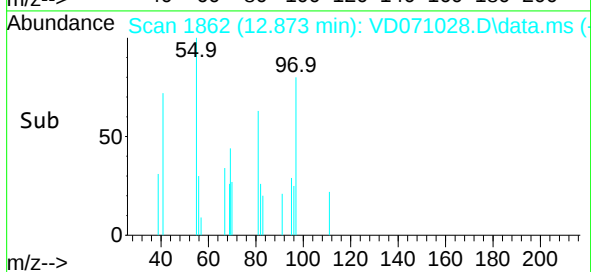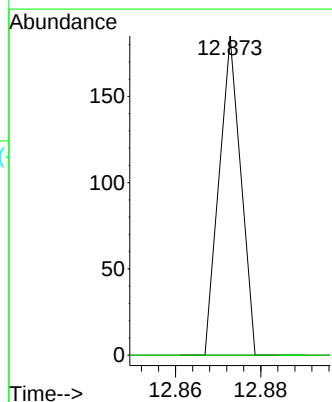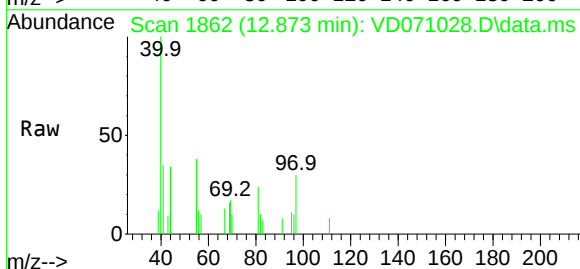






#80
 1,3,5-Trimethylbenzene
 Concen: 1.475 ug/l
 RT: 12.914 min Scan# 1869
 Delta R.T. -0.035 min
 Lab File: VD071028.D
 Acq: 15 Nov 2021 14:49

Instrument :
 MSVOA_D
 ClientSampleId :



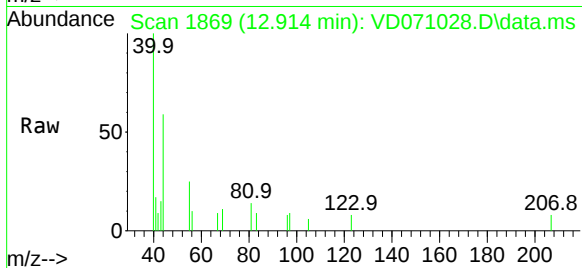



Tgt Ion:105 Resp: 54
 Ion Ratio Lower Upper
 105 100
 120 0.0 24.6 73.8#

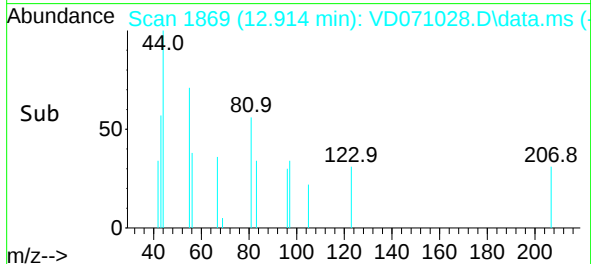

#81
 trans-1,4-Dichloro-2-butene
 Concen: 84.847 ug/l
 RT: 12.626 min Scan# 1820
 Delta R.T. 0.112 min
 Lab File: VD071028.D
 Acq: 15 Nov 2021 14:49

Tgt Ion: 75 Resp: 239
 Ion Ratio Lower Upper
 75 100
 53 0.0 62.6 94.0#
 89 0.0 34.5 51.7#


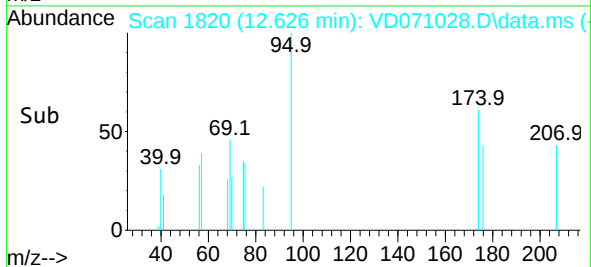

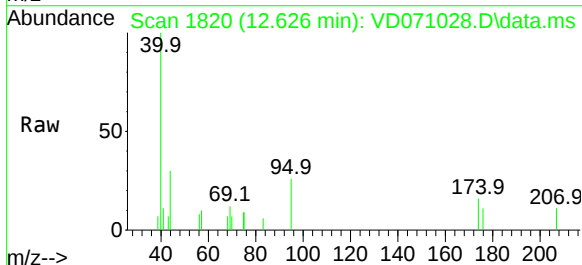




#82
4-Chlorotoluene
Concen: 2.098 ug/l
RT: 12.949 min Scan# 11
Delta R.T. -0.047 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 91 Resp: 68
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.1#

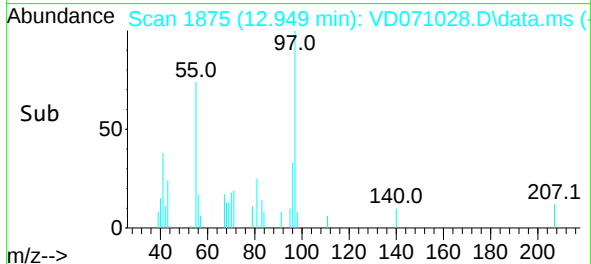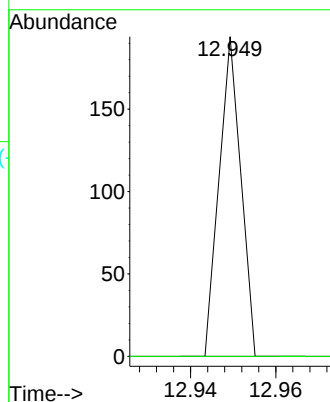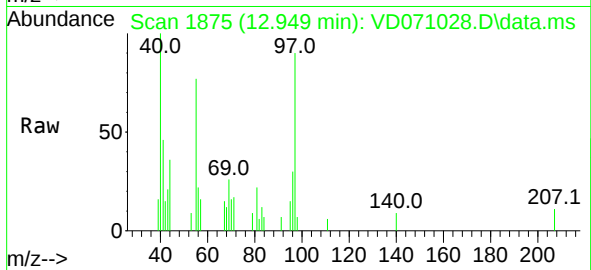

#83
tert-Butylbenzene
Concen: 1.745 ug/l
RT: 13.220 min Scan# 1921
Delta R.T. 0.012 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion: 119 Resp: 55
Ion Ratio Lower Upper
119 100
91 100.0 32.5 97.5#
134 0.0 13.2 39.6#


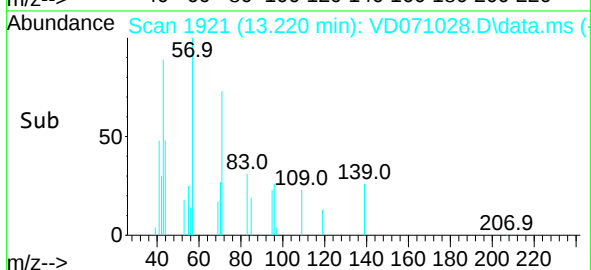
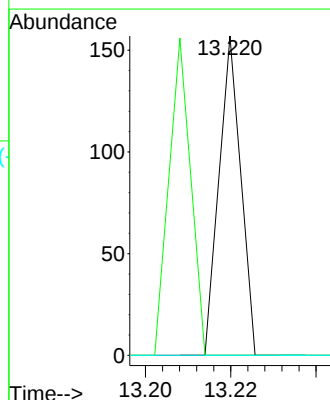
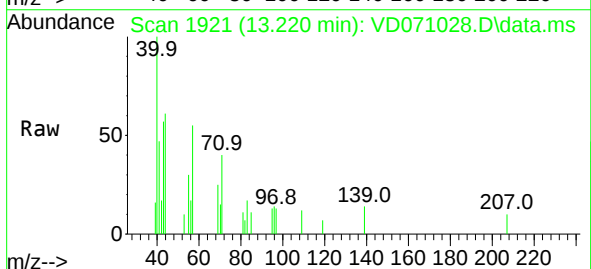




#84
1,2,4-Trimethylbenzene
Concen: 68.774 ug/l
RT: 13.390 min Scan# 1927
Delta R.T. 0.135 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:105 Resp: 2465
Ion Ratio Lower Upper
105 100
120 0.0 22.9 68.7#

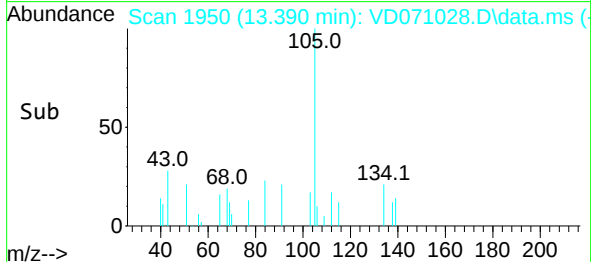

#85
sec-Butylbenzene
Concen: 52.008 ug/l
RT: 13.390 min Scan# 1950
Delta R.T. -0.001 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion:105 Resp: 2465
Ion Ratio Lower Upper
105 100
134 15.8 9.7 28.9


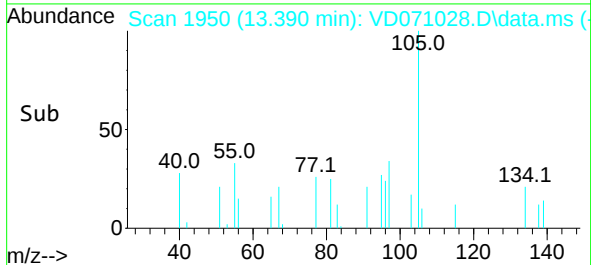

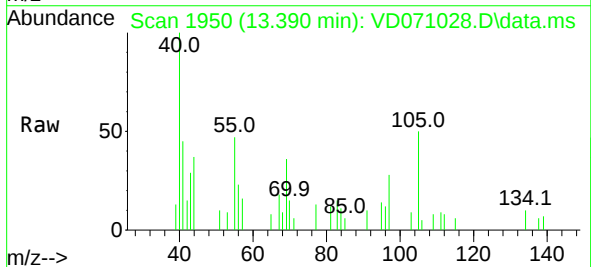


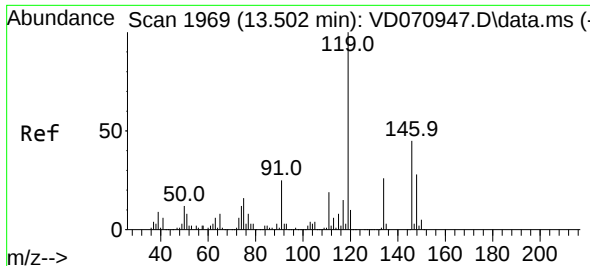

#86
p-Isopropyltoluene
Concen: 22.518 ug/l
RT: 13.502 min Scan# 1969
Delta R.T. 0.000 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:119 Resp: 857
Ion Ratio Lower Upper
119 100
134 9.2 13.0 38.9#
91 42.2 11.4 34.2#

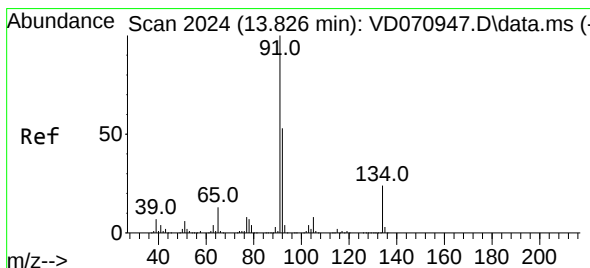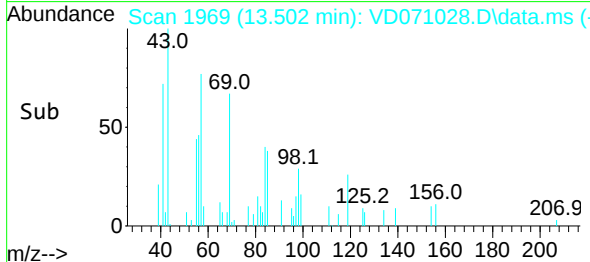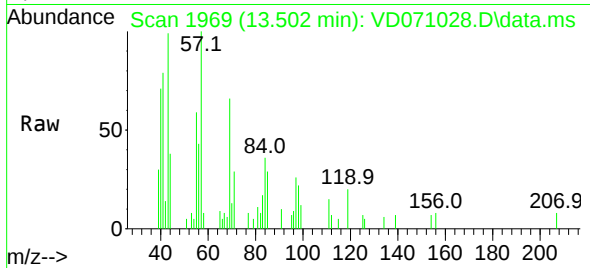

#89
n-Butylbenzene
Concen: 34.538 ug/l
RT: 13.826 min Scan# 2024
Delta R.T. -0.000 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Tgt Ion: 91 Resp: 1321
Ion Ratio Lower Upper
91 100
92 11.4 27.3 81.9#
134 17.9 12.3 36.9

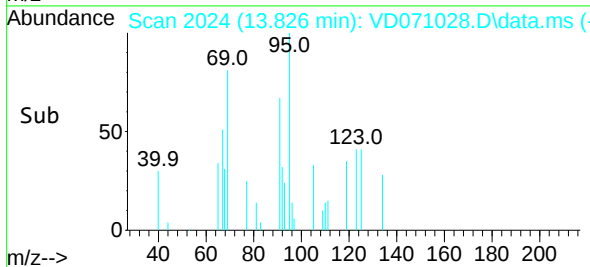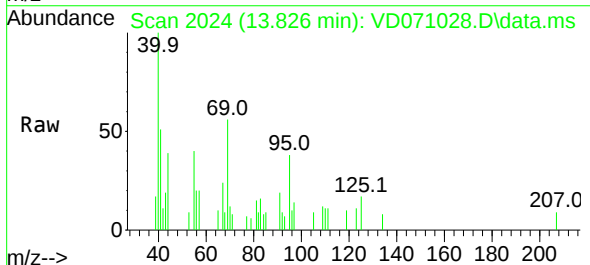



#90
Hexachloroethane
Concen: 19.519 ug/l
RT: 14.090 min Scan# 20
Delta R.T. -0.006 min
Lab File: VD071028.D
Acq: 15 Nov 2021 14:49

Instrument :
MSVOA_D
ClientSampleId :

Tgt Ion:117 Resp: 147
Ion Ratio Lower Upper
117 100
201 0.0 36.0 108.1#

