
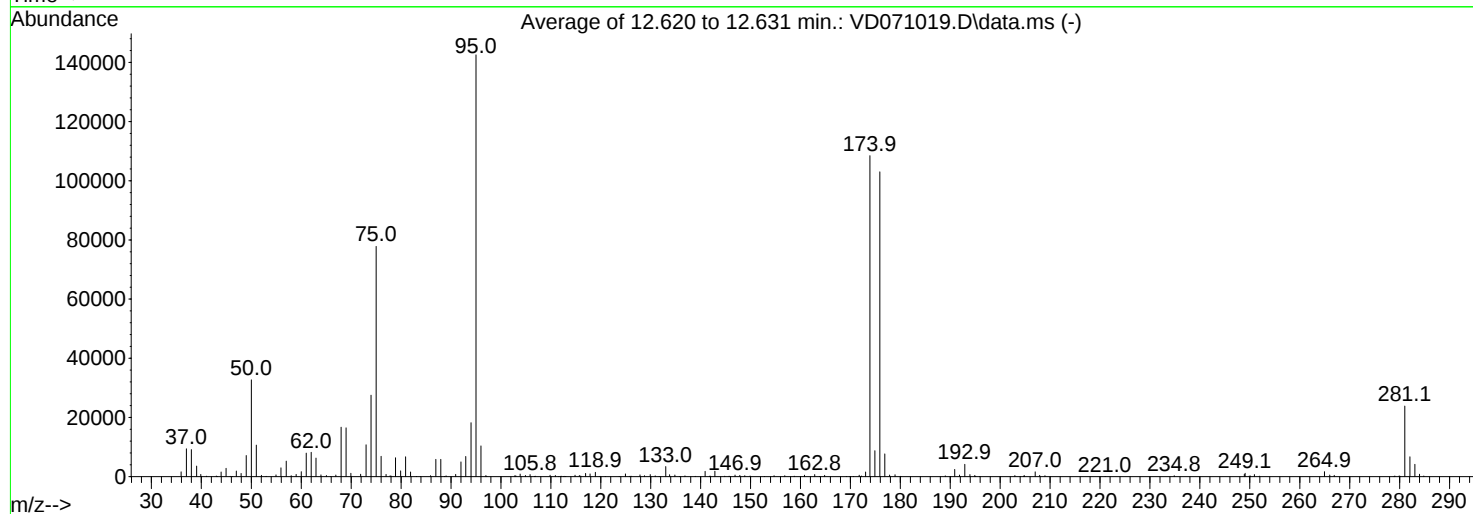


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111521\
Data File : VD071019.D
Acq On : 15 Nov 2021 09:50
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
Title : SW846 8260
Last Update : Wed Nov 10 03:55:51 2021

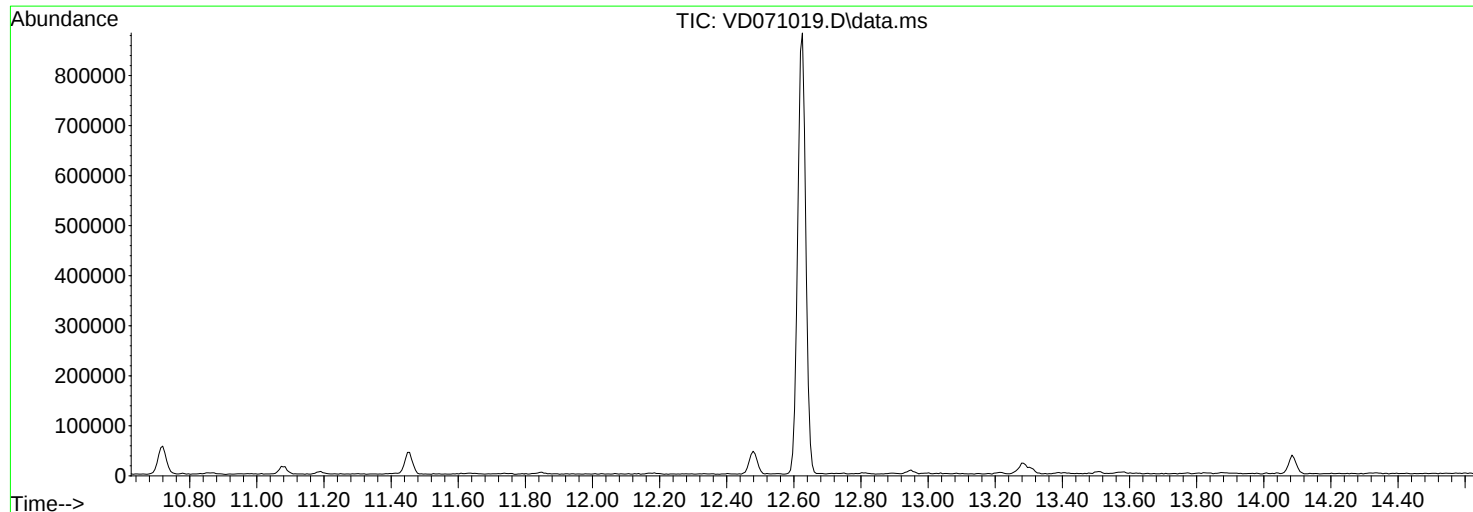

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	32704	PASS
75	95	30	60	54.6	77821	PASS
95	95	100	100	100.0	142555	PASS
96	95	5	9	7.3	10368	PASS
173	174	0.00	2	1.5	1593	PASS
174	95	50	100	76.1	108480	PASS
175	174	5	9	8.1	8763	PASS
176	174	95	101	95.0	103019	PASS
177	176	5	9	7.5	7686	PASS