


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111523\
Data File : VD077573.D
Acq On : 15 Nov 2023 08:07
Operator : JC/SY
Sample : BFB178
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB178

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Title : SFAM01.0
Last Update : Fri Nov 10 02:07:44 2023

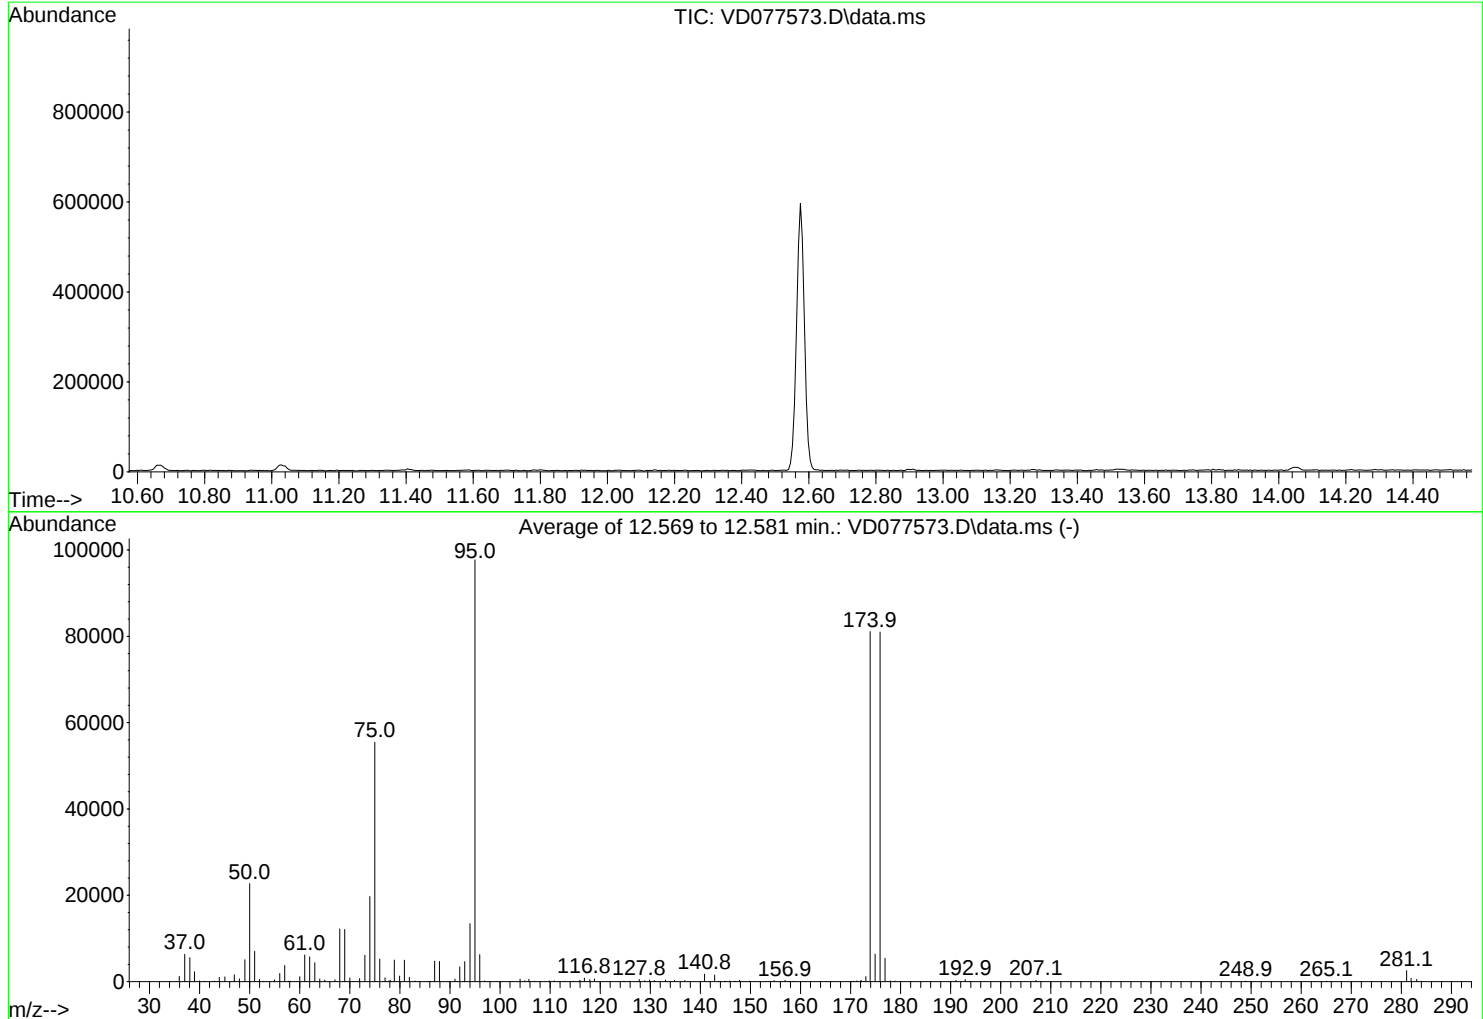

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.3	22720	PASS
75	95	30	80	56.8	55452	PASS
95	95	100	100	100.0	97712	PASS
96	95	5	9	6.4	6255	PASS
173	174	0.00	2	1.5	1197	PASS
174	95	50	120	83.0	81112	PASS
175	174	5	9	7.9	6389	PASS
176	174	95	105	99.8	80989	PASS
177	176	5	10	6.7	5398	PASS

m/z	Abundance
35.50	186.0
36.70	180.0
37.40	161.0
39.00	193.0
39.90	1708.0
44.10	850.0
50.50	178.0
75.20	161.0
95.80	161.0
206.80	158.0

Instrument :
MSVOA_D
ClientSampleId :
BFB178

m/z	Abundance
35.90	968.0
37.10	5761.0
38.00	5278.0
39.00	2220.0
39.90	1969.0
40.90	218.0
42.70	205.0
43.10	167.0
43.90	1825.0
45.10	1230.0
46.90	1753.0
47.90	577.0
49.00	4938.0
50.00	21648.0
51.00	6883.0
52.00	430.0
52.80	194.0
55.00	371.0
56.00	2264.0
57.00	3527.0
57.80	195.0
60.00	853.0
61.00	6178.0
62.00	5822.0
63.00	4275.0
64.00	709.0
65.00	351.0
67.10	521.0
68.00	11703.0
69.00	11742.0
70.00	838.0
72.00	729.0
73.00	5366.0
74.00	19784.0
75.00	52576.0
76.00	4691.0
77.00	728.0
78.10	589.0
78.90	5140.0
79.90	1515.0
80.90	4412.0
81.90	862.0
83.00	214.0
85.70	181.0
87.00	4236.0
87.90	4219.0
91.00	490.0
91.90	3393.0
92.90	4249.0
94.00	12349.0
95.00	94600.0
96.00	5657.0
96.90	287.0
104.00	644.0
104.90	259.0
105.70	456.0
110.80	159.0
115.80	390.0
116.90	802.0
117.90	407.0
118.90	615.0
127.80	432.0
129.00	224.0
129.80	268.0
130.80	277.0
133.00	342.0
134.80	293.0
136.90	306.0
140.90	1535.0
142.80	1582.0
147.00	189.0
147.80	398.0
153.00	154.0
154.70	194.0
156.90	210.0
172.00	382.0
173.90	73472.0
174.90	5890.0
175.90	71464.0
176.90	5006.0
177.90	209.0
179.00	255.0
191.00	210.0
193.00	460.0
207.00	338.0
248.90	208.0
281.00	1966.0
281.90	777.0
283.00	348.0

Instrument :
MSVOA_D
ClientSampleId :
BFB178

m/z	Abundance
36.00	1493.0
37.00	7145.0
38.10	6229.0
39.00	2952.0
40.00	1937.0
42.90	168.0
44.00	1848.0
45.00	1226.0
46.90	1721.0
48.00	755.0
49.10	5739.0
50.00	23992.0
51.00	7555.0
51.90	535.0
54.90	445.0
55.90	1690.0
57.00	3781.0
58.20	292.0
60.00	1481.0
61.00	6785.0
62.00	5588.0
63.00	4954.0
64.00	515.0
65.00	581.0
67.10	354.0
68.00	13596.0
69.00	12523.0
70.00	819.0
72.00	806.0
73.00	6987.0
74.00	21888.0
75.00	61464.0
76.00	6216.0
77.00	1014.0
78.10	372.0
78.90	5332.0
80.00	1509.0
80.90	5610.0
81.90	1104.0
86.90	5470.0
87.90	5147.0
90.90	742.0
92.00	4092.0
93.00	5884.0
94.00	14623.0
95.00	107040.0
96.00	7873.0
104.00	618.0
105.00	254.0
105.80	542.0
106.80	206.0
109.90	355.0
110.90	238.0
112.90	202.0
114.80	231.0
116.00	614.0
116.80	943.0
117.90	611.0
118.80	745.0
124.60	225.0
125.80	152.0
127.80	400.0
128.90	208.0
129.90	350.0
130.80	260.0
133.00	341.0
133.80	166.0
134.80	160.0
136.80	300.0
140.90	1622.0
141.90	246.0
142.90	1603.0
143.70	179.0
144.80	240.0
145.90	290.0
146.90	171.0
147.80	407.0
149.90	219.0
154.70	385.0
156.90	326.0
157.80	225.0
158.60	263.0
165.20	162.0
170.10	225.0
170.60	242.0
171.30	291.0
172.20	650.0
173.10	1865.0
173.90	90840.0
174.90	6805.0
175.90	90456.0
176.90	5987.0

Instrument :
MSVOA_D
ClientSampleId :
BFB178

178.80	161.0
191.10	311.0
192.90	409.0
207.10	165.0
281.10	2474.0
282.00	858.0
283.10	625.0
284.00	227.0

Instrument :
MSVOA_D
ClientSampleId :
BFB178

m/z	Abundance
36.00	1206.0
37.00	6161.0
38.00	5209.0
39.00	2270.0
40.10	1755.0
44.00	1845.0
45.00	893.0
47.00	1310.0
47.90	553.0
49.00	4591.0
50.00	22520.0
51.00	6659.0
51.90	588.0
54.90	382.0
56.10	1748.0
57.00	3883.0
57.80	153.0
60.00	1148.0
61.00	5601.0
62.00	5780.0
63.00	3908.0
64.00	654.0
64.90	200.0
67.00	470.0
68.00	11267.0
69.00	11977.0
70.00	950.0
70.70	171.0
71.90	569.0
73.00	5967.0
74.00	17528.0
75.00	52800.0
76.00	4833.0
77.10	944.0
77.80	527.0
78.90	4495.0
80.00	829.0
80.90	4915.0
81.90	1039.0
83.10	199.0
86.10	180.0
86.90	4532.0
87.90	4687.0
91.10	550.0
92.00	2784.0
93.00	3797.0
94.00	13439.0
95.00	91496.0
96.00	5717.0
96.90	325.0
104.00	516.0
104.90	195.0
105.70	656.0
106.90	181.0
109.70	195.0
110.90	184.0
114.60	160.0
115.90	452.0
116.90	723.0
118.00	408.0
118.90	567.0
124.90	204.0
125.80	164.0
127.80	632.0
128.80	198.0
129.90	463.0
130.80	205.0
133.10	392.0
134.90	350.0
137.00	156.0
140.80	2125.0
142.90	1357.0
145.00	190.0
145.90	229.0
147.80	178.0
149.90	177.0
154.80	219.0
156.90	308.0
171.20	217.0
171.80	225.0
173.00	1726.0
173.90	79024.0
174.90	6473.0
175.90	81048.0
176.90	5200.0
177.90	335.0
191.10	360.0
192.80	575.0
193.80	199.0
207.00	422.0
249.00	158.0
265.10	342.0

Instrument :
MSVOA_D
ClientSampleId :
BFB178

281.10	3298.0
282.00	759.0
283.10	555.0
284.10	151.0

Instrument :
MSVOA_D
ClientSampleId :
BFB178