


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111618\
 Data File : VD060389.D
 Acq On : 16 Nov 2018 10:17
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Title : SW846 8260
 Last Update : Tue Nov 06 13:56:04 2018

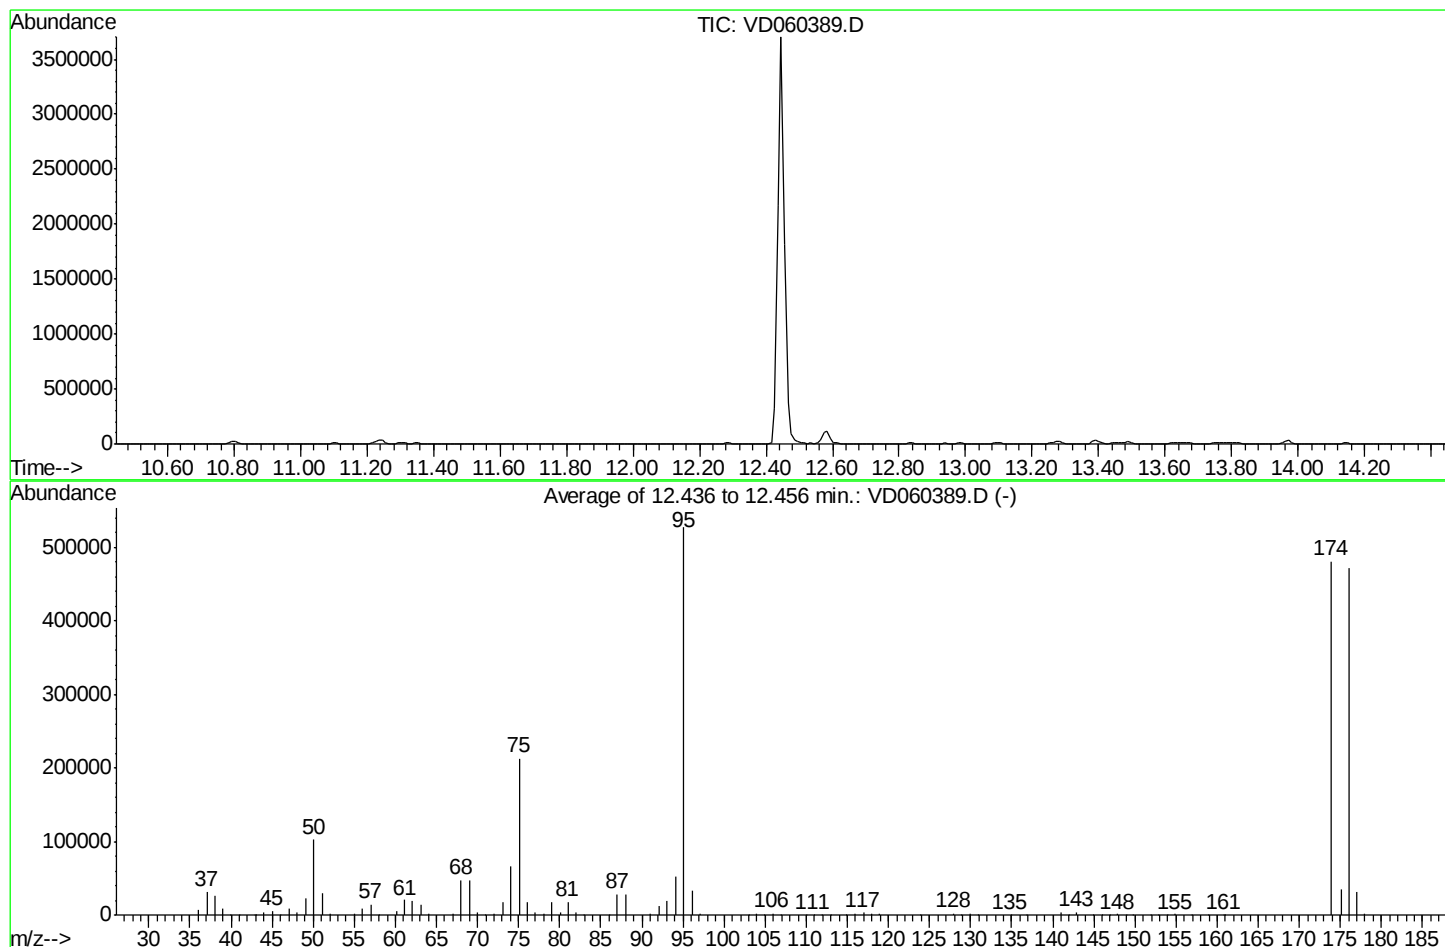

AutoFind: Scans 1109, 1110, 1111; Background Corrected with Scan 1104

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	102157	PASS
75	95	30	60	40.3	212578	PASS
95	95	100	100	100.0	527146	PASS
96	95	5	9	6.2	32706	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.3	481237	PASS
175	174	5	9	7.2	34490	PASS
176	174	95	101	98.2	472426	PASS
177	176	5	9	6.6	31277	PASS