



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111622\
Data File : VD074941.D
Acq On : 16 Nov 2022 09:25
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
Title : SW846 8260
Last Update : Mon Nov 14 00:51:58 2022

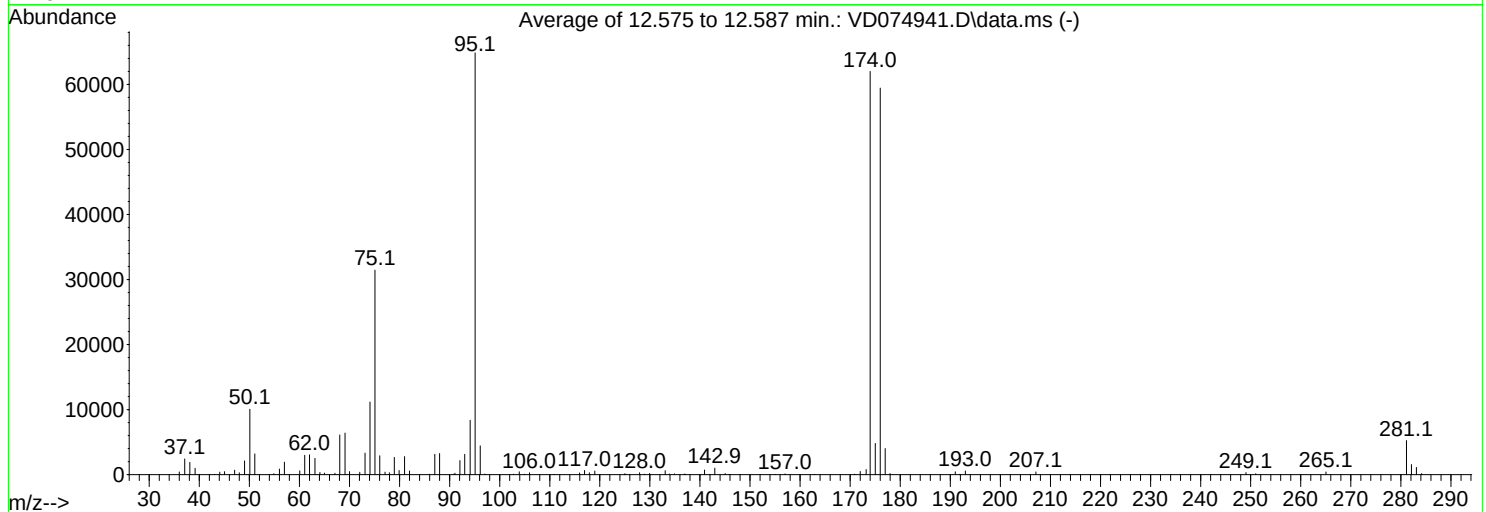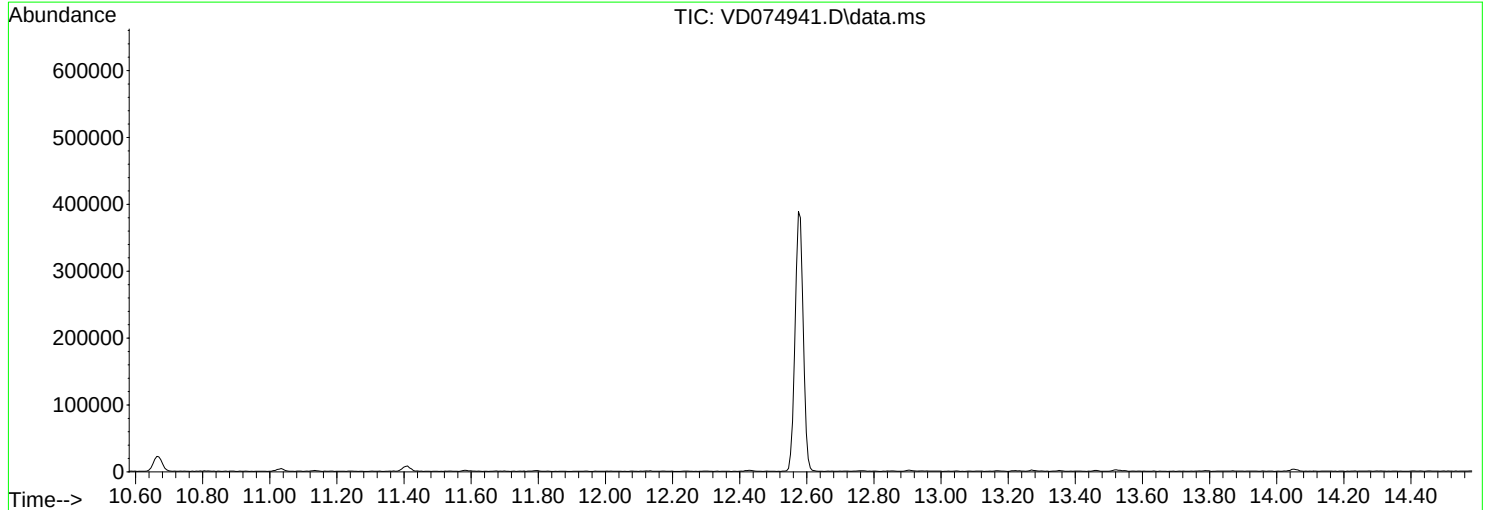

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	10057	PASS
75	95	30	60	48.5	31437	PASS
95	95	100	100	100.0	64856	PASS
96	95	5	9	6.8	4432	PASS
173	174	0.00	2	1.3	780	PASS
174	95	50	100	95.6	61989	PASS
175	174	5	9	7.8	4811	PASS
176	174	95	101	95.9	59435	PASS
177	176	5	9	6.8	4012	PASS