
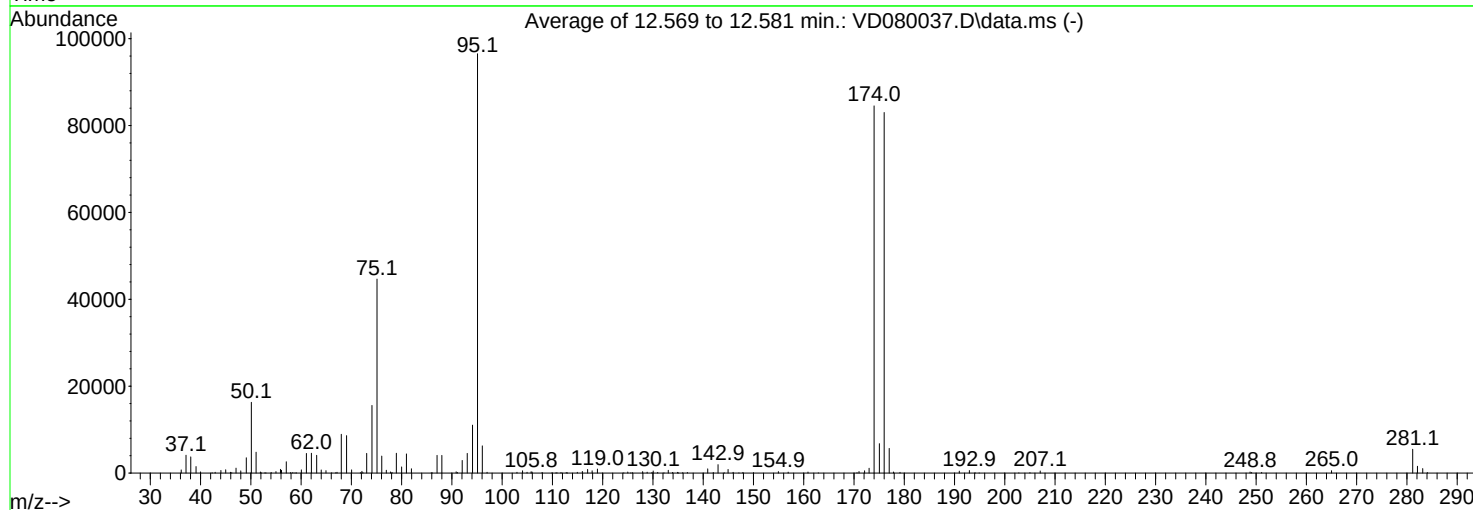


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111724\
Data File : VD080037.D
Acq On : 17 Nov 2024 11:29
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
Title : SW846 8260
Last Update : Fri Nov 15 16:25:47 2024

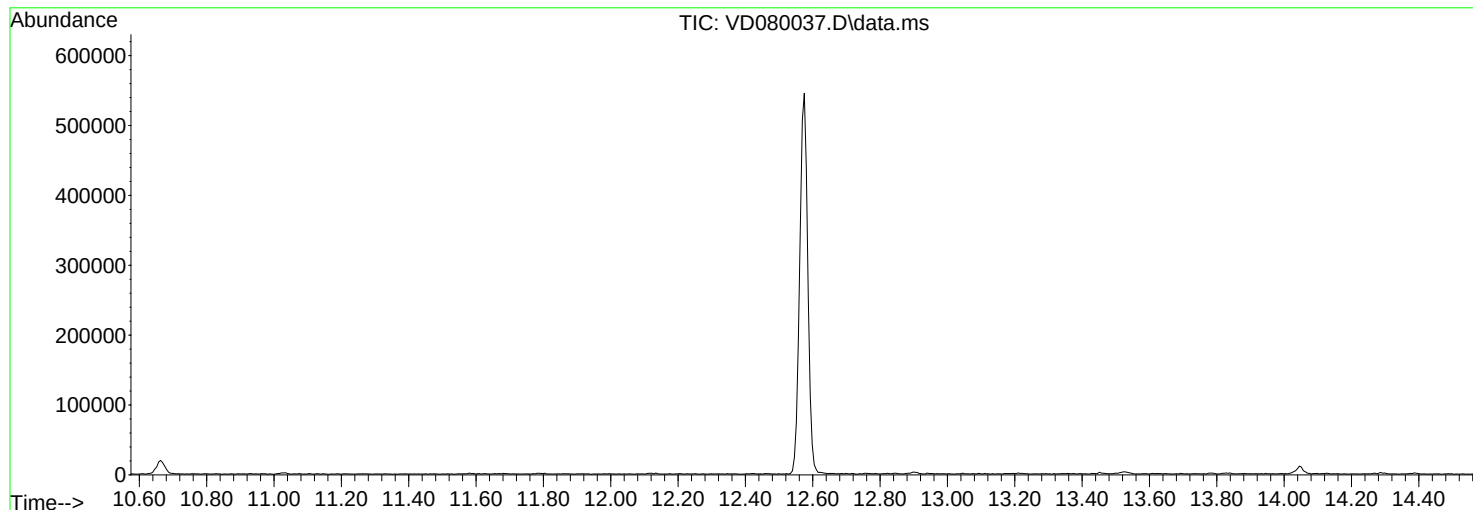

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	16292	PASS
75	95	30	60	46.3	44661	PASS
95	95	100	100	100.0	96536	PASS
96	95	5	9	6.5	6266	PASS
173	174	0.00	2	1.3	1122	PASS
174	95	50	100	87.6	84531	PASS
175	174	5	9	8.0	6776	PASS
176	174	95	101	98.2	83008	PASS
177	176	5	9	6.8	5678	PASS