


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111819\
Data File : VD064254.D
Acq On : 18 Nov 2019 09:52
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Title : SW846 8260
Last Update : Tue Nov 12 02:43:24 2019

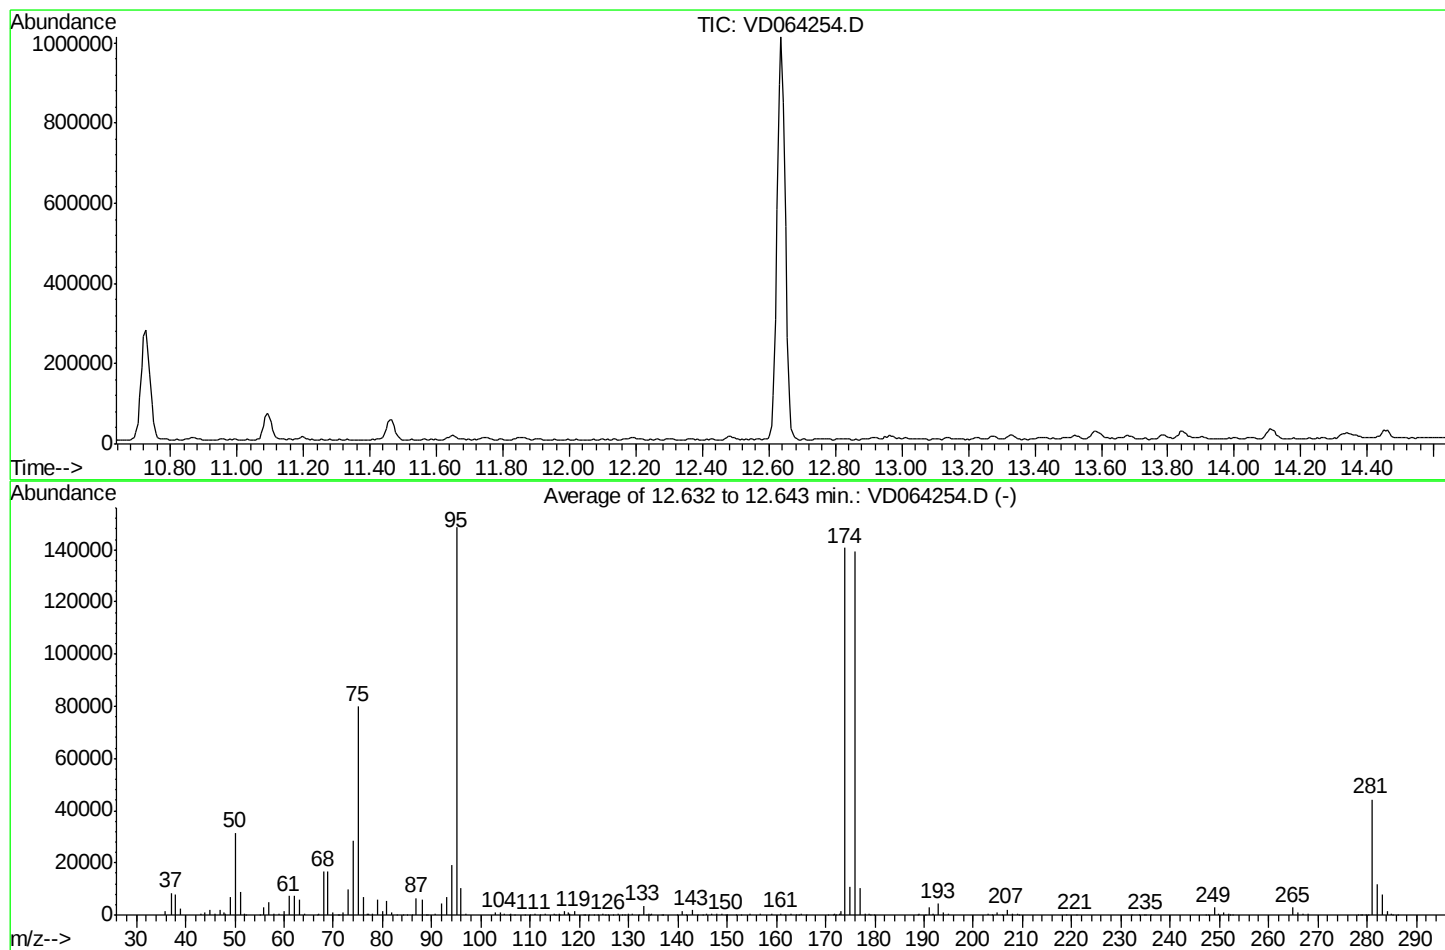

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	31466	PASS
75	95	30	60	53.8	79955	PASS
95	95	100	100	100.0	148608	PASS
96	95	5	9	6.8	10146	PASS
173	174	0.00	2	0.9	1334	PASS
174	95	50	100	94.7	140765	PASS
175	174	5	9	7.8	11035	PASS
176	174	95	101	98.8	139130	PASS
177	176	5	9	7.4	10241	PASS