


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111820\  
 Data File : VD067673.D  
 Acq On : 18 Nov 2020 09:10  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D110320S.M  
 Title : SW846 8260  
 Last Update : Wed Nov 04 00:56:28 2020

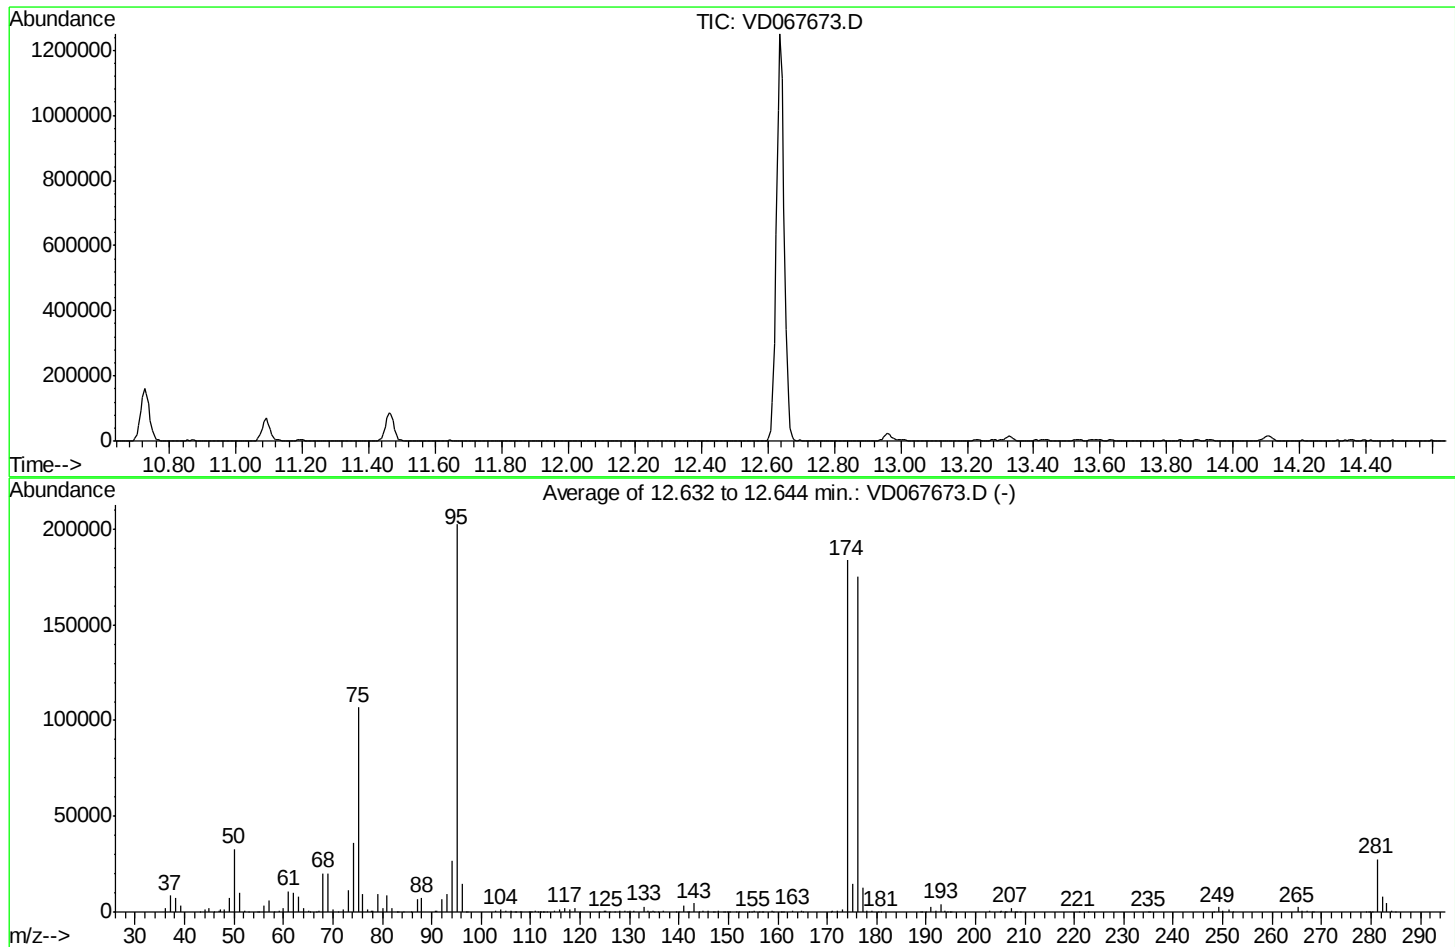

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.2      | 32794   | PASS             |
| 75          | 95           | 30           | 60           | 52.8      | 106941  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 202538  | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 14544   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.6       | 1136    | PASS             |
| 174         | 95           | 50           | 100          | 90.7      | 183786  | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 14664   | PASS             |
| 176         | 174          | 95           | 101          | 95.3      | 175189  | PASS             |
| 177         | 176          | 5            | 9            | 7.3       | 12876   | PASS             |