




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077623.D
 Acq On : 18 Nov 2023 11:43
 Operator : JC/SY
 Sample : 05416-22
 Misc : 3.16G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AH5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:23:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

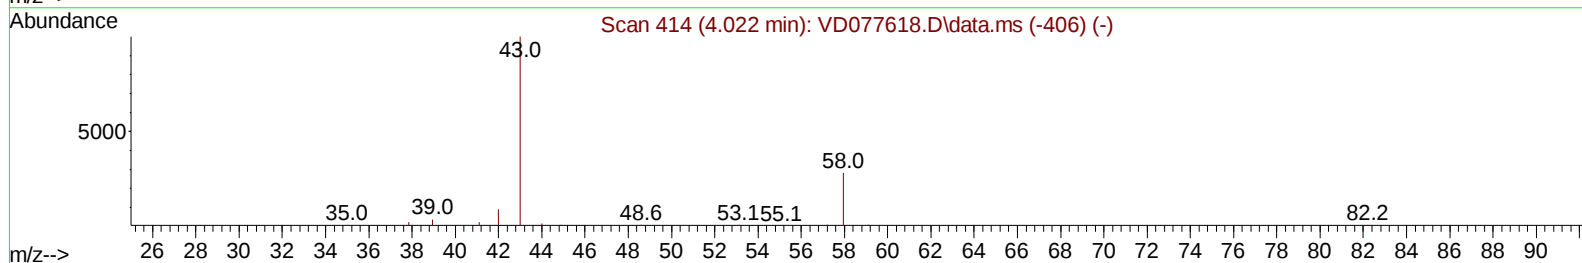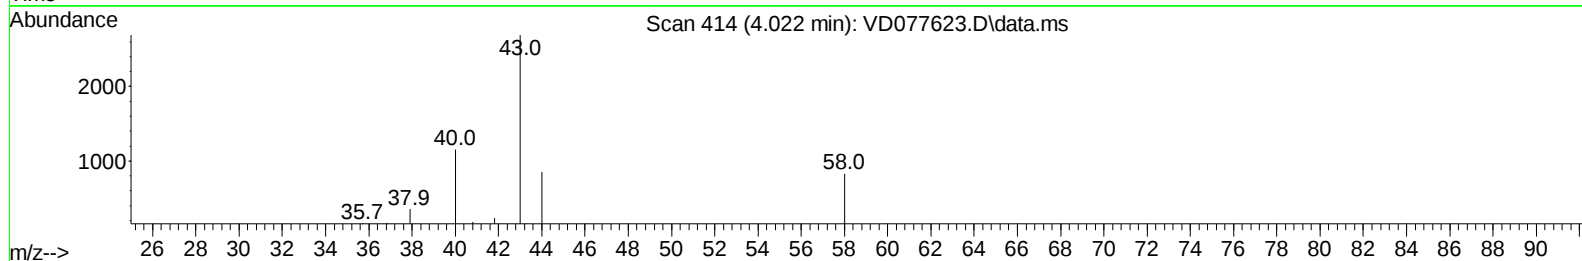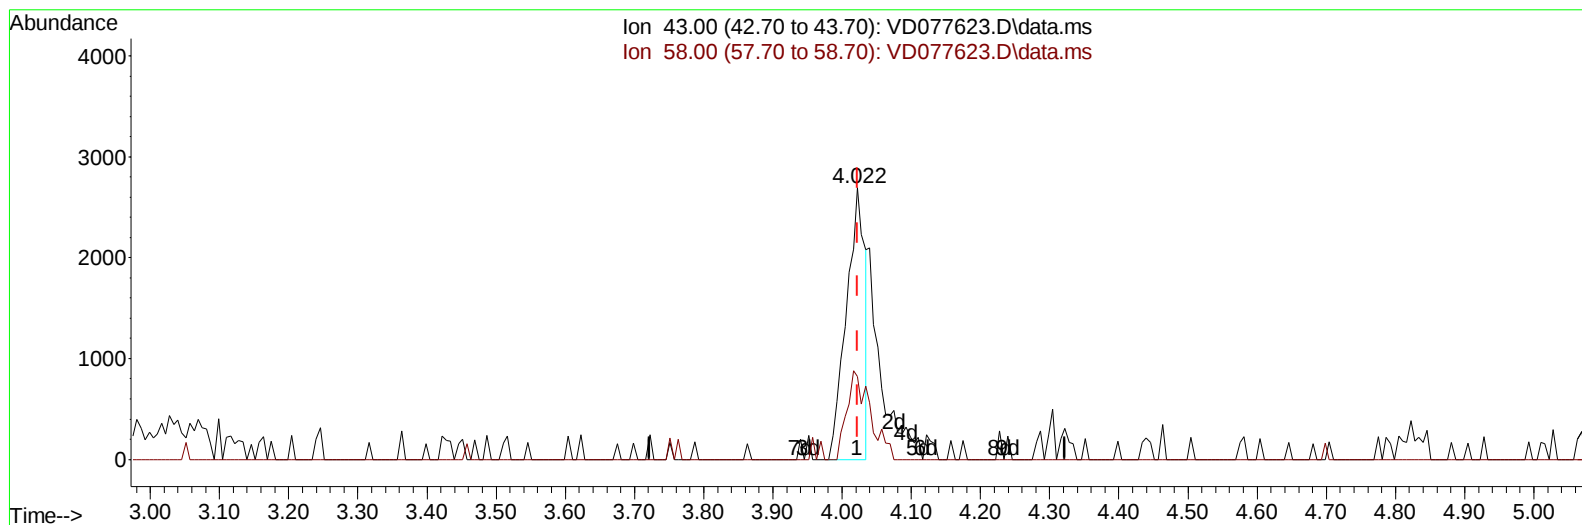

TIC: VD077623.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 4.53 ug/L

response 4961

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	24.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077623.D
 Acq On : 18 Nov 2023 11:43
 Operator : JC/SY
 Sample : 05416-22
 Misc : 3.16G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AH5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:23:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

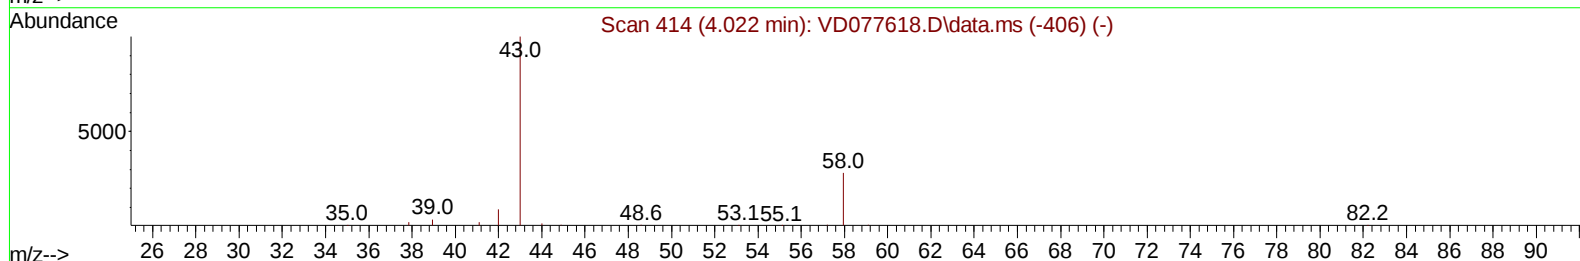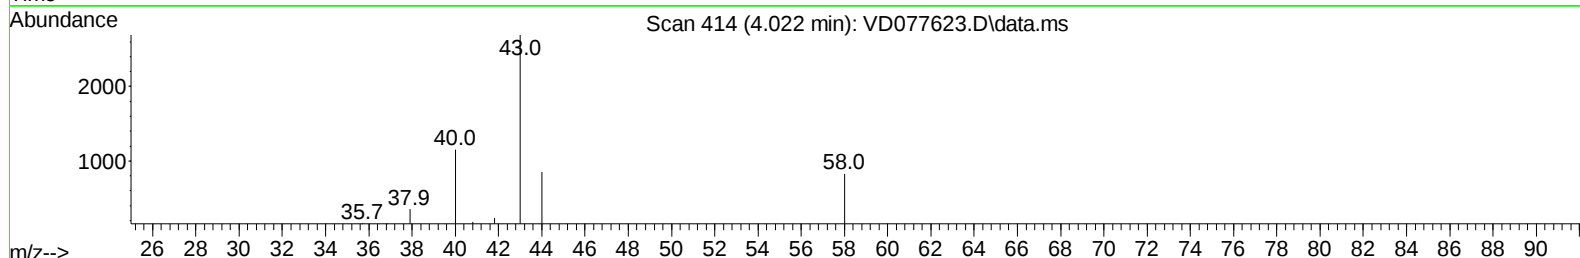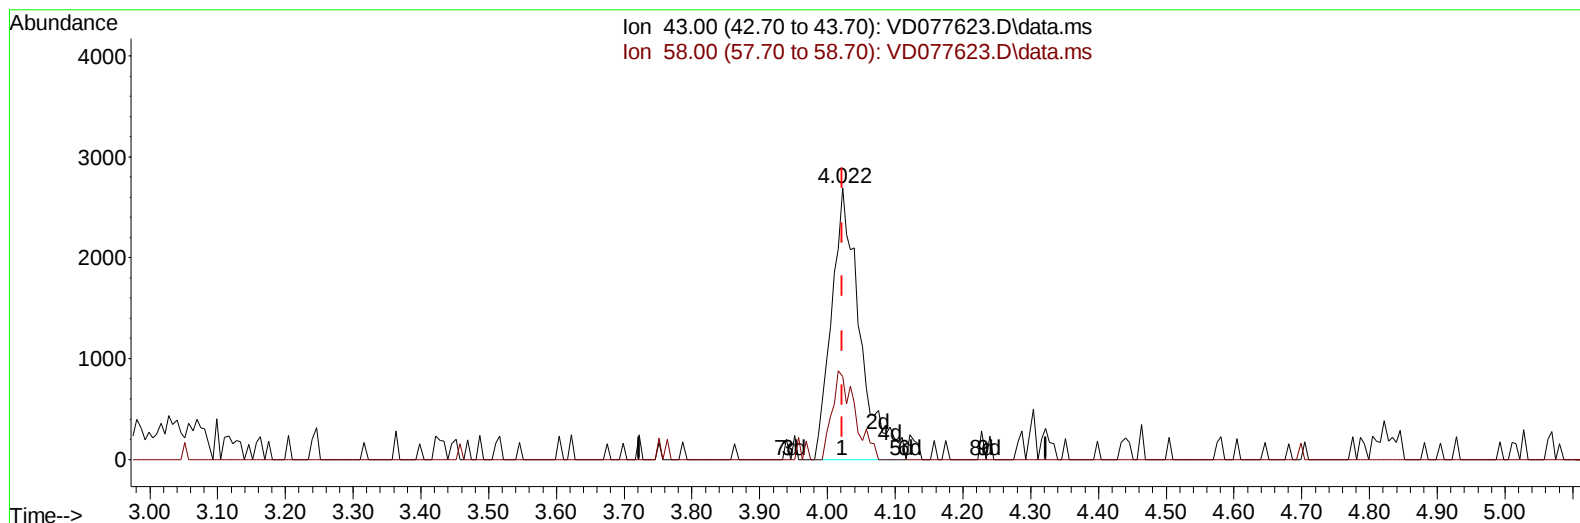

TIC: VD077623.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 7.12 ug/L m

response 7808

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	15.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077623.D
 Acq On : 18 Nov 2023 11:43
 Operator : JC/SY
 Sample : 05416-22
 Misc : 3.16G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AH5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:23:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		236791	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.580	117		227396	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		98287	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		91182	15.137	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	60.560%	
7) Chloroethane-d5	2.804	69		85987	18.171	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.680%	
11) 1,1-Dichloroethene-d2	3.916	65		28288	15.187	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	60.760%	
21) 2-Butanone-d5	6.981	46		61442	58.915	ug/L	-0.01
Spiked Amount 50.000	Range 20	- 135		Recovery	=	117.820%	
24) Chloroform-d	7.569	84		145609	21.287	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	85.160%	
26) 1,2-Dichloroethane-d4	8.228	65		93044	25.572	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	102.280%	
32) Benzene-d6	8.204	84		285934	19.374	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	77.480%	
36) 1,2-Dichloropropane-d6	9.210	67		104189	21.673	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	86.680%	
41) Toluene-d8	10.269	98		249099	18.678	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	74.720%	
43) trans-1,3-Dichloroprop...	10.528	79		45999	22.192	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	88.760%	
47) 2-Hexanone-d5	10.875	63		45647	53.079	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	106.160%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		80922	25.406	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	101.640%	
66) 1,2-Dichlorobenzene-d4	13.816	152		82020	23.457	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.840%	
Target Compounds							
13) Acetone	4.022	43		7808m	7.123	ug/L	
16) Methylene chloride	4.804	84		53194	13.305	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
Data File : VD077623.D
Acq On : 18 Nov 2023 11:43
Operator : JC/SY
Sample : 05416-22
Misc : 3.16G/10ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0AH5

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/20/2023
Supervised By :Mahesh Dadoda 11/20/2023

Quant Time: Nov 19 23:23:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Nov 19 23:22:21 2023
Response via : Initial Calibration

