




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077636.D
 Acq On : 18 Nov 2023 17:32
 Operator : JC/SY
 Sample : 05438-02RE
 Misc : 5.02G/10ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EY1G3RE

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:26:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

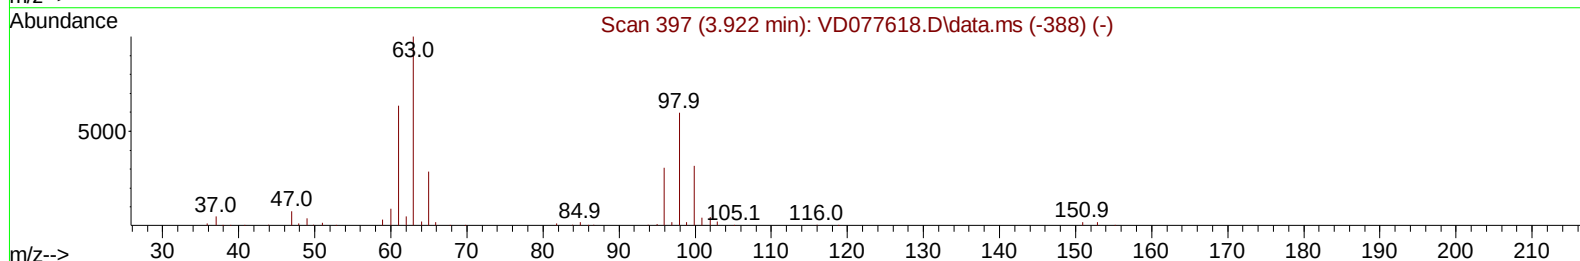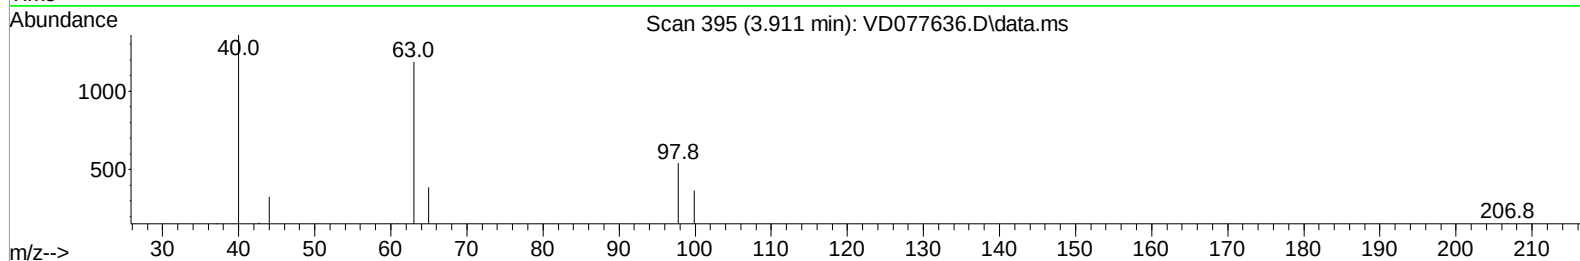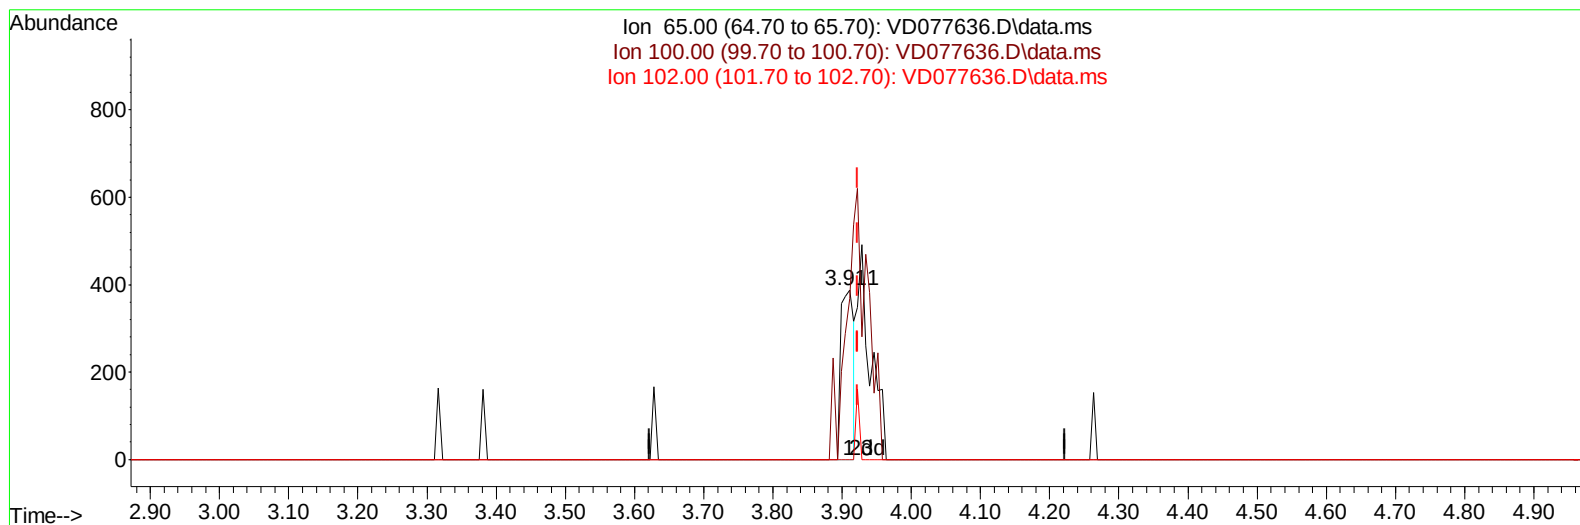

TIC: VD077636.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.911min (-0.011) 6.64 ug/L

response 506

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	125.30	160.08
102.00	19.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
Data File : VD077636.D
Acq On : 18 Nov 2023 17:32
Operator : JC/SY
Sample : 05438-02RE
Misc : 5.02G/10ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EY1G3RE

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:26:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Nov 19 23:22:21 2023
Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
Supervised By :Mahesh Dadoda 11/20/2023

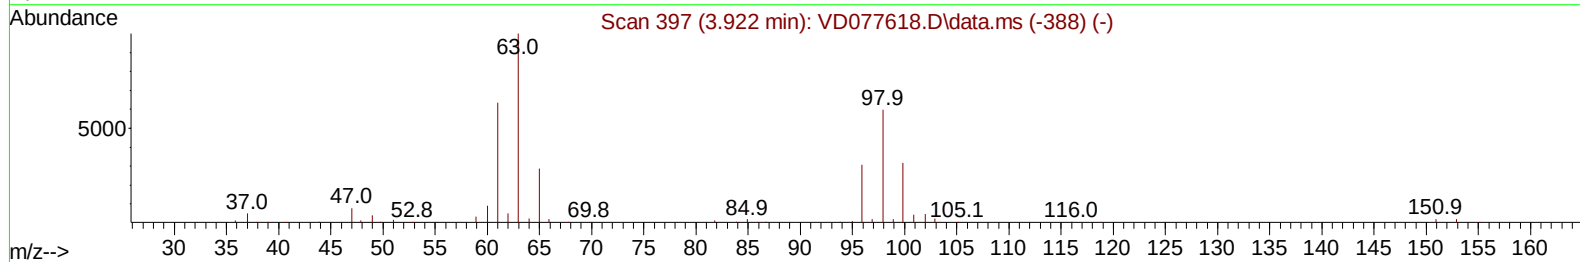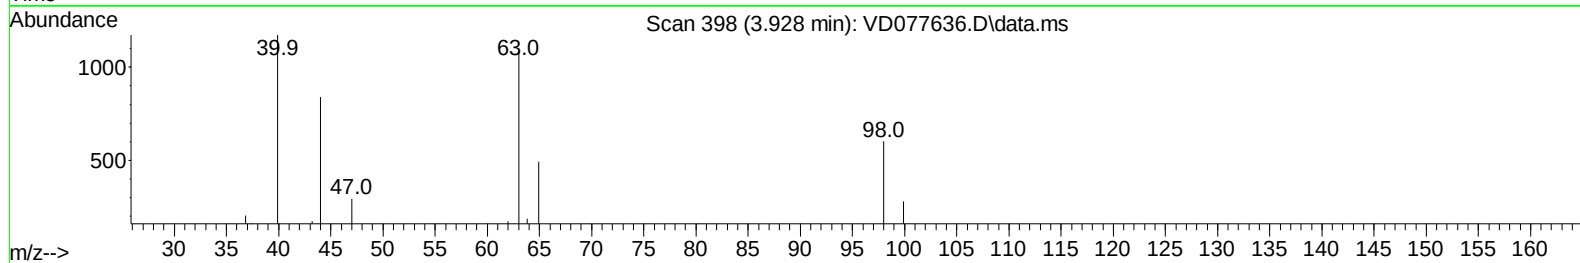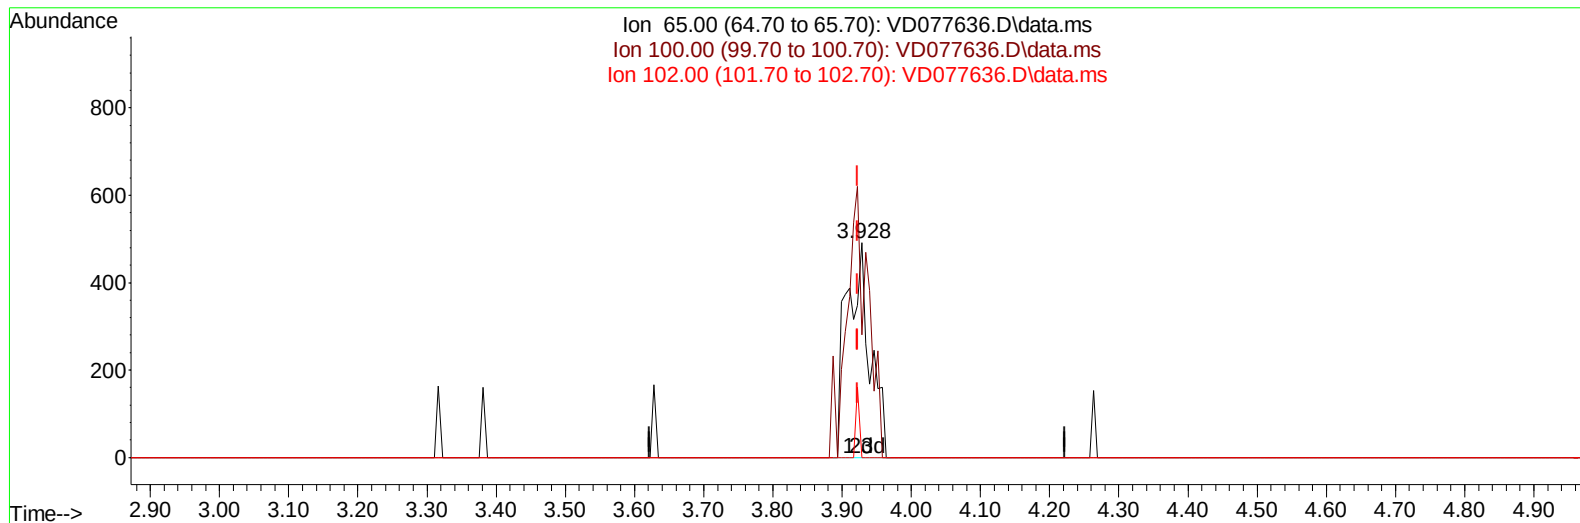

TIC: VD077636.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.928min (+ 0.006) 15.11 ug/L m

response 1152

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	125.30	70.31#
102.00	19.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077636.D
 Acq On : 18 Nov 2023 17:32
 Operator : JC/SY
 Sample : 05438-02RE
 Misc : 5.02G/10ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EY1G3RE

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:26:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

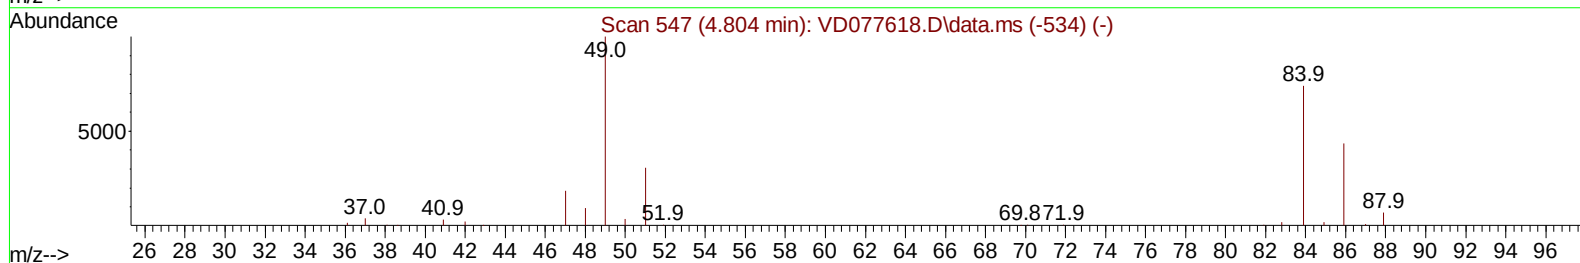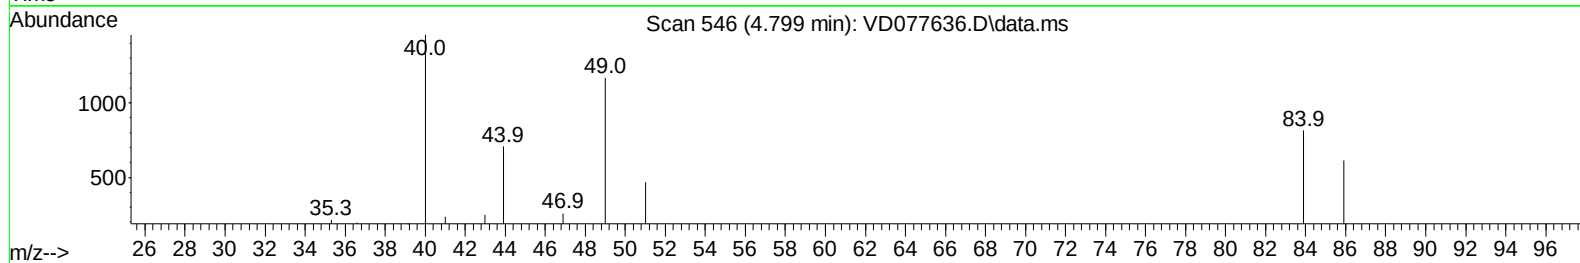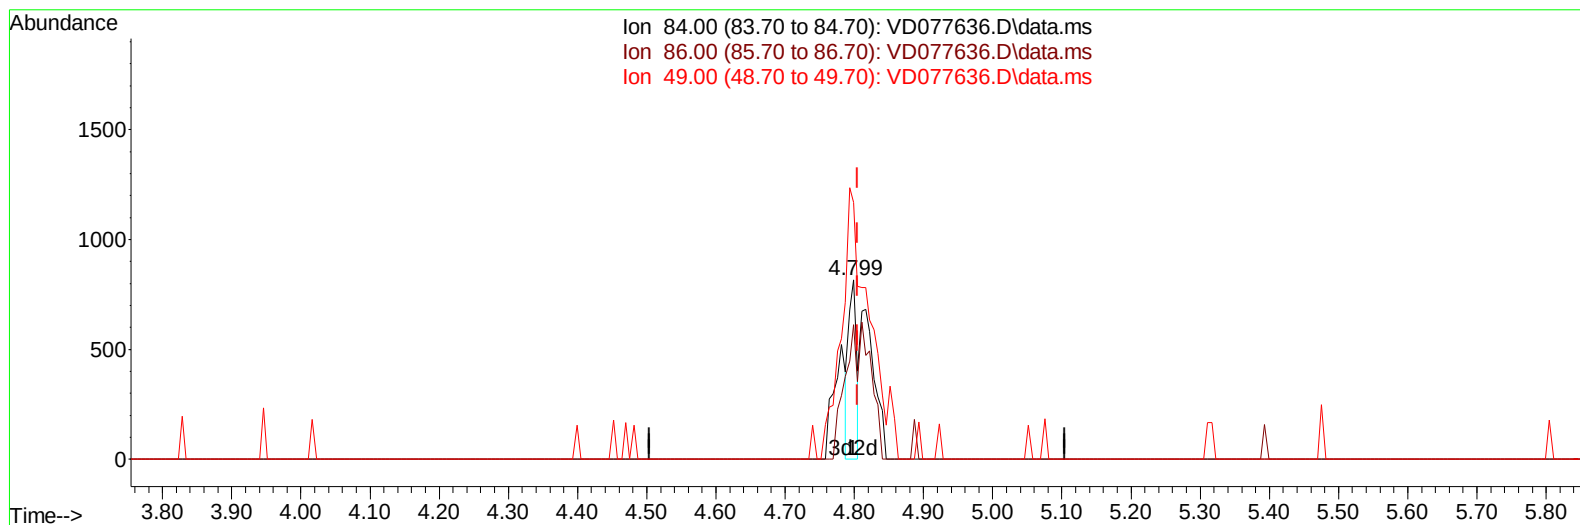

TIC: VD077636.D\data.ms

(16) Methylene chloride (T)

4.799min (-0.006) 4.09 ug/L

response 669

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	66.50	75.12
49.00	140.50	143.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077636.D
 Acq On : 18 Nov 2023 17:32
 Operator : JC/SY
 Sample : 05438-02RE
 Misc : 5.02G/10ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EY1G3RE

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:26:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

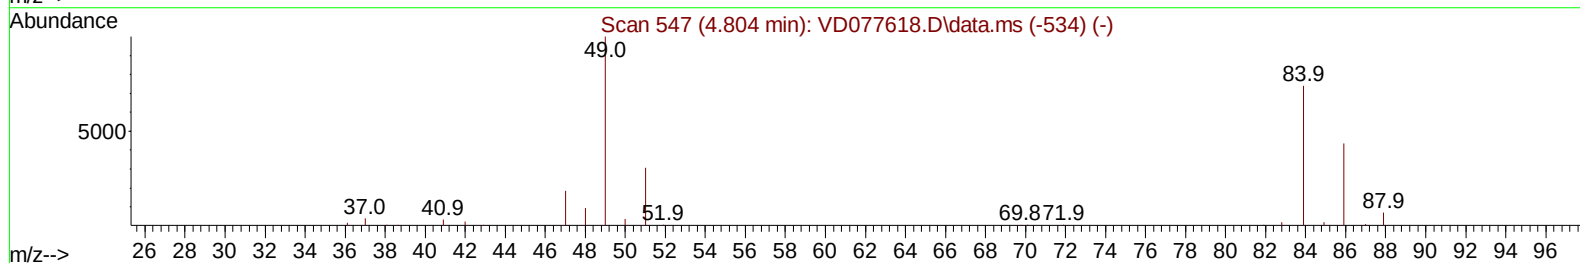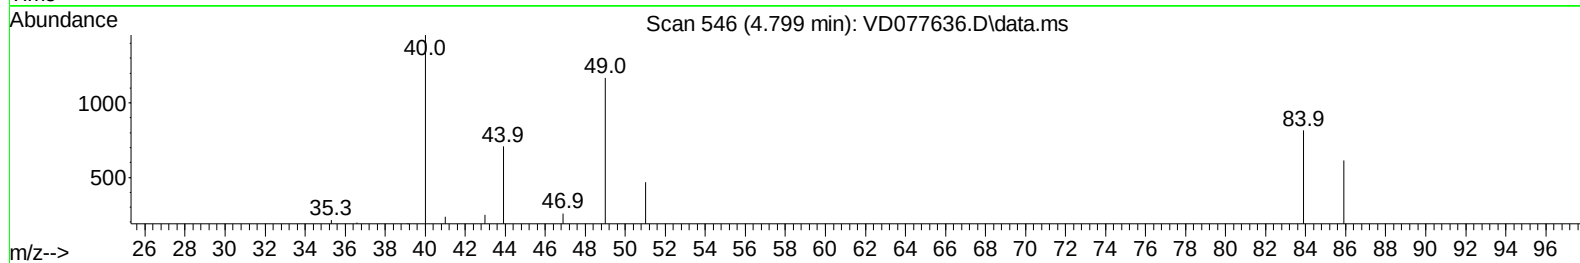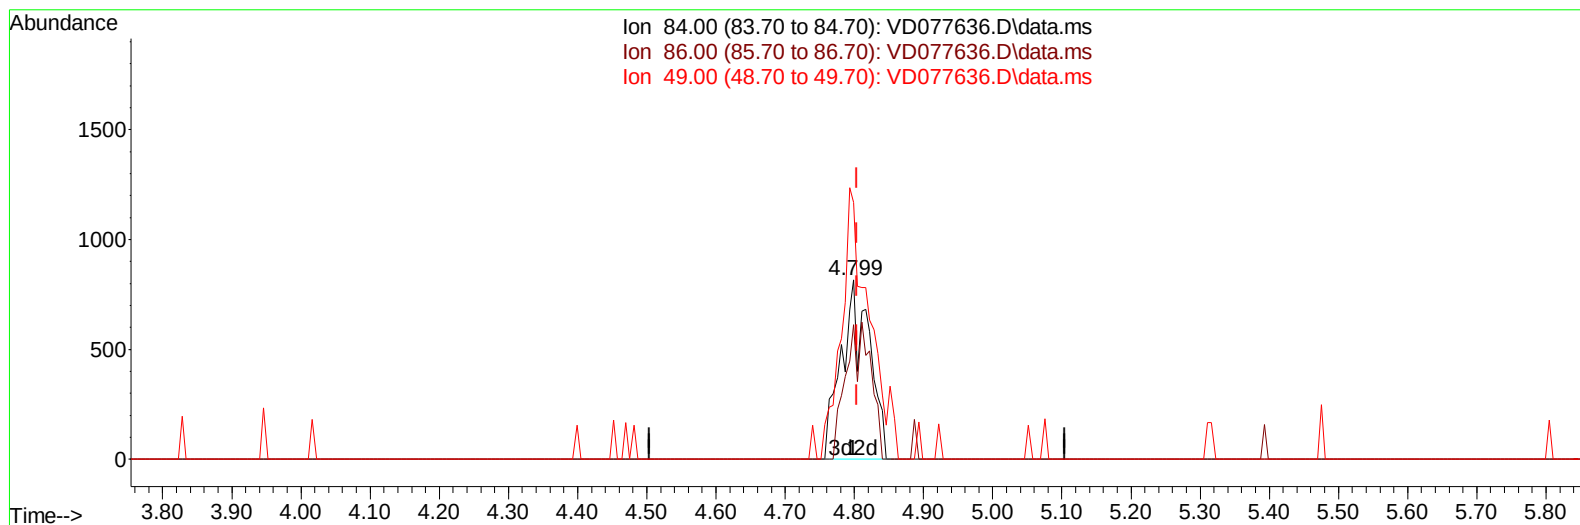

TIC: VD077636.D\data.ms

(16) Methylene chloride (T)

4.799min (-0.006) 14.17 ug/L m

response 2320

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	66.50	75.12
49.00	140.50	143.38
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077636.D
 Acq On : 18 Nov 2023 17:32
 Operator : JC/SY
 Sample : 05438-02RE
 Misc : 5.02G/10mL/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EY1G3RE

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:26:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	9694	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.587	117	9456	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	3543	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.281	65	3596	14.582	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.320%	
7) Chloroethane-d5	2.805	69	2710	13.989	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	55.960%	
11) 1,1-Dichloroethene-d2	3.928	65	1152m	15.107	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	60.440%	
21) 2-Butanone-d5	6.999	46	3177	74.411	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	148.820%#	
24) Chloroform-d	7.569	84	6988	24.954	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	8.222	65	4707	31.600	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	126.400%	
32) Benzene-d6	8.199	84	11855	19.316	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	77.280%	
36) 1,2-Dichloropropane-d6	9.210	67	4211	21.065	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	84.240%	
41) Toluene-d8	10.269	98	9050	16.319	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	65.280%	
43) trans-1,3-Dichloroprop...	10.528	79	1823	21.150	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.600%	
47) 2-Hexanone-d5	10.881	63	2512	70.243	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	140.480%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	4865	36.731	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	146.920%#	
66) 1,2-Dichlorobenzene-d4	13.822	152	2436	19.327	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	77.320%	
Target Compounds						
16) Methylene chloride	4.799	84	2320m	14.175	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
Data File : VD077636.D
Acq On : 18 Nov 2023 17:32
Operator : JC/SY
Sample : 05438-02RE
Misc : 5.02G/10ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EY1G3RE

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/20/2023
Supervised By :Mahesh Dadoda 11/20/2023

Quant Time: Nov 19 23:26:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Nov 19 23:22:21 2023
Response via : Initial Calibration

