

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
 Data File : VD077638.D
 Acq On : 18 Nov 2023 18:26
 Operator : JC/SY
 Sample : 05438-05
 Misc : 5.02G/10ml/MSVOA_D/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EY1G7

Quant Time: Nov 19 23:26:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Nov 19 23:22:21 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :John Carlone 11/20/2023
 Supervised By :Mahesh Dadoda 11/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	324285	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	257192	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	80132	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	129804	15.735	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.960%		
7) Chloroethane-d5	2.805	69	122904	18.965	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.880%		
11) 1,1-Dichloroethene-d2	3.916	65	40960	16.057	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.240%		
21) 2-Butanone-d5	6.981	46	46514	32.567	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	65.140%		
24) Chloroform-d	7.569	84	193214	20.625	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.520%		
26) 1,2-Dichloroethane-d4	8.234	65	111545m	22.385	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.560%		
32) Benzene-d6	8.204	84	355020	21.268	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.080%		
36) 1,2-Dichloropropane-d6	9.210	67	128647	23.660	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.640%		
41) Toluene-d8	10.269	98	288480	19.125	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.480%		
43) trans-1,3-Dichloroprop...	10.528	79	46538	19.851	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.400%		
47) 2-Hexanone-d5	10.875	63	37141	38.184	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.360%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	85530	23.742	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.960%		
66) 1,2-Dichlorobenzene-d4	13.816	152	59513	20.877	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.520%		
Target Compounds					Qvalue	
13) Acetone	4.028	43	5588	3.722	ug/L	74
16) Methylene chloride	4.799	84	77125	14.086	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
Data File : VD077638.D
Acq On : 18 Nov 2023 18:26
Operator : JC/SY
Sample : 05438-05
Misc : 5.02G/10ml/MSVOA_D/SOIL
ALS Vial : 22 Sample Multiplier: 1


Instrument :
MSVOA_D
ClientSampleId :
EY1G7

Quant Time: Nov 19 23:26:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Nov 19 23:22:21 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 11/20/2023
Supervised By : Mahesh Dadoda 11/20/2023

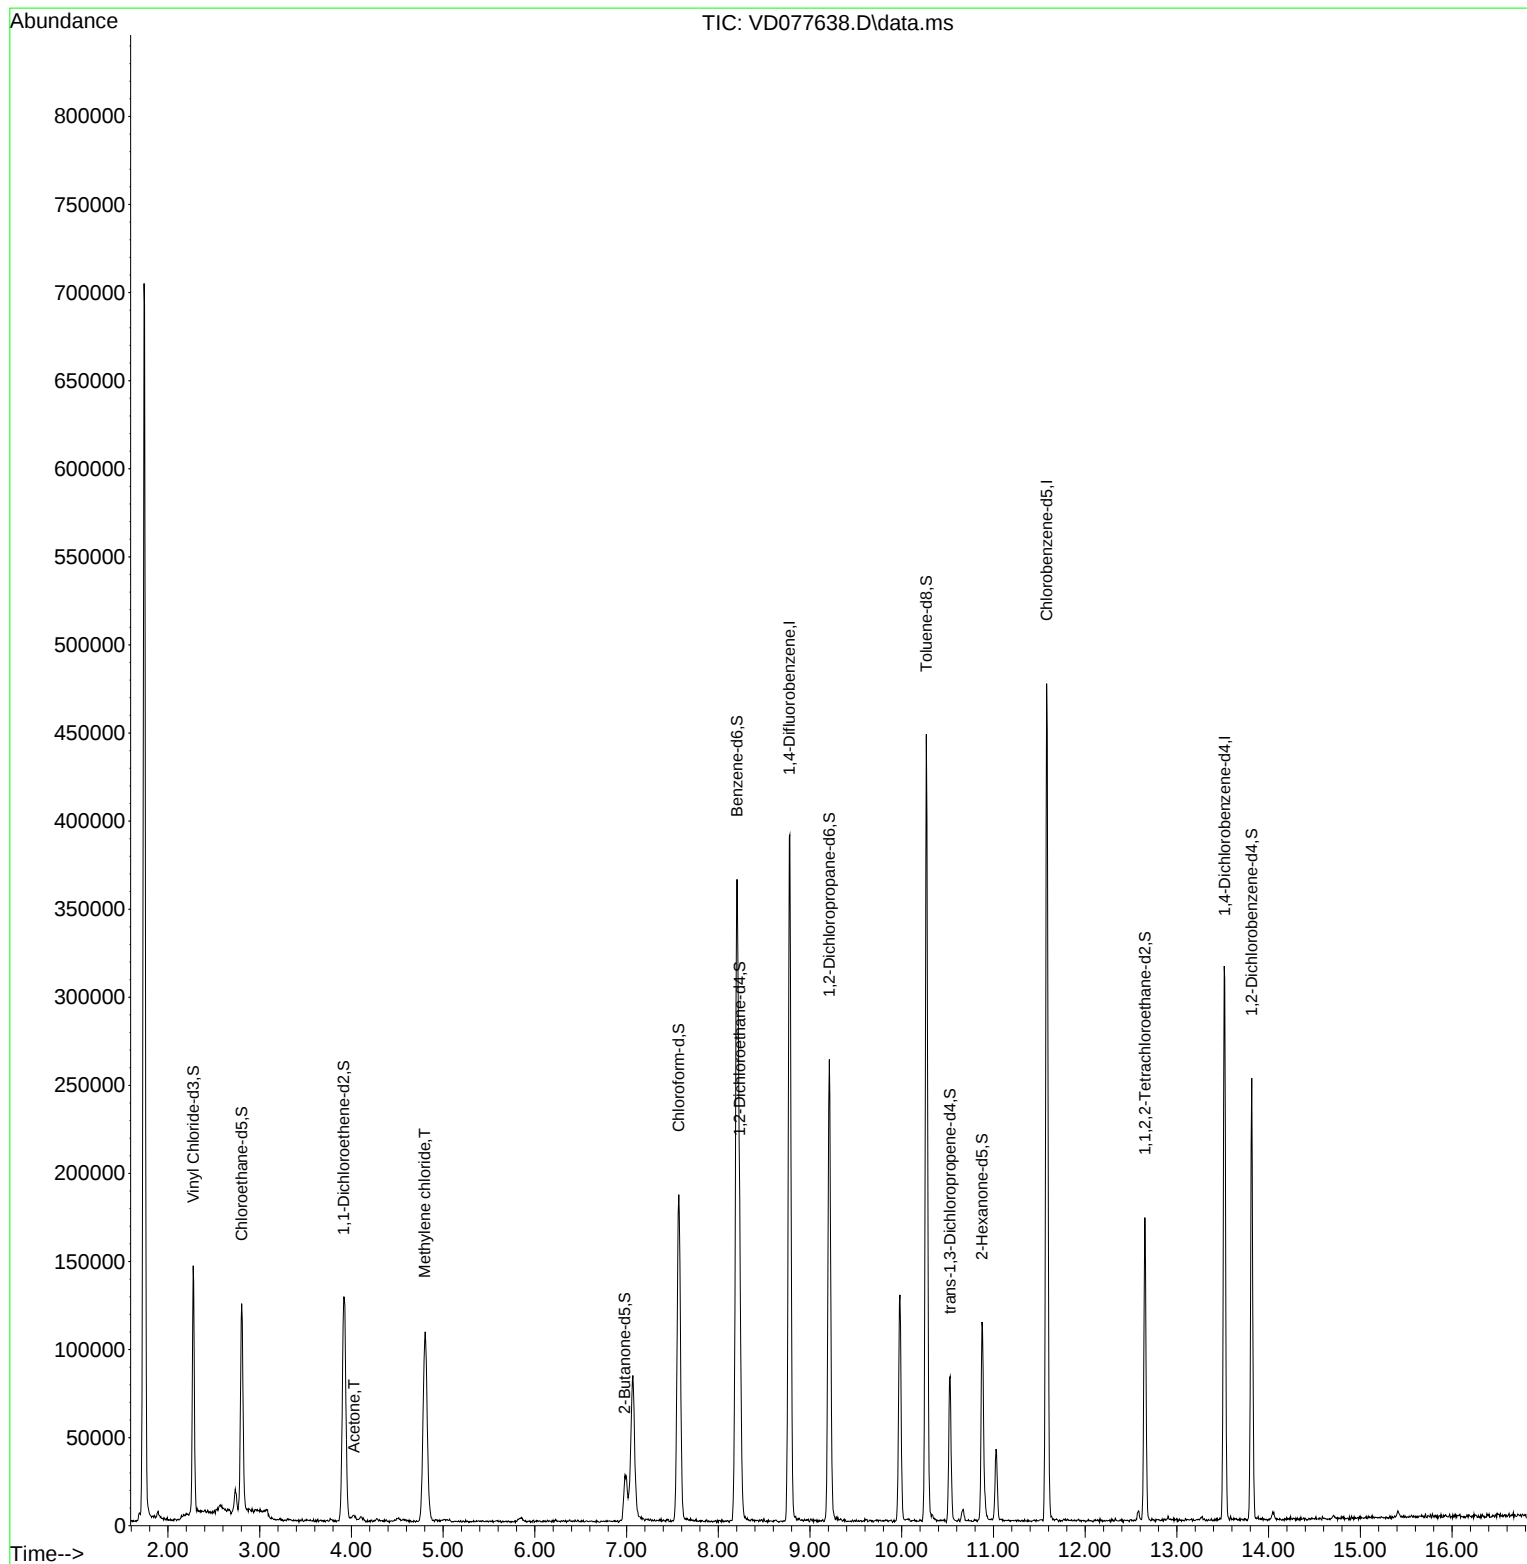

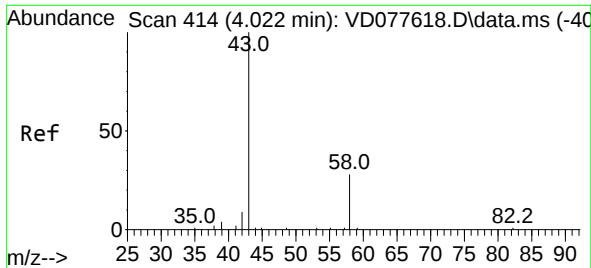

#13

Acetone

Concen: 3.722 ug/L

RT: 4.028 min Scan# 41

Delta R.T. 0.006 min

Lab File: VD077638.D

Acq: 18 Nov 2023 18:26

Instrument :

MSVOA_D

ClientSampleId :

EY1G7

Tgt Ion: 43 Resp: 5588

Ion Ratio Lower Upper

43 100





58 17.5 0.0 64.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 11/20/2023

Supervised By :Mahesh Dadoda 11/20/2023

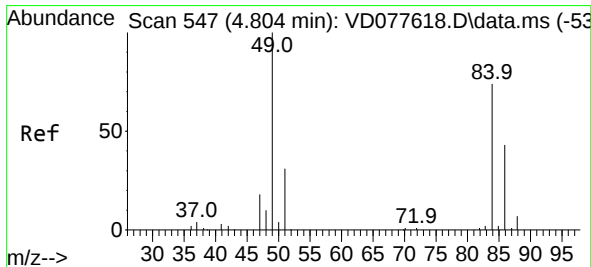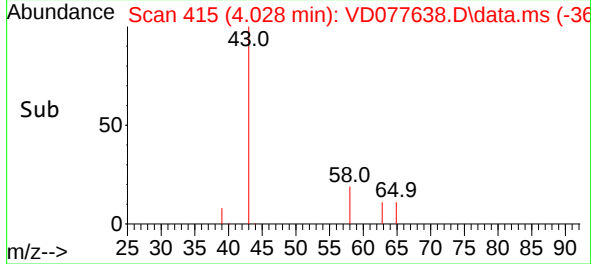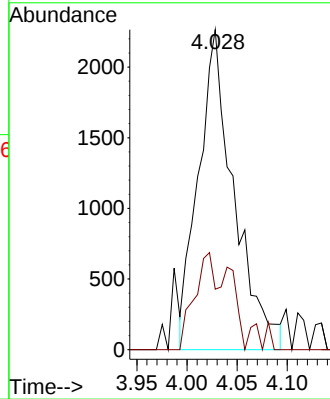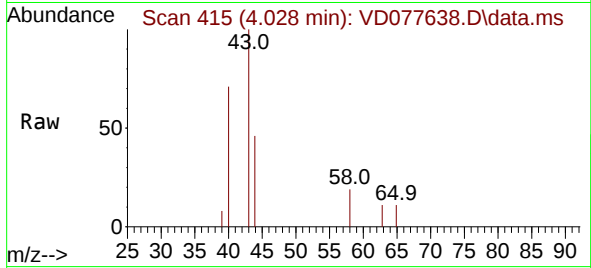

#16

Methylene chloride

Concen: 14.086 ug/L

RT: 4.799 min Scan# 546

Delta R.T. -0.006 min

Lab File: VD077638.D

Acq: 18 Nov 2023 18:26

Tgt Ion: 84 Resp: 77125

Ion Ratio Lower Upper

84 100

86 62.3 46.5 86.5

49 129.1 98.3 182.7

