
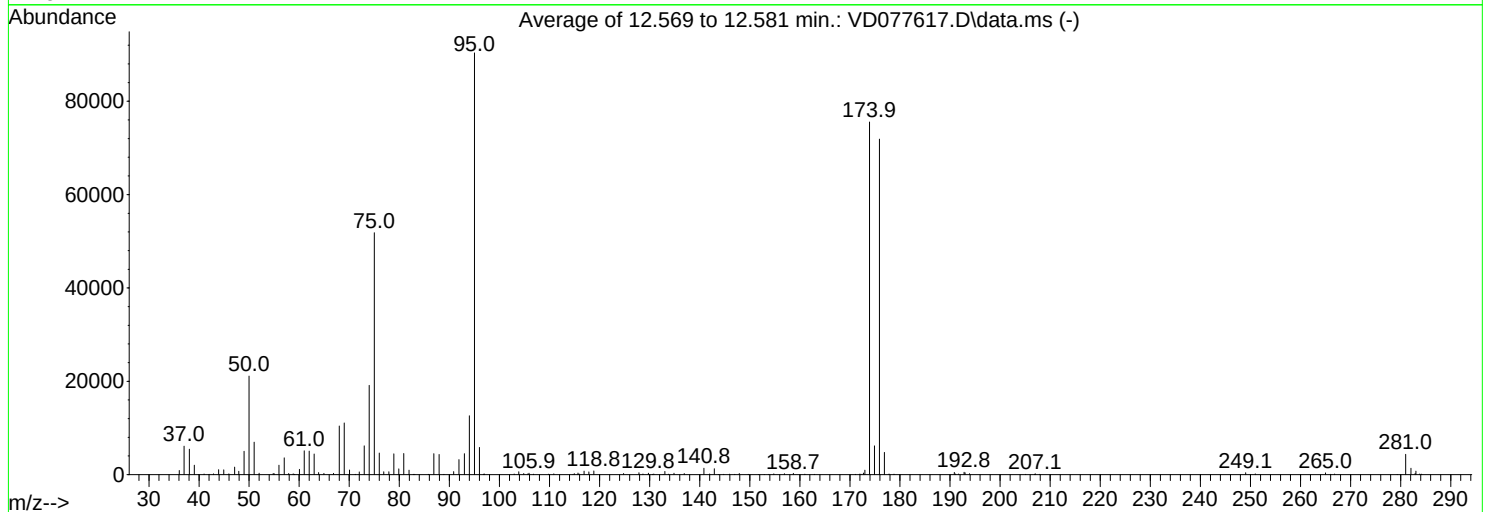


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111823\
Data File : VD077617.D
Acq On : 18 Nov 2023 08:43
Operator : JC/SY
Sample : BFB181
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB181

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Title : SFAM01.0
Last Update : Sun Nov 19 23:22:21 2023

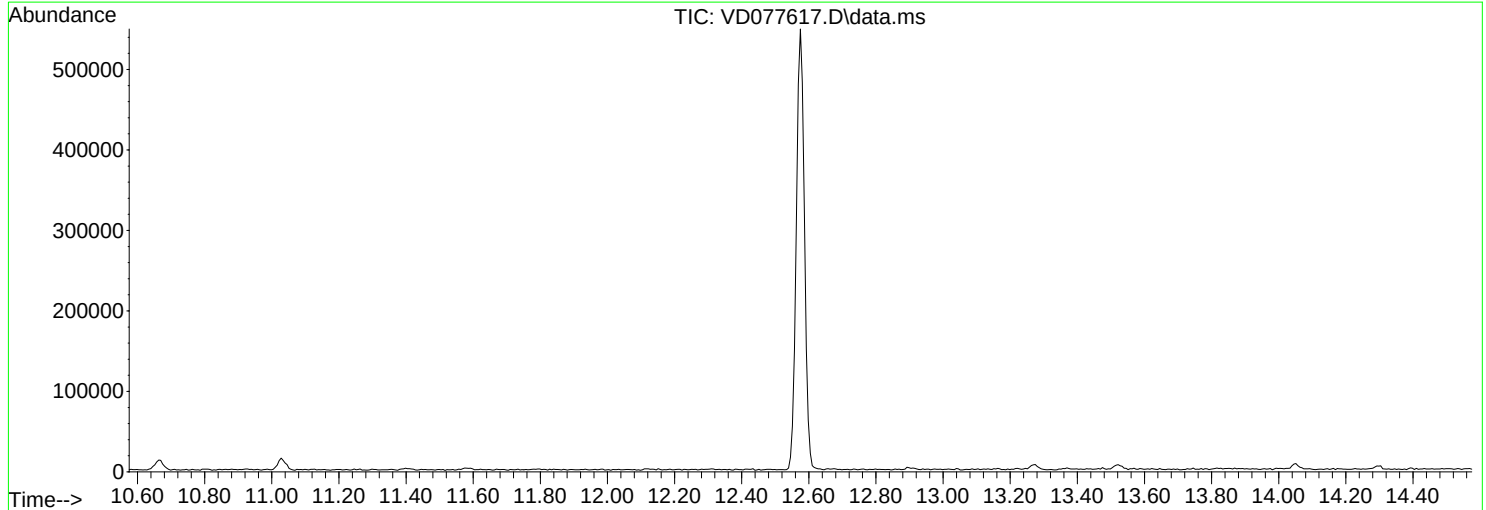

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	21133	PASS
75	95	30	80	57.3	51824	PASS
95	95	100	100	100.0	90373	PASS
96	95	5	9	6.5	5832	PASS
173	174	0.00	2	1.3	965	PASS
174	95	50	120	83.6	75573	PASS
175	174	5	9	8.2	6181	PASS
176	174	95	105	95.1	71877	PASS
177	176	5	10	6.6	4762	PASS

Scan 1860 (12.528 min): VD077617.D\data.ms
BFB181

m/z	Abundance
40.00	1672.0
43.90	635.0
89.20	160.0
207.10	168.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181

m/z	Abundance
36.10	918.0
37.00	6903.0
38.00	5050.0
39.10	2056.0
39.90	1526.0
41.10	161.0
42.90	199.0
44.00	1886.0
45.00	1024.0
45.90	181.0
47.20	1245.0
48.10	626.0
49.00	4823.0
50.00	20456.0
51.00	7064.0
52.00	553.0
54.80	506.0
56.00	2091.0
57.00	3782.0
58.80	313.0
60.00	849.0
61.00	5192.0
62.00	4519.0
63.00	4445.0
63.90	434.0
64.90	188.0
68.00	10139.0
69.00	10598.0
70.00	1037.0
72.00	617.0
73.00	5567.0
74.00	19352.0
75.00	49168.0
76.00	4370.0
76.80	565.0
77.90	506.0
78.90	4611.0
80.00	1164.0
80.90	4078.0
82.00	1053.0
85.80	201.0
86.80	4787.0
87.90	4198.0
90.80	512.0
91.90	3340.0
93.00	4453.0
94.00	12297.0
95.00	87008.0
96.00	5315.0
96.80	287.0
103.90	704.0
104.90	273.0
105.70	569.0
109.80	197.0
110.90	239.0
114.70	175.0
115.70	332.0
116.90	578.0
117.90	696.0
118.90	490.0
124.80	301.0
127.90	422.0
128.60	283.0
129.80	402.0
130.90	204.0
132.70	258.0
133.20	496.0
133.80	193.0
134.80	349.0
137.00	245.0
140.80	1182.0
142.00	188.0
142.80	1083.0
143.80	157.0
147.90	274.0
154.70	155.0
158.70	269.0
161.10	159.0
162.90	208.0
171.90	350.0
173.00	1259.0
173.90	70240.0
174.90	6339.0
175.90	67776.0
176.90	4903.0
191.10	436.0
192.80	699.0
193.90	156.0
206.90	358.0
249.00	324.0
251.00	349.0
265.00	288.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181

281.00	2843.0
282.00	1064.0
282.90	738.0
284.20	313.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181

m/z	Abundance
36.00	1061.0
37.00	6092.0
38.10	5496.0
39.00	1984.0
40.00	1786.0
42.00	177.0
43.90	1412.0
45.00	1100.0
46.00	158.0
47.00	1977.0
47.90	715.0
49.00	5241.0
50.00	23632.0
51.00	7528.0
52.00	226.0
54.80	181.0
56.00	2258.0
57.00	4098.0
57.90	358.0
58.80	223.0
60.10	1572.0
61.00	5358.0
62.00	5594.0
63.00	4389.0
63.90	429.0
65.00	362.0
66.90	584.0
68.00	11385.0
69.00	11730.0
70.10	985.0
71.20	173.0
72.00	668.0
73.00	6429.0
74.00	20936.0
75.00	57120.0
76.00	4970.0
76.90	771.0
77.90	795.0
78.90	4660.0
79.80	1478.0
80.90	5555.0
81.90	937.0
83.10	239.0
86.90	4594.0
87.90	4449.0
88.90	167.0
90.90	848.0
91.90	3508.0
93.00	4954.0
94.00	13177.0
95.00	100216.0
96.00	6818.0
103.00	161.0
103.80	670.0
104.80	162.0
105.90	470.0
106.80	156.0
110.70	153.0
115.00	289.0
115.70	731.0
116.90	812.0
117.90	550.0
118.80	1237.0
127.80	402.0
129.80	240.0
130.60	216.0
133.00	624.0
134.90	289.0
136.80	196.0
140.90	1722.0
142.00	220.0
142.90	1478.0
146.00	159.0
147.00	226.0
147.90	295.0
151.80	153.0
152.90	156.0
154.80	246.0
156.90	341.0
158.70	172.0
160.90	159.0
171.10	231.0
172.20	323.0
173.00	1635.0
173.90	81744.0
174.90	6313.0
175.90	79480.0
176.90	4423.0
177.80	234.0
190.80	656.0
191.70	190.0
192.80	824.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181

193.80	199.0
205.10	173.0
207.10	472.0
249.10	525.0
265.00	528.0
266.00	185.0
266.80	171.0
279.30	156.0
281.00	4574.0
282.00	1680.0
283.10	1117.0
283.80	214.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181

m/z	Abundance
36.10	736.0
37.00	5325.0
38.00	5866.0
39.00	1992.0
39.90	1849.0
40.90	232.0
42.90	345.0
44.00	1785.0
44.90	964.0
45.90	172.0
47.10	1599.0
47.90	836.0
49.00	4943.0
50.00	19312.0
51.00	6253.0
51.90	194.0
55.00	603.0
55.90	1771.0
57.00	2932.0
57.90	367.0
59.10	228.0
60.00	1019.0
61.00	4827.0
62.00	5015.0
63.00	4395.0
63.90	502.0
64.90	326.0
66.80	294.0
68.00	9740.0
69.00	10877.0
70.00	917.0
72.00	455.0
73.00	6481.0
74.00	17088.0
75.00	49184.0
76.00	4527.0
77.00	536.0
77.90	597.0
78.90	4117.0
79.90	1029.0
80.90	3909.0
81.90	872.0
82.80	229.0
87.00	4143.0
88.00	4368.0
90.90	553.0
91.90	2827.0
93.00	4081.0
94.00	12418.0
95.00	83896.0
96.00	5362.0
97.00	374.0
102.90	258.0
103.90	501.0
104.90	329.0
105.90	487.0
106.80	162.0
109.90	169.0
110.90	164.0
114.90	345.0
115.90	407.0
116.90	835.0
117.80	491.0
118.90	605.0
124.80	461.0
127.80	412.0
128.70	158.0
129.70	260.0
130.80	201.0
133.00	906.0
133.70	176.0
134.90	253.0
136.90	334.0
140.90	1219.0
143.00	1273.0
144.80	214.0
145.90	180.0
147.90	150.0
149.70	181.0
153.80	197.0
154.90	169.0
156.90	258.0
158.70	370.0
172.70	1067.0
173.90	74736.0
174.90	5891.0
175.90	68376.0
176.90	4961.0
177.80	182.0
178.80	292.0
190.90	781.0
191.70	237.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181

193.00	1265.0
194.00	236.0
207.00	606.0
207.90	193.0
249.00	393.0
250.90	171.0
265.00	364.0
266.80	270.0
281.00	5687.0
282.10	1407.0
283.00	1150.0
283.80	228.0

Instrument :
MSVOA_D
ClientSampleId :
BFB181