

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111824\
 Data File : VD080075.D
 Acq On : 18 Nov 2024 18:00
 Operator : RP/MD
 Sample : P4860-04
 Misc : 6.28G/5ml/MSVOA_D/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PH2-BOT-003

Quant Time: Nov 19 04:50:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 15 16:25:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	207332	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	367976	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	326426	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	150989	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	84545	39.605	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	79.220%
35) Dibromofluoromethane	7.804	113	94139	38.440	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	76.880%
50) Toluene-d8	10.269	98	314551	34.078	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	68.160%
62) 4-Bromofluorobenzene	12.575	95	92979	30.703	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	61.400%


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111824\
Data File : VD080075.D
Acq On : 18 Nov 2024 18:00
Operator : RP/MD
Sample : P4860-04
Misc : 6.28G/5ml/MSVOA_D/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PH2-BOT-003


Quant Time: Nov 19 04:50:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 15 16:25:47 2024
Response via : Initial Calibration

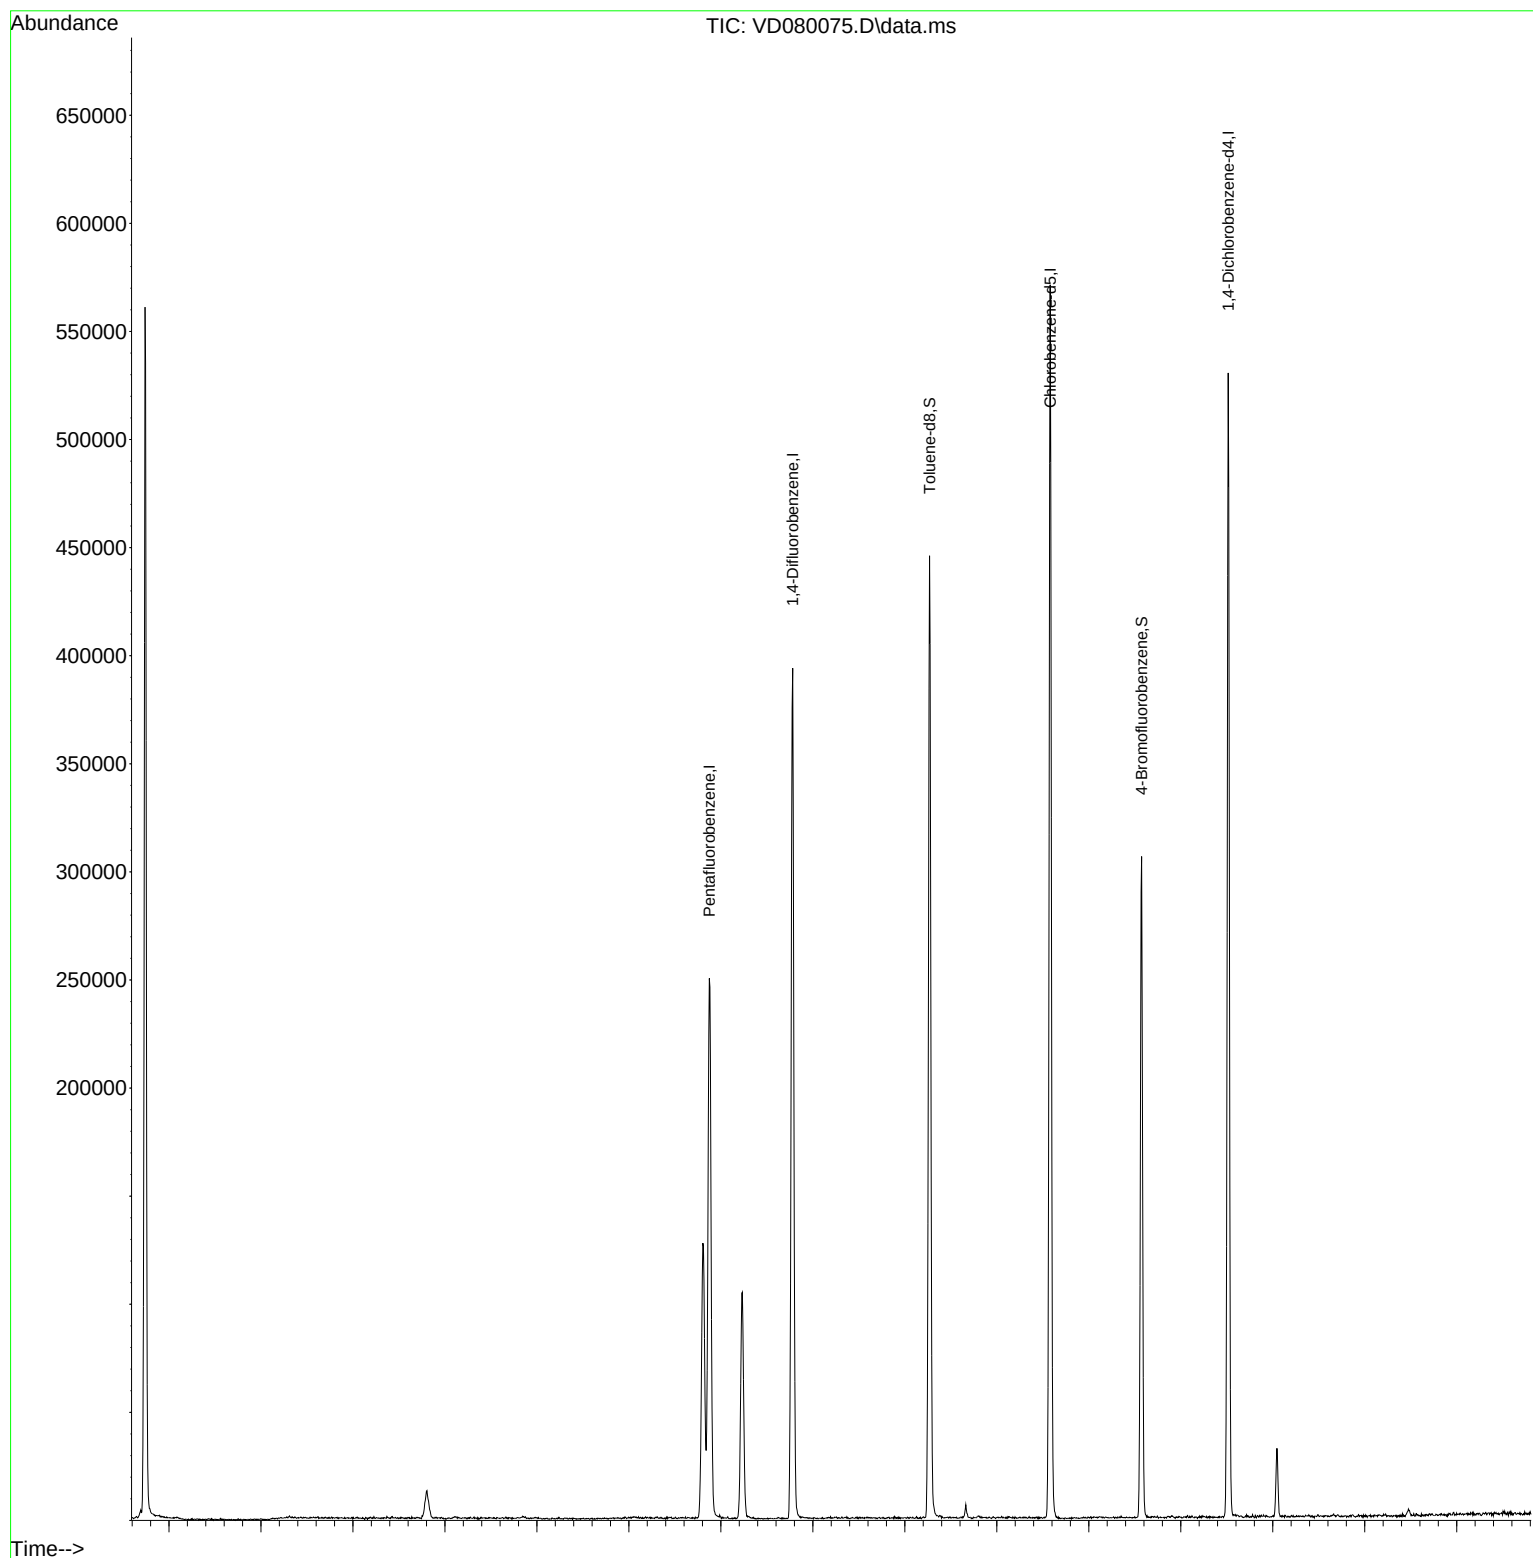



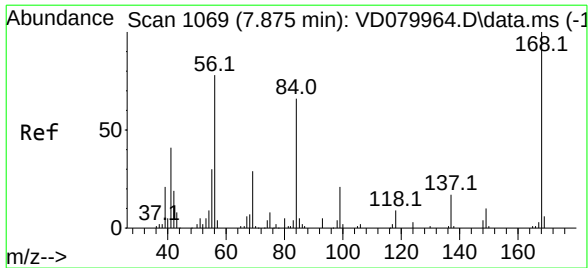


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. -0.000 min
Lab File: VD080075.D
Acq: 18 Nov 2024 18:00

Instrument :
MSVOA_D
ClientSampleId :
PH2-BOT-003



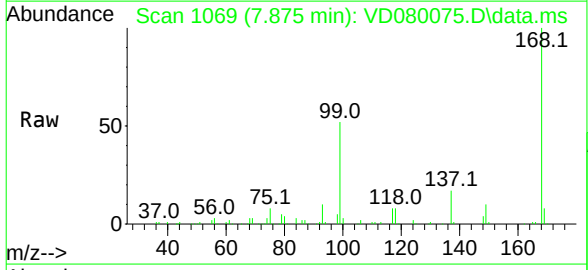



Tgt Ion:168 Resp: 207332
Ion Ratio Lower Upper
168 100
99 51.7 46.0 69.0

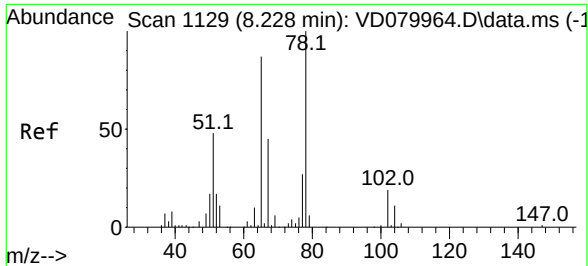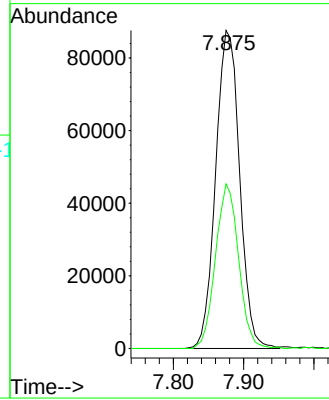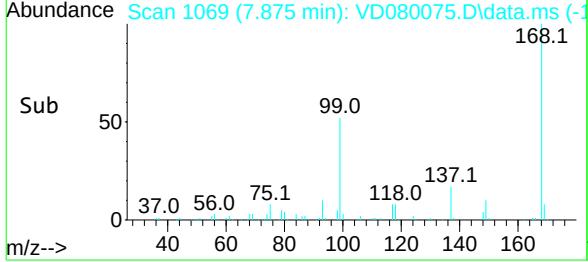

#33
1,2-Dichloroethane-d4
Concen: 39.605 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD080075.D
Acq: 18 Nov 2024 18:00


Tgt Ion: 65 Resp: 84545
Ion Ratio Lower Upper
65 100
67 55.2 0.0 109.2

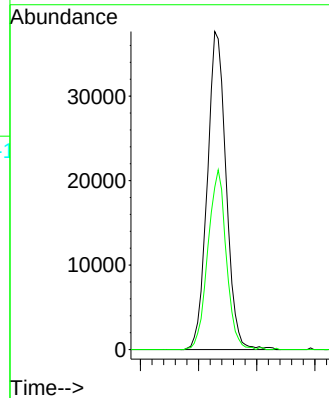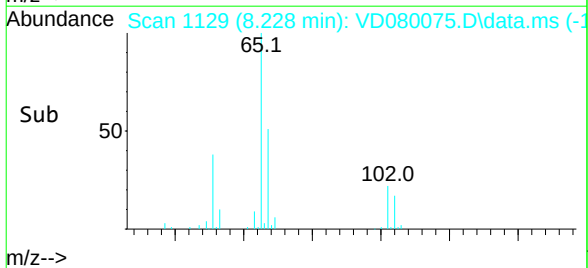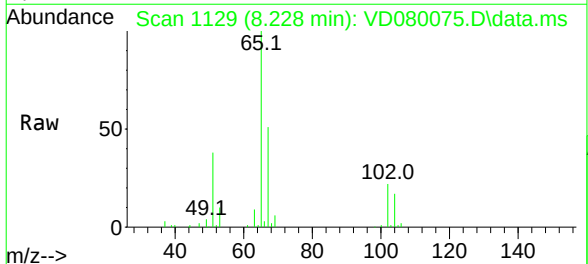



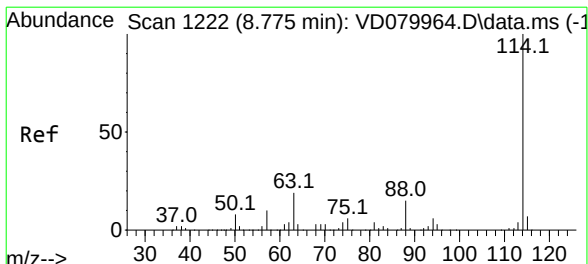


#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.781 min Scan# 1222
 Delta R.T. 0.006 min
 Lab File: VD080075.D
 Acq: 18 Nov 2024 18:00

Instrument :
 MSVOA_D
 ClientSampleId :
 PH2-BOT-003



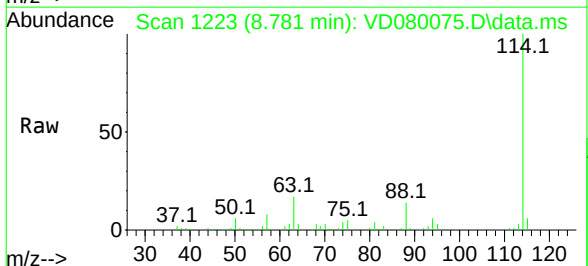



Tgt Ion:	114	Resp:	367976
Ion	Ratio	Lower	Upper
114	100		
63	16.7	0.0	38.8
88	14.3	0.0	30.6

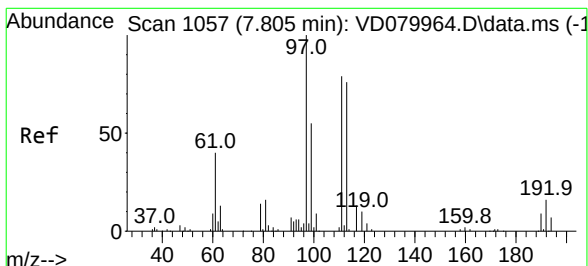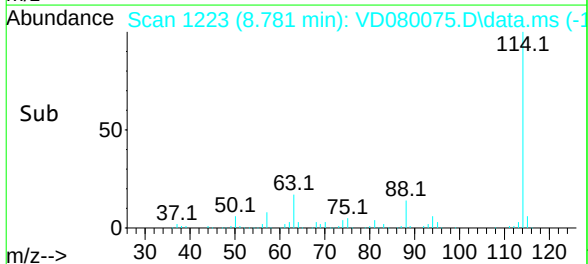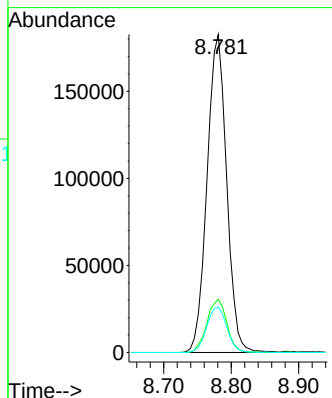

#35
 Dibromofluoromethane
 Concen: 38.440 ug/l
 RT: 7.804 min Scan# 1057
 Delta R.T. -0.001 min
 Lab File: VD080075.D
 Acq: 18 Nov 2024 18:00

Tgt Ion:	113	Resp:	94139
Ion	Ratio	Lower	Upper
113	100		
111	101.6	82.5	123.7
192	20.5	16.6	25.0

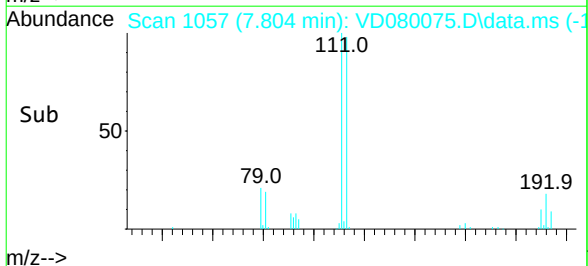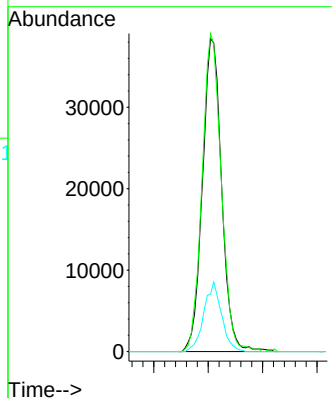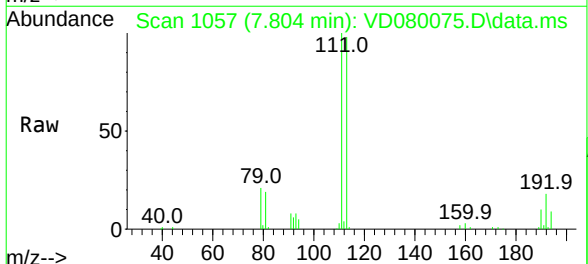

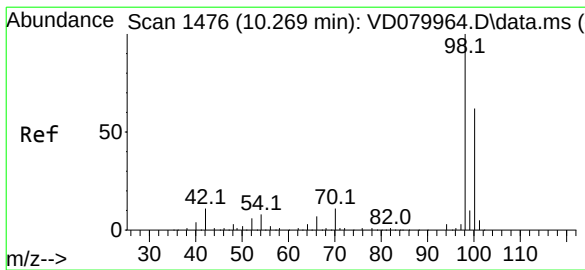

#50

Toluene-d8

Concen: 34.078 ug/l

RT: 10.269 min Scan# 14

Delta R.T. -0.000 min

Lab File: VD080075.D

Acq: 18 Nov 2024 18:00

Instrument :

MSVOA_D

ClientSampleId :





PH2-BOT-003

Tgt Ion: 98 Resp: 314551

Ion Ratio Lower Upper

98 100

100 62.5 50.2 75.4

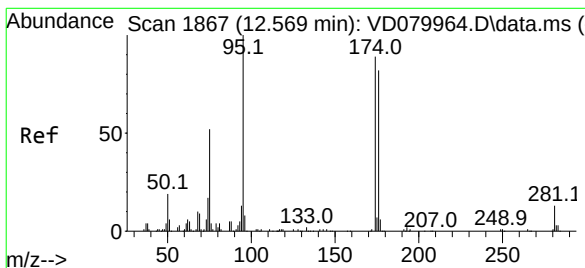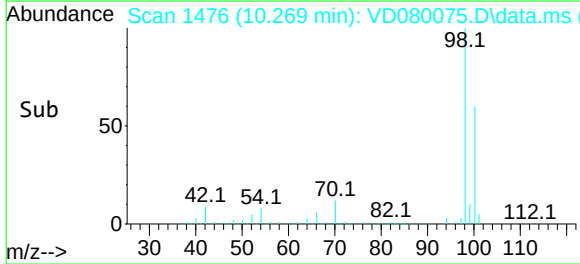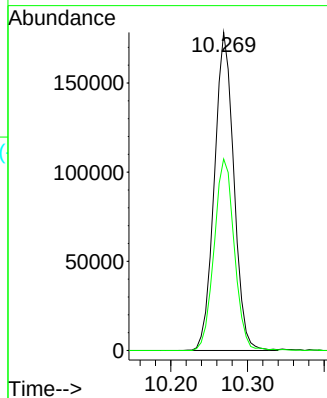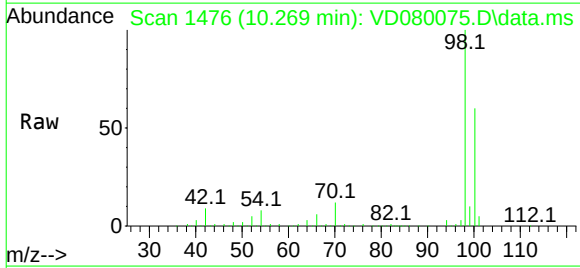

#62

4-Bromofluorobenzene

Concen: 30.703 ug/l

RT: 12.575 min Scan# 1868

Delta R.T. 0.006 min

Lab File: VD080075.D

Acq: 18 Nov 2024 18:00




Tgt Ion: 95 Resp: 92979


Ion Ratio Lower Upper

95 100

174 94.8 0.0 173.4

176 91.9 0.0 166.6


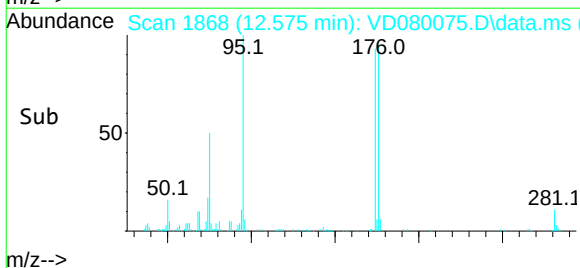
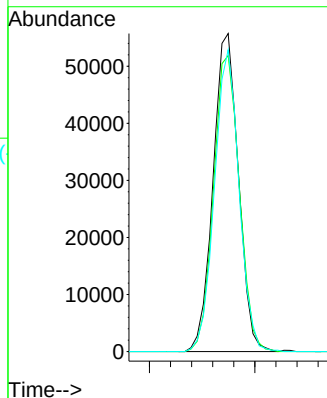
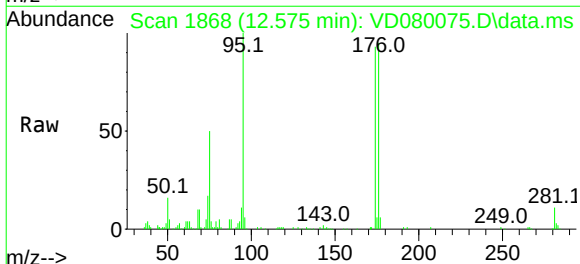


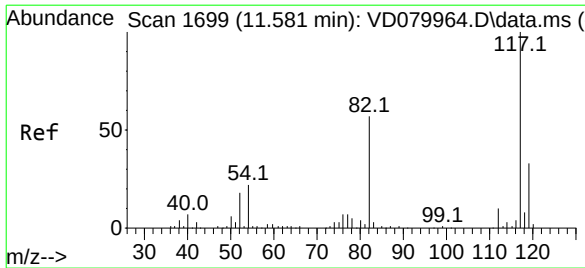

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD080075.D
Acq: 18 Nov 2024 18:00

Instrument :
MSVOA_D
ClientSampleId :
PH2-BOT-003

Tgt Ion:117 Resp: 326426
Ion Ratio Lower Upper
117 100
82 52.1 45.8 68.6
119 32.1 26.2 39.2

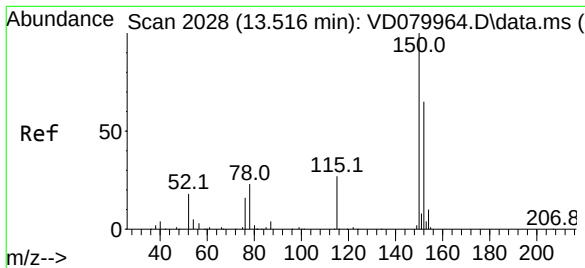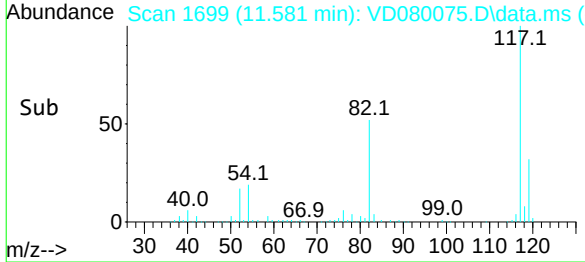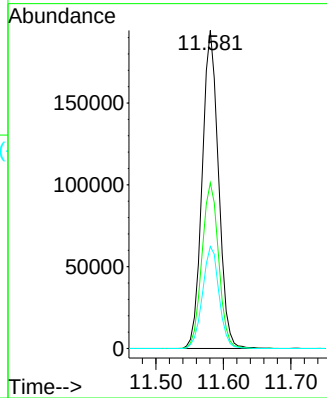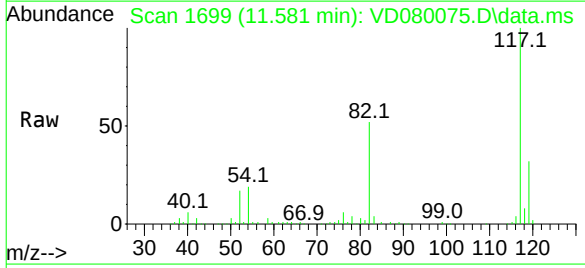

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD080075.D
Acq: 18 Nov 2024 18:00

Tgt Ion:152 Resp: 150989
Ion Ratio Lower Upper
152 100
115 57.3 28.9 86.8
150 155.6 0.0 354.8

