
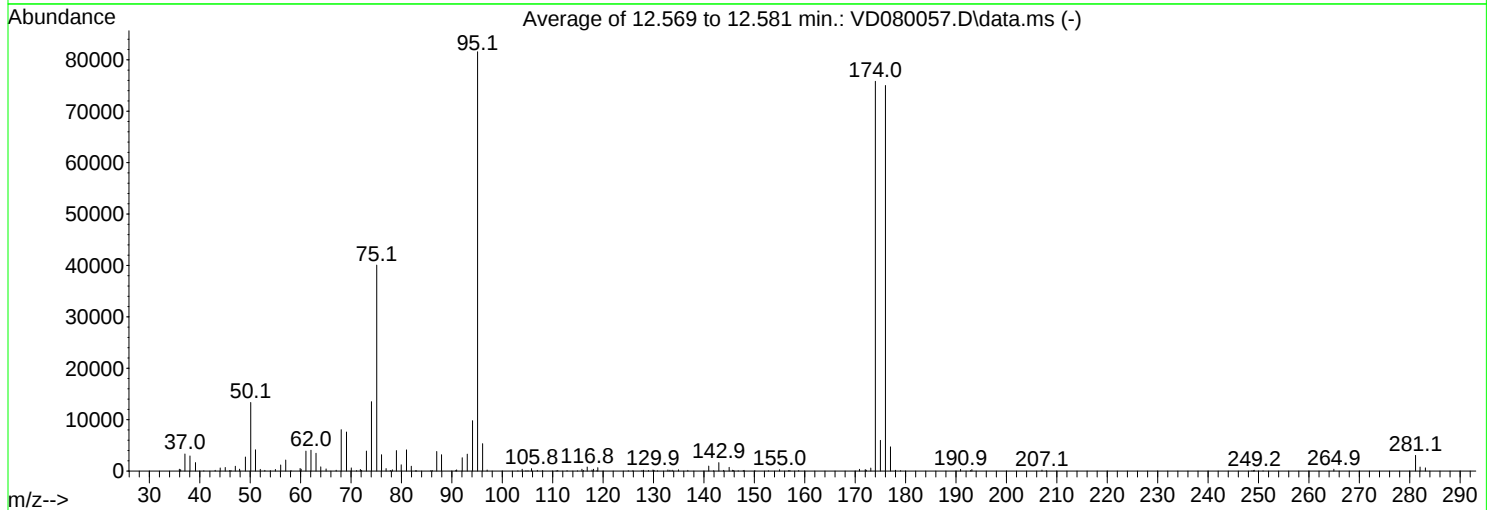


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111824\
Data File : VD080057.D
Acq On : 18 Nov 2024 09:21
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111524S.M
Title : SW846 8260
Last Update : Fri Nov 15 16:25:47 2024

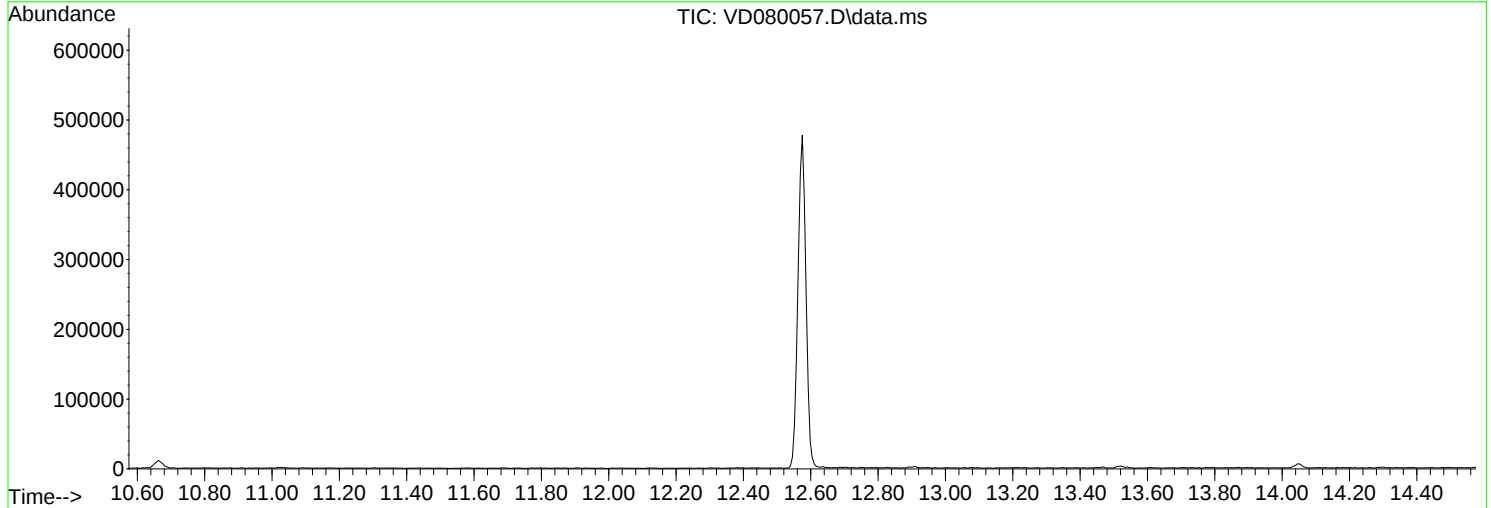

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	13343	PASS
75	95	30	60	49.1	40069	PASS
95	95	100	100	100.0	81573	PASS
96	95	5	9	6.5	5338	PASS
173	174	0.00	2	0.8	585	PASS
174	95	50	100	93.0	75827	PASS
175	174	5	9	7.9	5977	PASS
176	174	95	101	98.9	75008	PASS
177	176	5	9	6.3	4717	PASS