


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD111918\
Data File : VD060410.D
Acq On : 19 Nov 2018 10:53
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Title : SW846 8260
Last Update : Mon Nov 19 16:31:59 2018

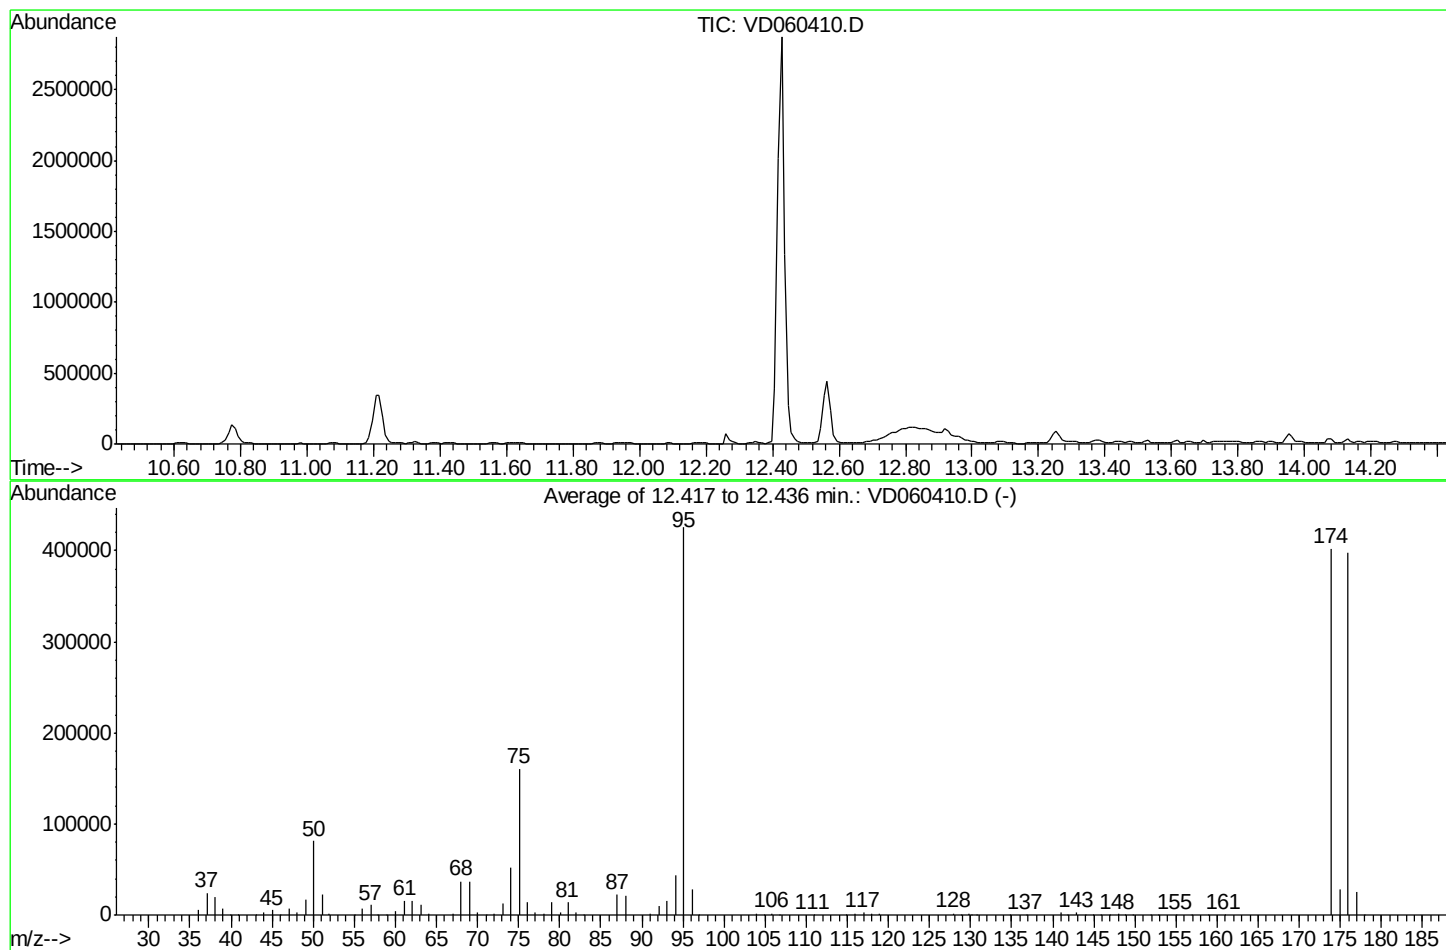

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	81237	PASS
75	95	30	60	37.7	160306	PASS
95	95	100	100	100.0	425685	PASS
96	95	5	9	6.5	27869	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.5	402133	PASS
175	174	5	9	7.1	28664	PASS
176	174	95	101	98.8	397440	PASS
177	176	5	9	6.5	25728	PASS