
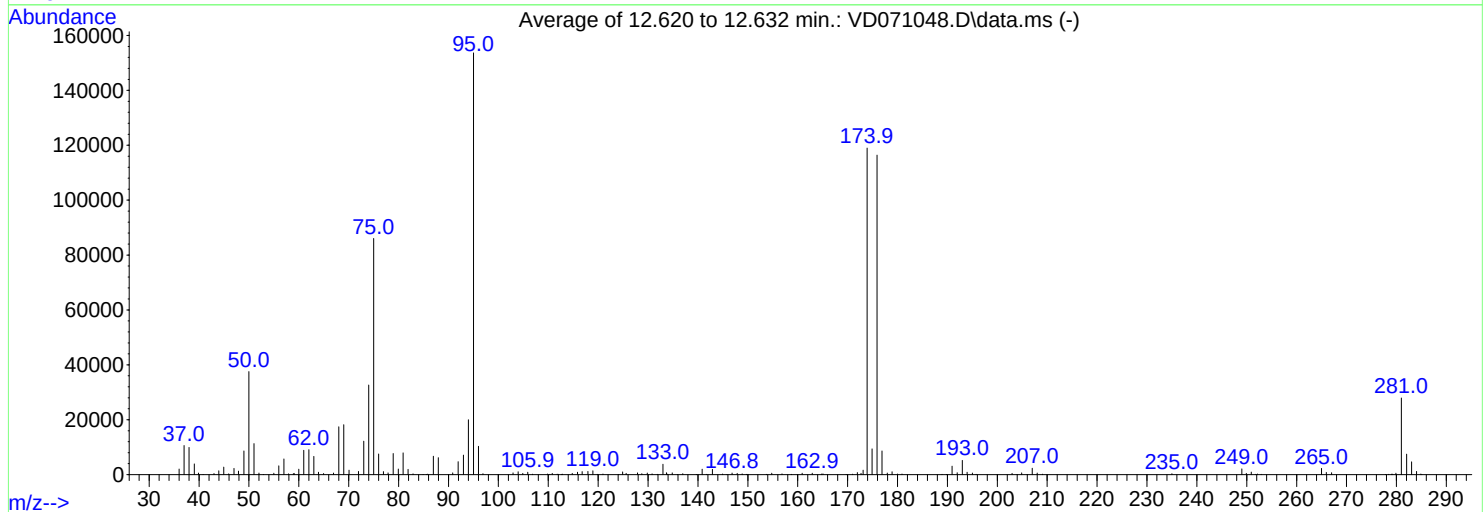


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111921\
Data File : VD071048.D
Acq On : 19 Nov 2021 09:59
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110921S.M
Title : SW846 8260
Last Update : Wed Nov 10 03:55:51 2021

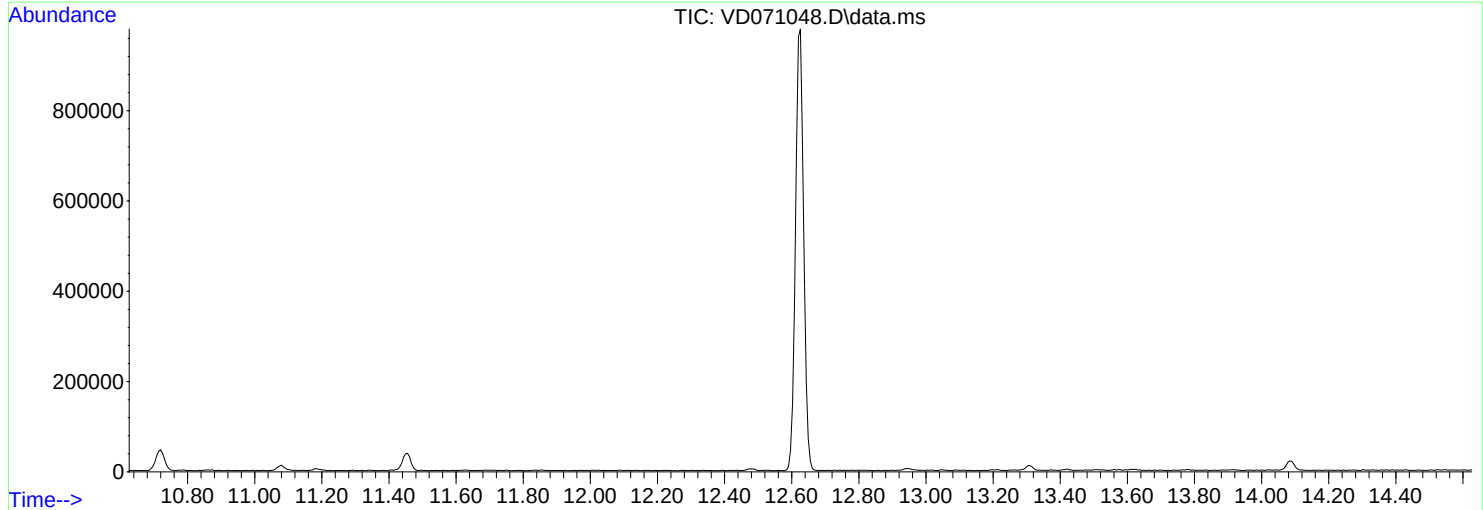

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.4	37528	PASS
75	95	30	60	56.0	86048	PASS
95	95	100	100	100.0	153664	PASS
96	95	5	9	6.7	10350	PASS
173	174	0.00	2	1.4	1645	PASS
174	95	50	100	77.4	118984	PASS
175	174	5	9	7.9	9395	PASS
176	174	95	101	97.8	116389	PASS
177	176	5	9	7.4	8601	PASS