


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD112019\
 Data File : VD064304.D
 Acq On : 20 Nov 2019 09:39
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
 Title : SW846 8260
 Last Update : Tue Nov 12 02:43:24 2019

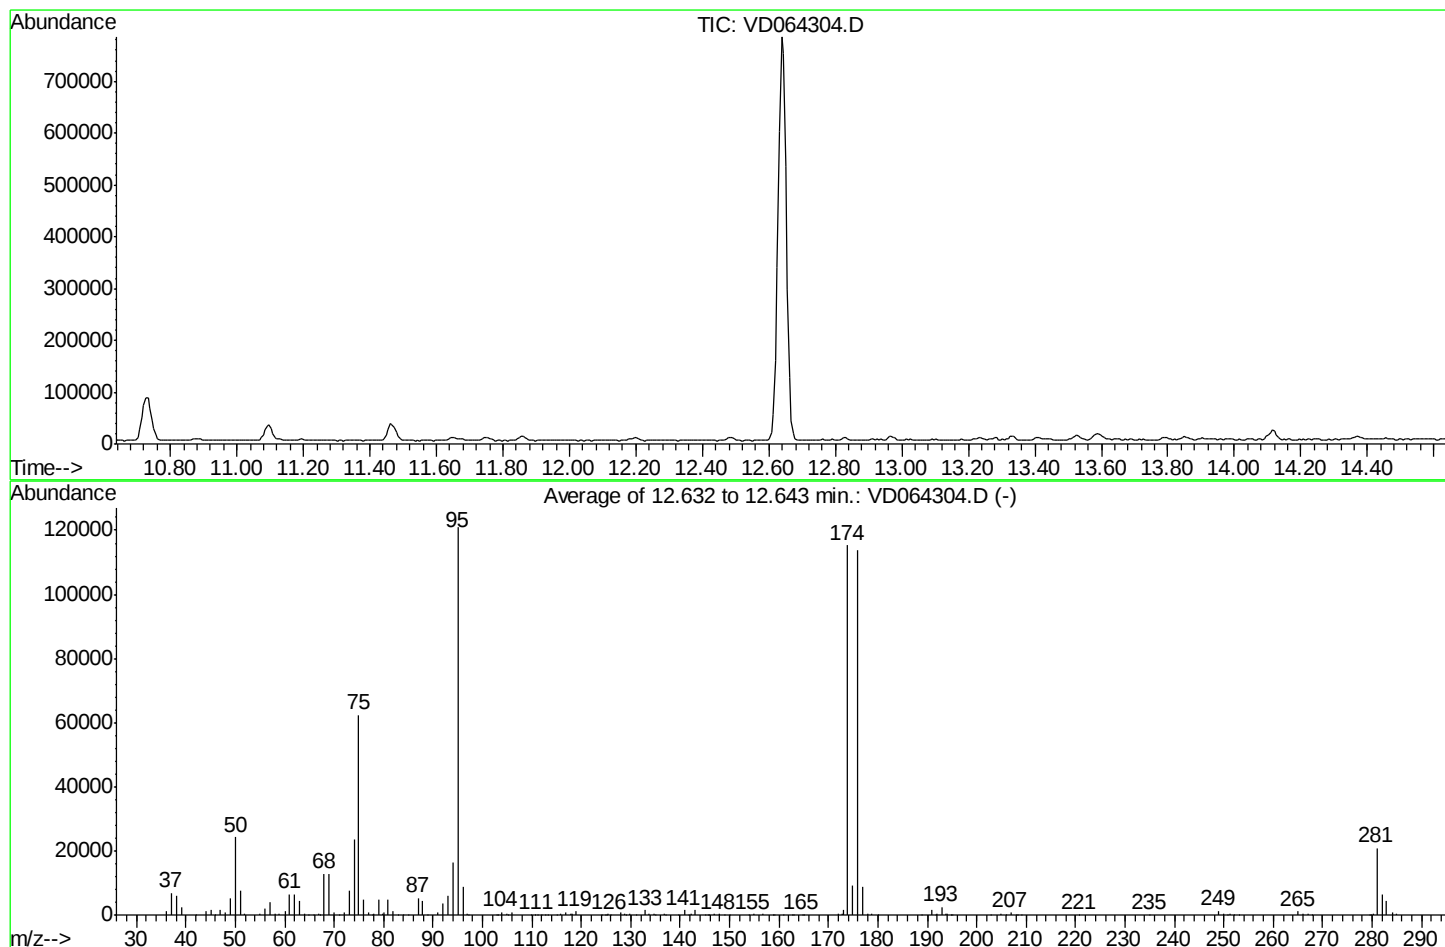

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	24192	PASS
75	95	30	60	51.6	62418	PASS
95	95	100	100	100.0	120922	PASS
96	95	5	9	7.2	8647	PASS
173	174	0.00	2	1.5	1759	PASS
174	95	50	100	95.3	115216	PASS
175	174	5	9	8.1	9332	PASS
176	174	95	101	98.6	113613	PASS
177	176	5	9	7.8	8857	PASS