


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD112020\
 Data File : VD067715.D
 Acq On : 20 Nov 2020 09:01
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110320S.M
 Title : SW846 8260
 Last Update : Sat Nov 21 00:19:04 2020

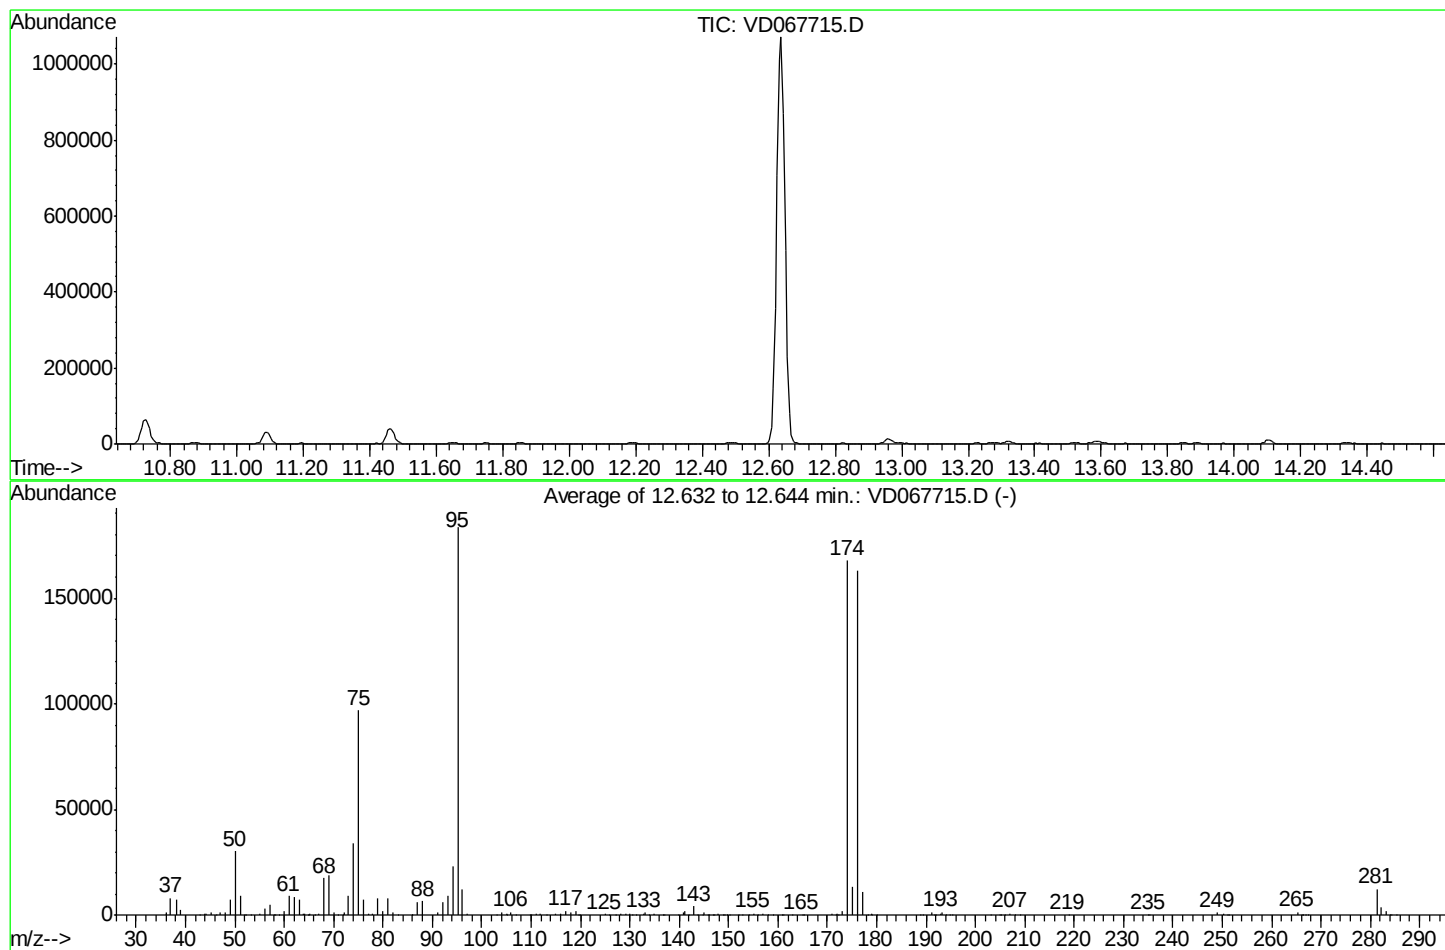

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	30269	PASS
75	95	30	60	52.7	96722	PASS
95	95	100	100	100.0	183530	PASS
96	95	5	9	6.6	12117	PASS
173	174	0.00	2	1.0	1595	PASS
174	95	50	100	91.4	167744	PASS
175	174	5	9	7.8	13104	PASS
176	174	95	101	97.1	162858	PASS
177	176	5	9	6.6	10689	PASS