

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD112118\
 Data File : VD060439.D
 Acq On : 21 Nov 2018 13:40
 Operator : JC/SY
 Sample : J5967-04
 Misc : 5.09g/5ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FDSB-14(16-18)

Quant Time: Nov 22 03:33:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 19 16:31:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-6.43
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-7.46
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.30
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.38
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_D\DATA\VD112118\
Data File : VD060439.D
Acq On : 21 Nov 2018 13:40
Operator : JC/SY
Sample : J5967-04
Misc : 5.09g/5ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FDSB-14(16-18)

Quant Time: Nov 22 03:33:18 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 19 16:31:59 2018
Response via : Initial Calibration

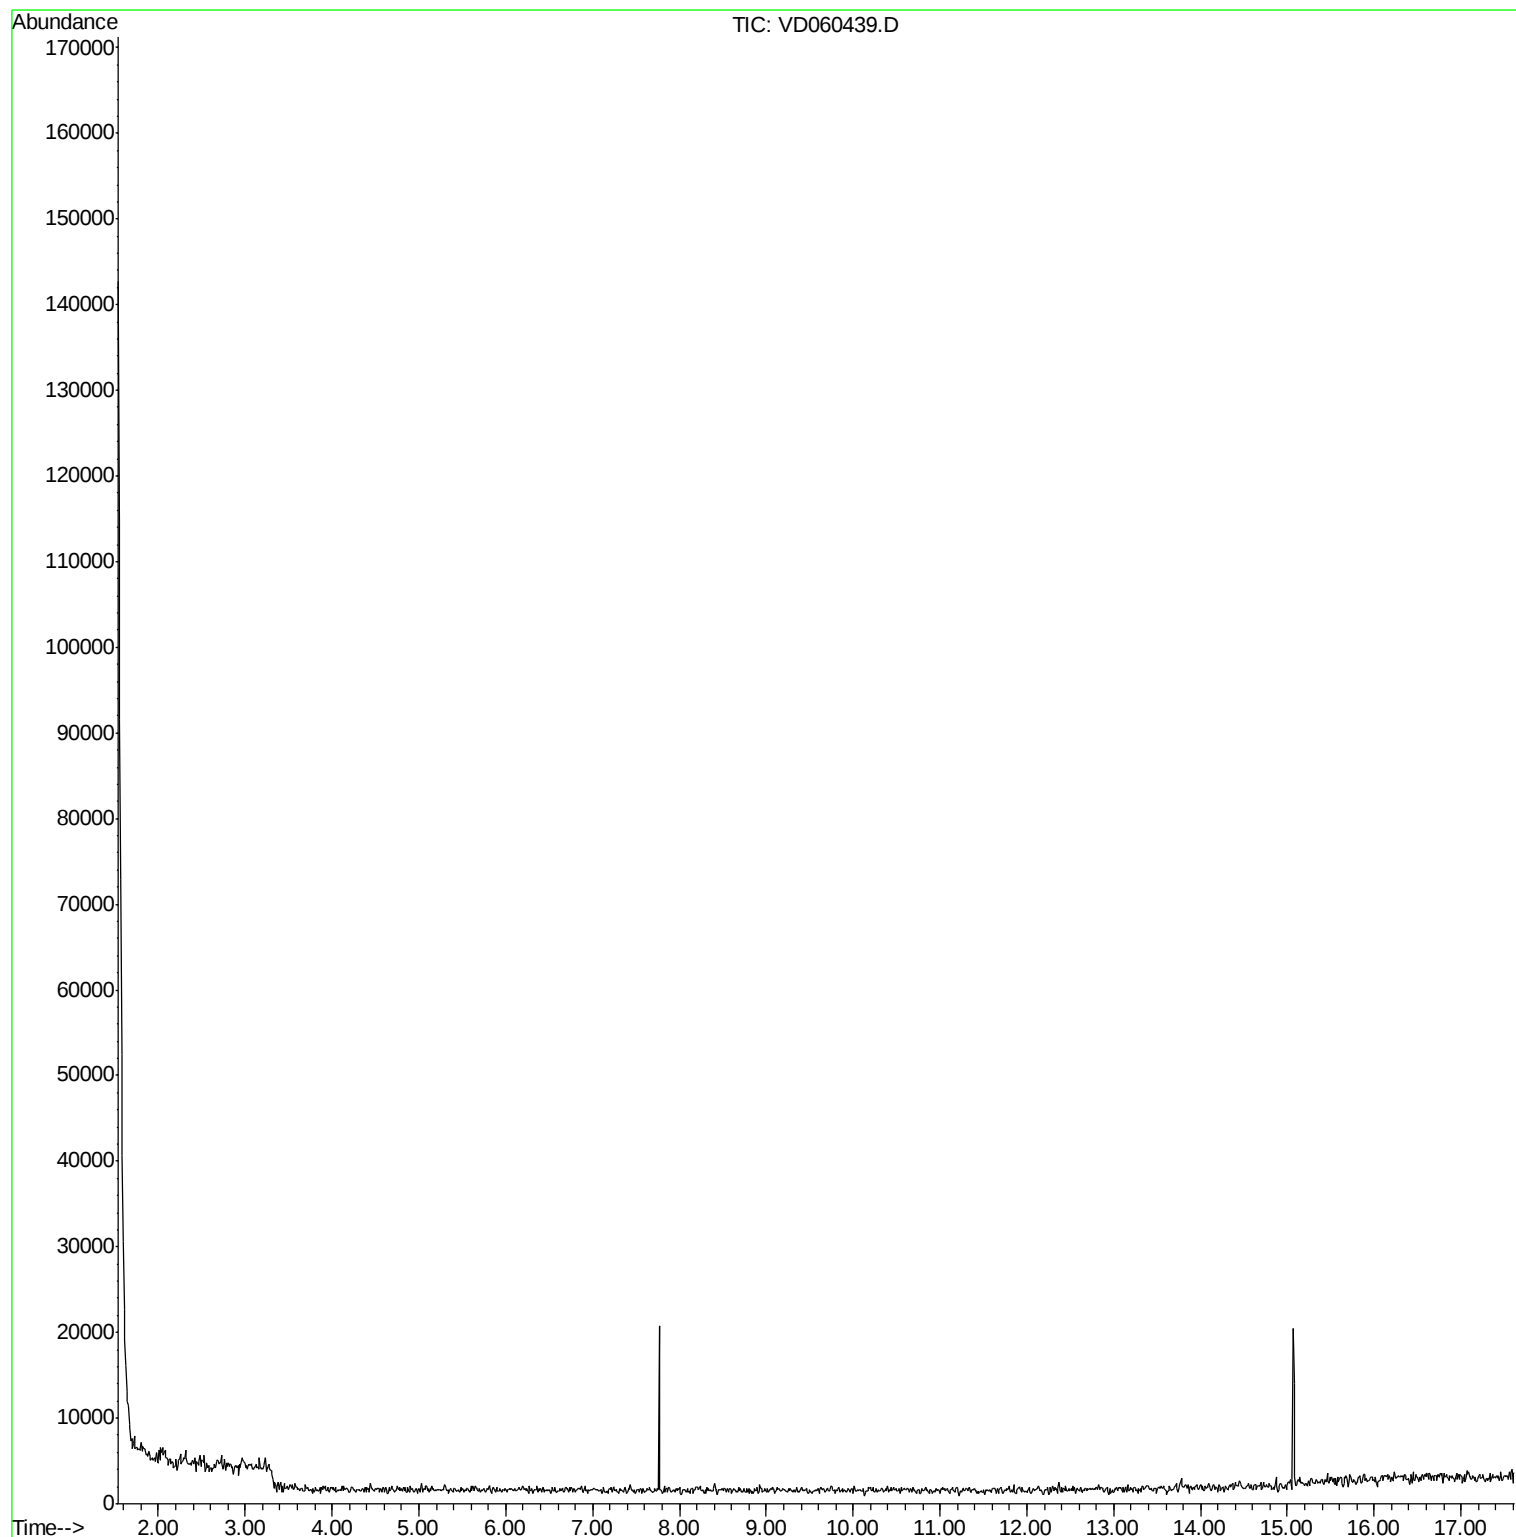

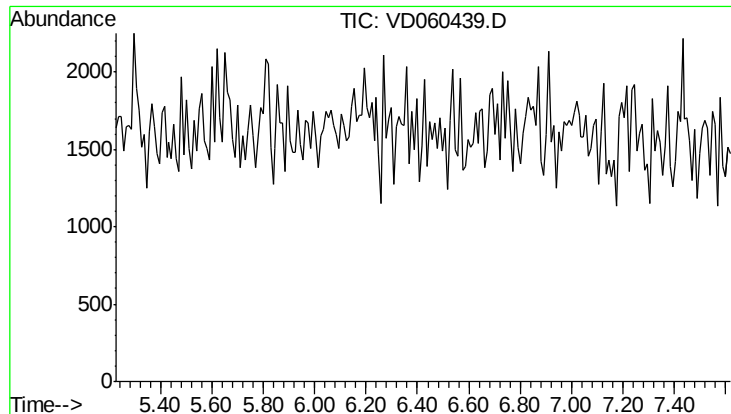

#1

Pentafluorobenzene

Concen: 0.00 ug/l

Expected RT: 6.43 min

Lab File: VD060439.D

Acq: 21 Nov 2018 13:40

Tgt Ion: 168

Sig Exp Ratio

168 100



99 49.8

Instrument :

MSVOA_D

ClientSampleId :

FDSB-14(16-18)

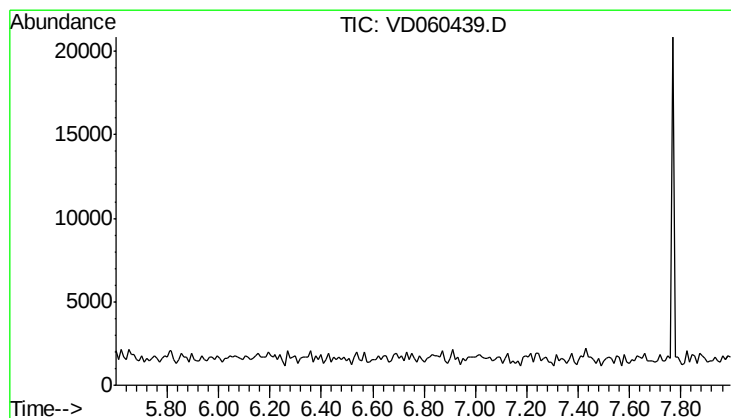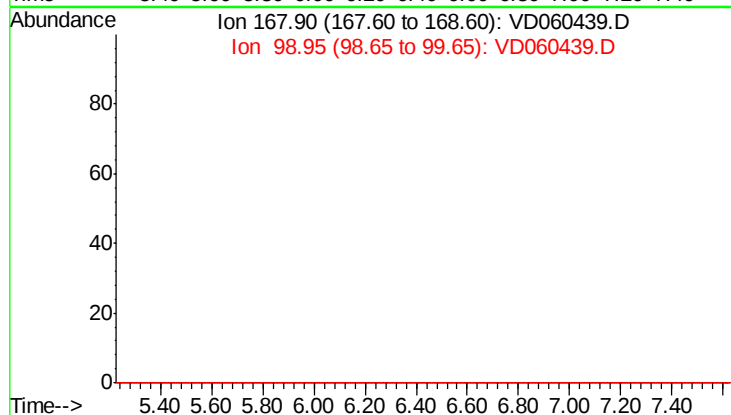

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

Expected RT: 6.80 min

Lab File: VD060439.D


Acq: 21 Nov 2018 13:40


Tgt Ion: 65

Sig Exp Ratio

65 100

67 54.9


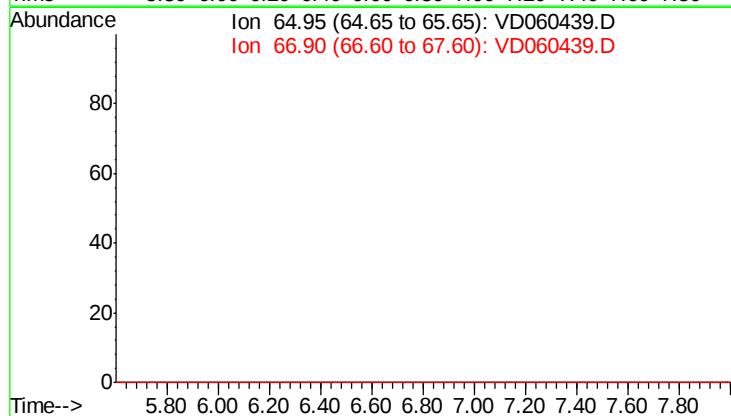


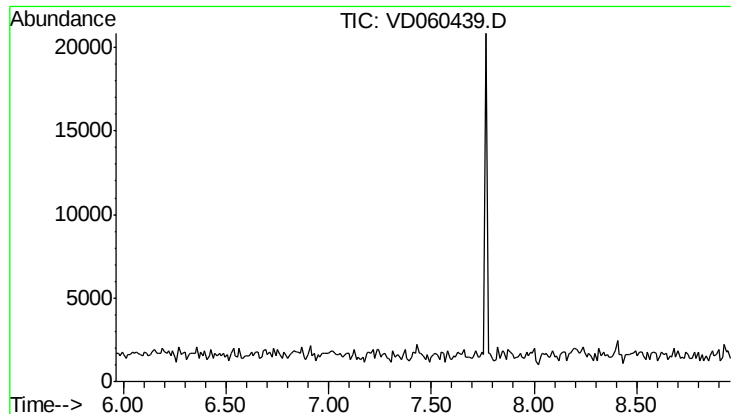

#34
 1,4-Difluorobenzene
 Concen: 0.00 ug/l
 Expected RT: 7.46 min
 Lab File: VD060439.D
 Acq: 21 Nov 2018 13:40


Instrument :
 MSVOA_D
 ClientSampleId :
 FDSB-14(16-18)


Tgt Ion: 114
 Sig Exp Ratio
 114 100
 63 17.0
 88 17.7

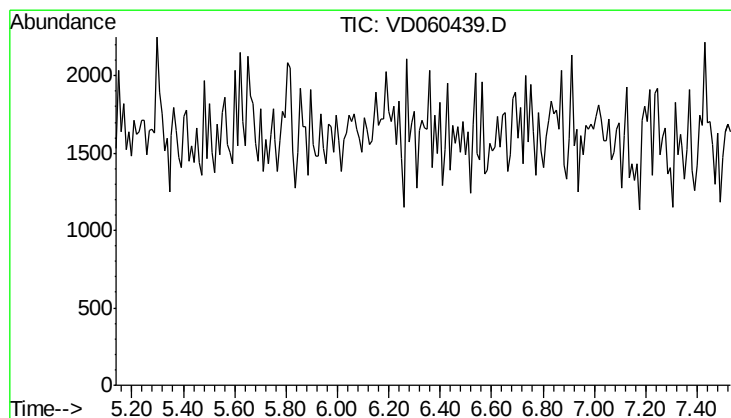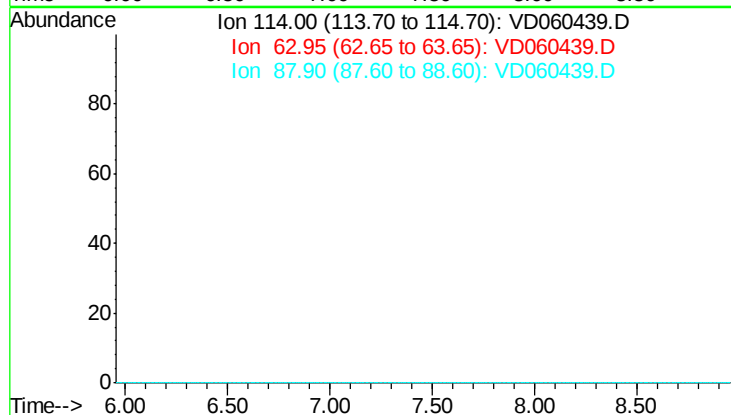

#35
 Dibromofluoromethane
 Concen: 0.00 ug/l
 Expected RT: 6.34 min
 Lab File: VD060439.D
 Acq: 21 Nov 2018 13:40

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 102.0
 192 20.6

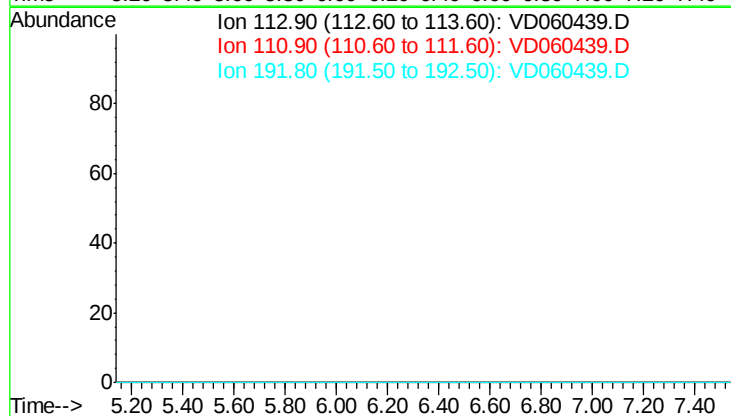


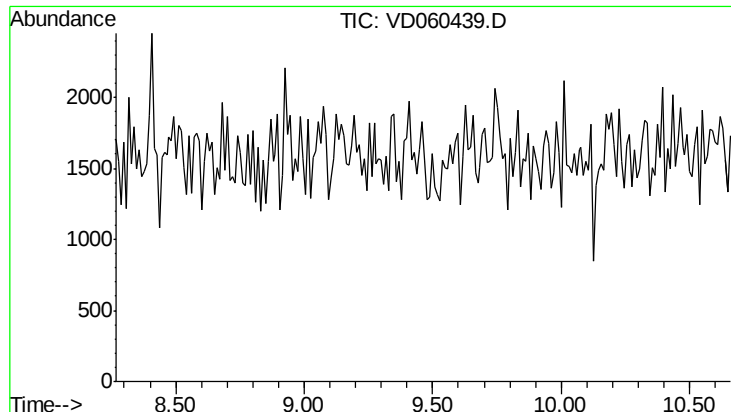


#50
Toluene-d8
Concen: N.D. ug/l
Expected RT: 9.47 min

Lab File: VD060439.D
Acq: 21 Nov 2018 13:40

Instrument :
MSVOA_D
ClientSampleId :
FDSB-14(16-18)


Tgt Ion: 98
Sig Exp Ratio
98 100
100 69.0

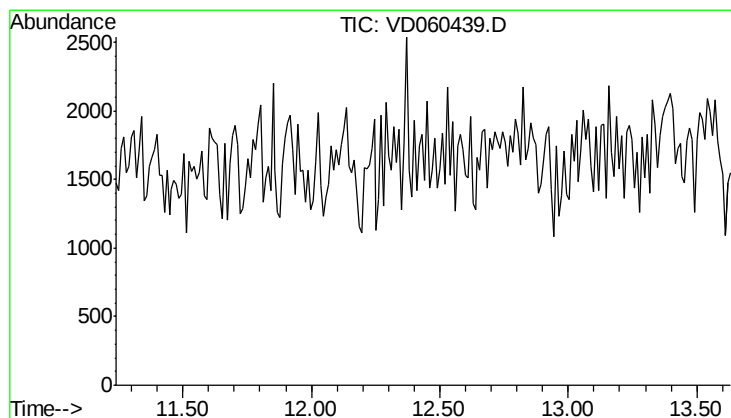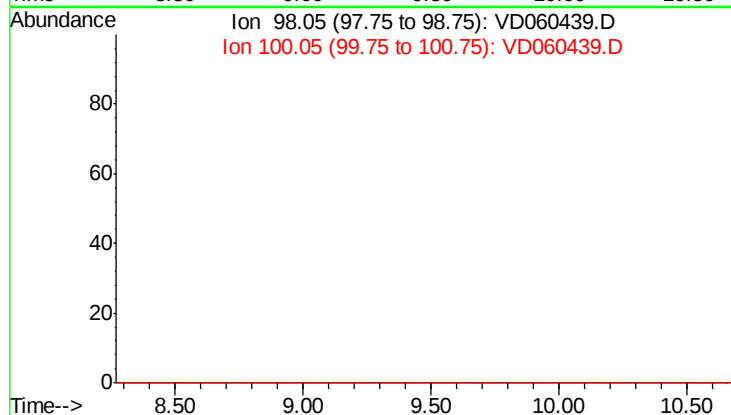


#62
4-Bromofluorobenzene
Concen: N.D. ug/l
Expected RT: 12.44 min

Lab File: VD060439.D
Acq: 21 Nov 2018 13:40

Tgt Ion: 95
Sig Exp Ratio
95 100
174 80.4
176 77.3

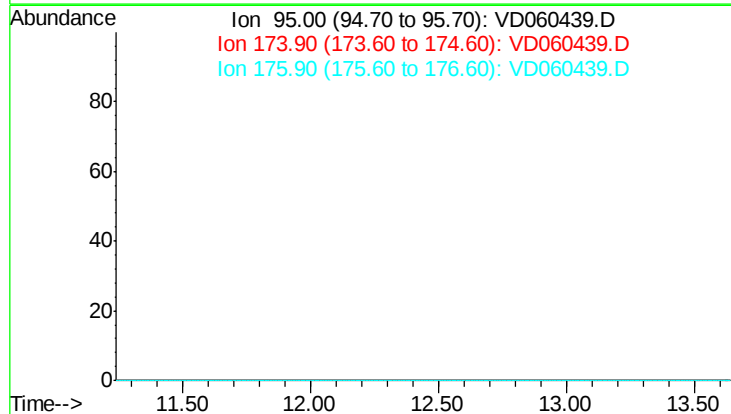


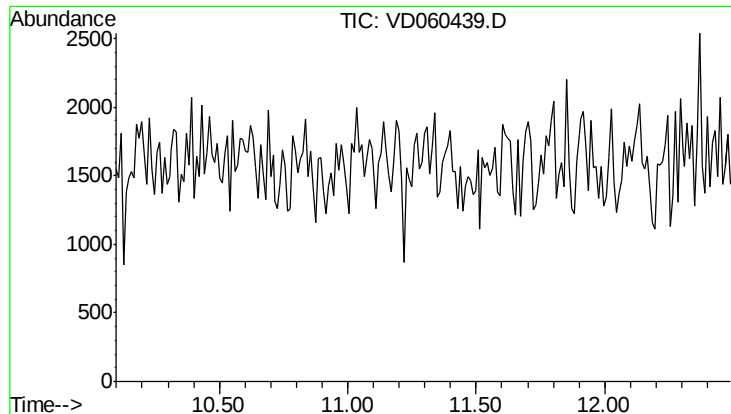


#63
 Chlorobenzene-d5
 Concen: 0.00 ug/l
 Expected RT: 11.30 min

Lab File: VD060439.D
 Acq: 21 Nov 2018 13:40

Instrument :
 MSVOA_D
 ClientSampleId :
 FDSB-14(16-18)

Tgt Ion: 117
 Sig Exp Ratio
 117 100
 82 54.6
 119 32.6

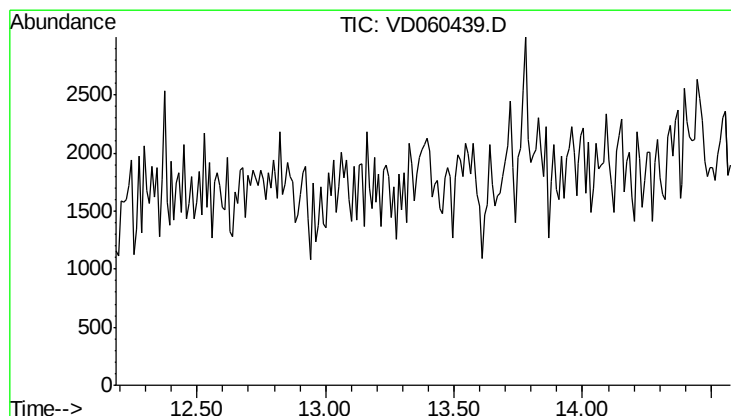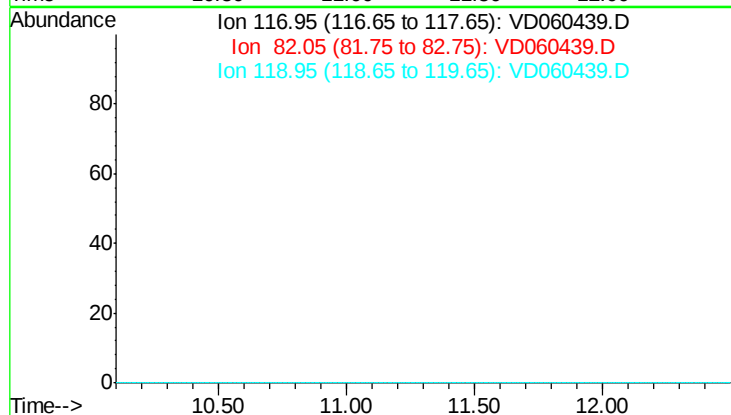

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ug/l
 Expected RT: 13.38 min

Lab File: VD060439.D
 Acq: 21 Nov 2018 13:40

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 48.2
 150 155.3

