


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD112118\
Data File : VD060433.D
Acq On : 21 Nov 2018 10:17
Operator : JC/SY
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Title : SW846 8260
Last Update : Mon Nov 19 16:31:59 2018

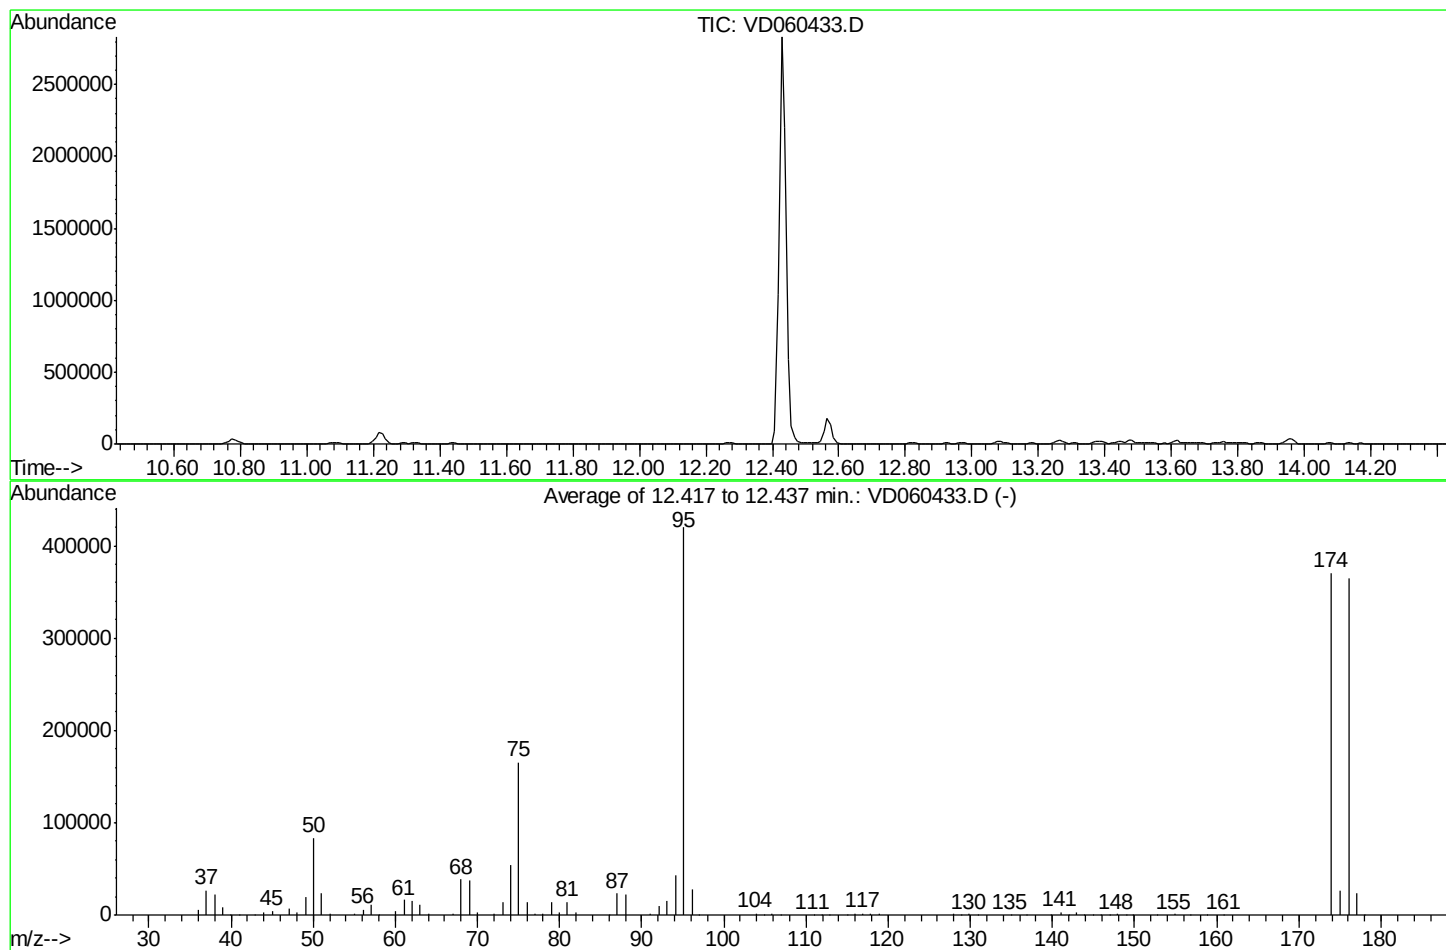

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	83562	PASS
75	95	30	60	39.4	165408	PASS
95	95	100	100	100.0	419968	PASS
96	95	5	9	6.8	28426	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.3	370888	PASS
175	174	5	9	7.2	26766	PASS
176	174	95	101	98.3	364704	PASS
177	176	5	9	6.5	23782	PASS