


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD112119\
Data File : VD064320.D
Acq On : 21 Nov 2019 12:09
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Title : SW846 8260
Last Update : Tue Nov 12 02:43:24 2019

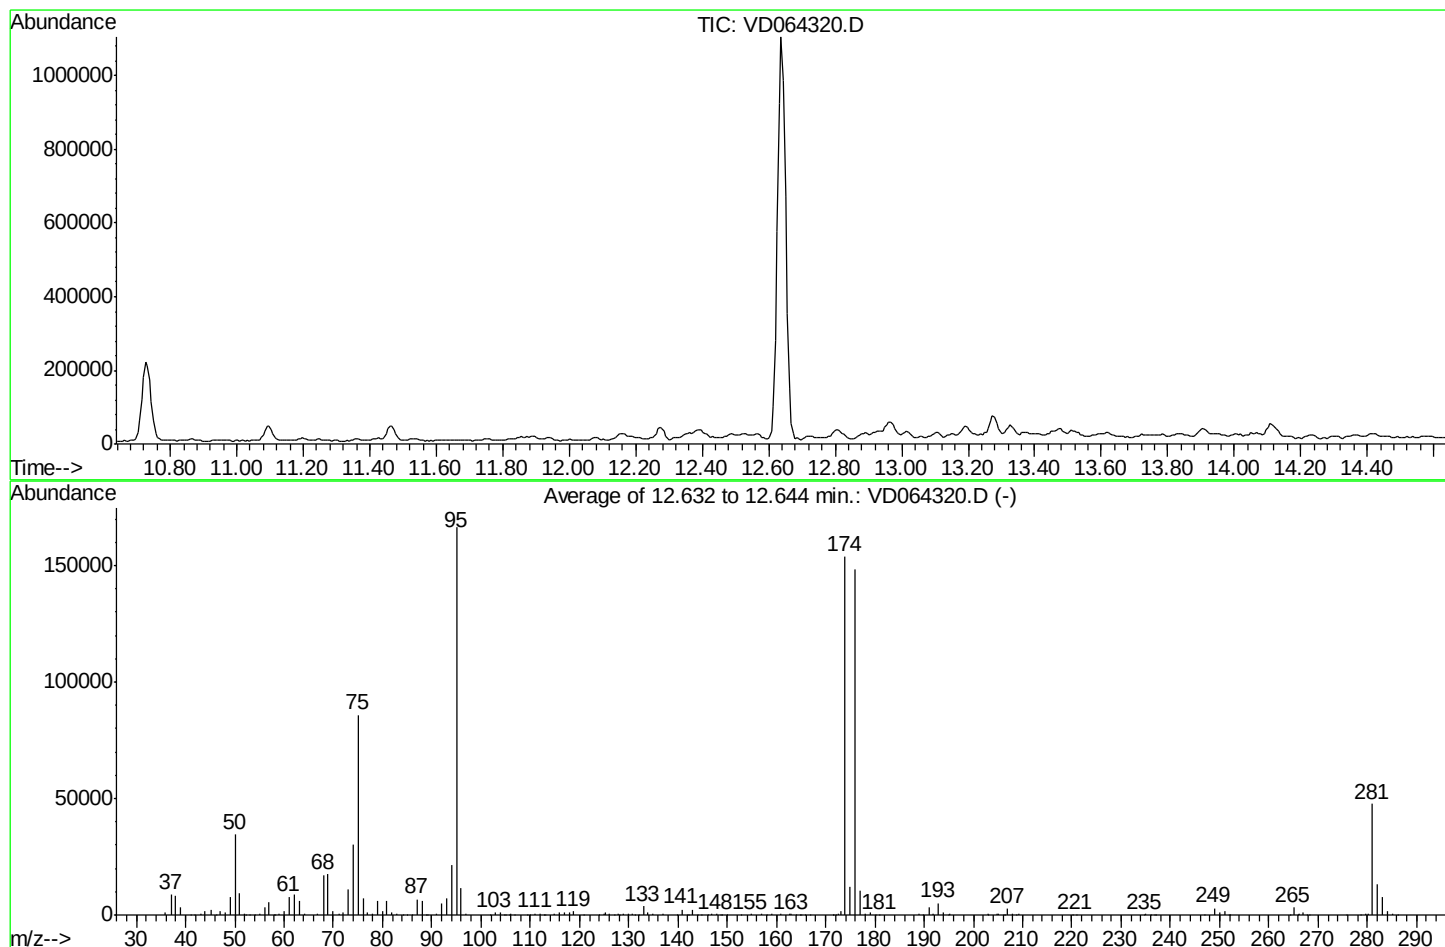

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	34450	PASS
75	95	30	60	51.5	85770	PASS
95	95	100	100	100.0	166440	PASS
96	95	5	9	7.0	11672	PASS
173	174	0.00	2	1.1	1748	PASS
174	95	50	100	92.5	153877	PASS
175	174	5	9	8.0	12328	PASS
176	174	95	101	96.5	148520	PASS
177	176	5	9	7.0	10402	PASS