




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112123\
 Data File : VD077650.D
 Acq On : 21 Nov 2023 17:28
 Operator : JC/SY
 Sample : 05459-06RE
 Misc : 4.25G/10ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AA4RE

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:42:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 22 01:40:25 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/22/2023
 Supervised By :Semsettin Yesilyurt 11/22/2023

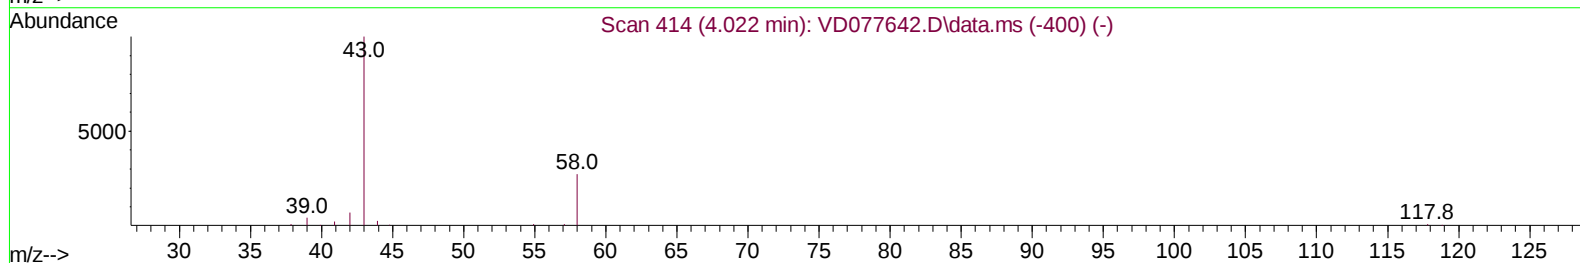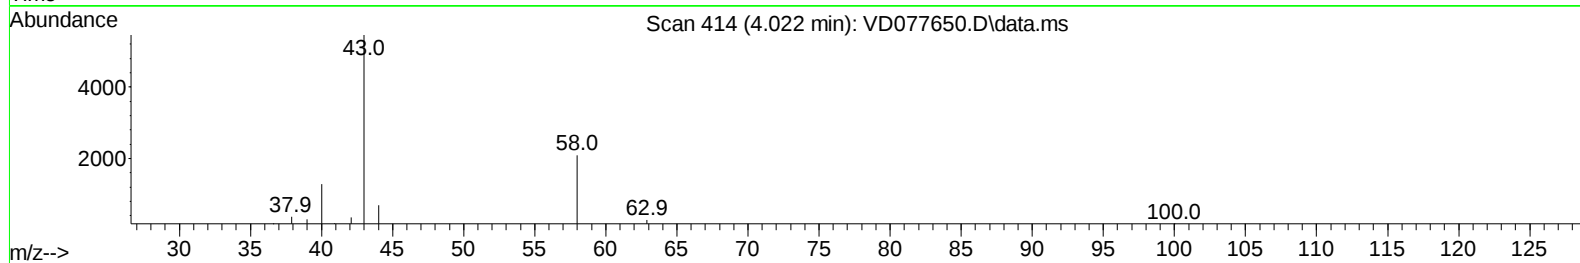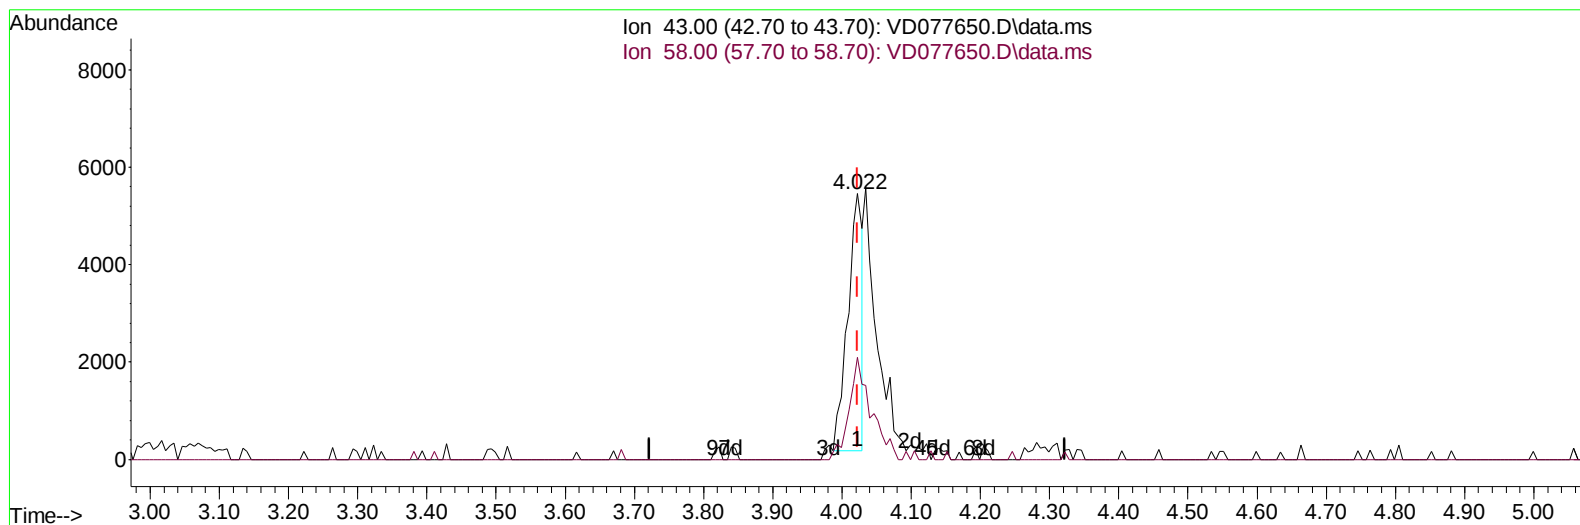

TIC: VD077650.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 4.75 ug/L

response 7612

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	46.02
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112123\
 Data File : VD077650.D
 Acq On : 21 Nov 2023 17:28
 Operator : JC/SY
 Sample : 05459-06RE
 Misc : 4.25G/10ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AA4RE

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:42:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 22 01:40:25 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/22/2023
 Supervised By :Semsettin Yesilyurt 11/22/2023

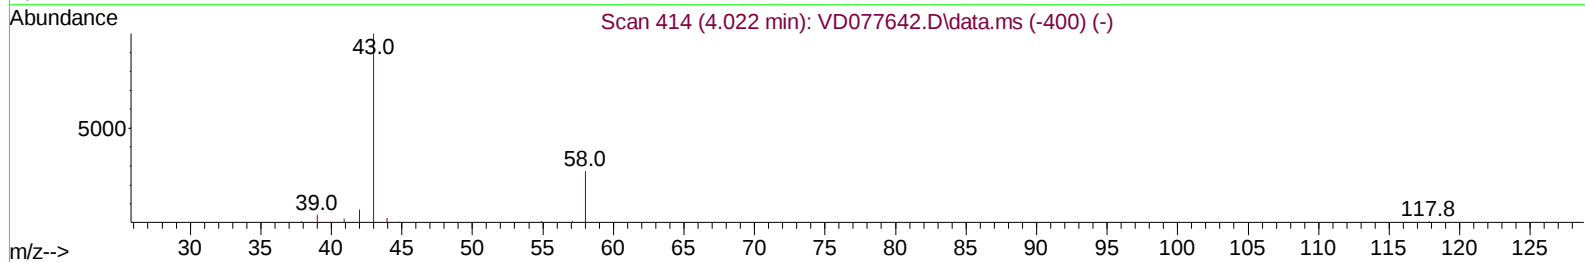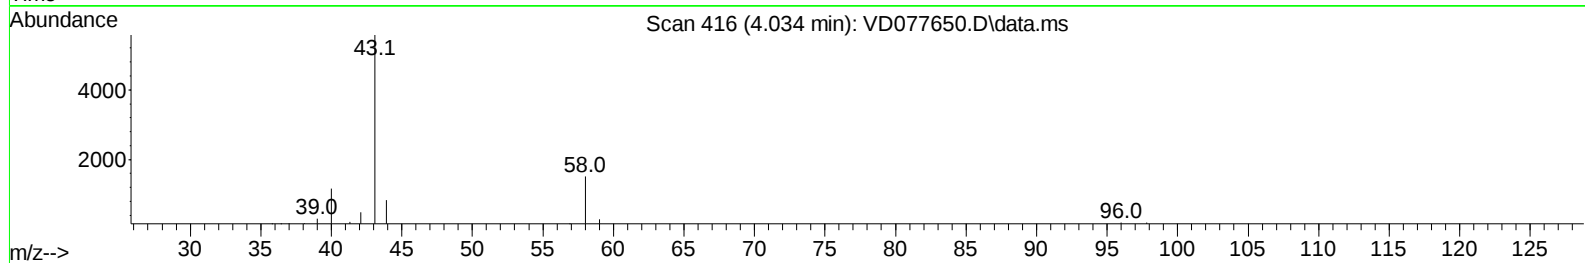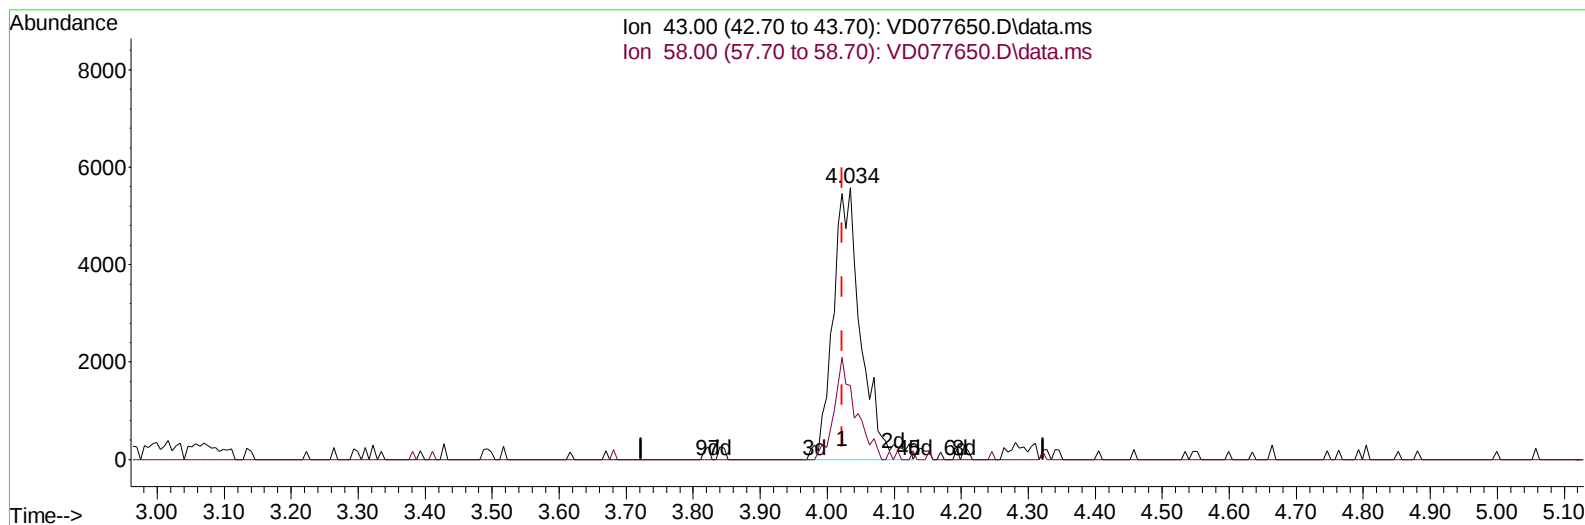

TIC: VD077650.D\data.ms

(13) Acetone (T)

4.034min (+ 0.012) 10.13 ug/L m

response 16215

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	21.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112123\
 Data File : VD077650.D
 Acq On : 21 Nov 2023 17:28
 Operator : JC/SY
 Sample : 05459-06RE
 Misc : 4.25G/10ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AA4RE

Manual IntegrationsAPPROVED

Quant Time: Nov 22 01:42:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 22 01:40:25 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/22/2023
 Supervised By :Semsettin Yesilyurt 11/22/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		345807	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		265332	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		83718	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.281	65		131516	14.950	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	59.800%		
7) Chloroethane-d5	2.811	69		127072	18.388	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	73.560%		
11) 1,1-Dichloroethene-d2	3.922	65		42490	15.620	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	62.480%		
21) 2-Butanone-d5	6.993	46		40956	26.891	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	53.780%		
24) Chloroform-d	7.569	84		196066	19.627	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	78.520%		
26) 1,2-Dichloroethane-d4	8.234	65		91162	17.156	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	68.640%#		
32) Benzene-d6	8.204	84		387903	22.525	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	90.120%		
36) 1,2-Dichloropropane-d6	9.210	67		127030	22.646	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	90.600%		
41) Toluene-d8	10.275	98		320040	20.566	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.280%		
43) trans-1,3-Dichloroprop...	10.528	79		36653	15.155	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	60.600%		
47) 2-Hexanone-d5	10.881	63		30642	30.536	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	61.080%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84		63666	17.131	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	68.520%		
66) 1,2-Dichlorobenzene-d4	13.816	152		62811	21.090	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	84.360%		
Target Compounds							
13) Acetone	4.034	43		16215m	10.129	ug/L	
16) Methylene chloride	4.805	84		37636	6.446	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112123\
Data File : VD077650.D
Acq On : 21 Nov 2023 17:28
Operator : JC/SY
Sample : 05459-06RE
Misc : 4.25G/10ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0AA4RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/22/2023
Supervised By :Semsettin Yesilyurt 11/22/2023

Quant Time: Nov 22 01:42:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 22 01:40:25 2023
Response via : Initial Calibration

