

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112123\
 Data File : VD077652.D
 Acq On : 21 Nov 2023 18:21
 Operator : JC/SY
 Sample : 05459-10RE
 Misc : 3.30G/10ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AJ4RE

Quant Time: Nov 22 01:43:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 22 01:40:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	388435	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	336616	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	127367	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.281	65	142565	14.428	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.720%
7) Chloroethane-d5	2.811	69	134316	17.303	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.200%
11) 1,1-Dichloroethene-d2	3.928	65	45043	14.742	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.960%
21) 2-Butanone-d5	6.987	46	52807	30.867	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.740%
24) Chloroform-d	7.569	84	212773	18.962	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.840%
26) 1,2-Dichloroethane-d4	8.234	65	106472	17.839	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.360%
32) Benzene-d6	8.204	84	420802	19.261	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.040%
36) 1,2-Dichloropropane-d6	9.210	67	139851	19.652	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.600%
41) Toluene-d8	10.269	98	361858	18.329	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.320%
43) trans-1,3-Dichloroprop...	10.528	79	49118	16.008	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.040%
47) 2-Hexanone-d5	10.875	63	39797	31.261	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.520%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	82712	17.542	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.160%
66) 1,2-Dichlorobenzene-d4	13.816	152	92598	20.436	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.760%
Target Compounds						Qvalue
16) Methylene chloride	4.810	84	32300	4.925	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112123\
Data File : VD077652.D
Acq On : 21 Nov 2023 18:21
Operator : JC/SY
Sample : 05459-10RE
Misc : 3.30G/10ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0AJ4RE


Quant Time: Nov 22 01:43:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 22 01:40:25 2023
Response via : Initial Calibration

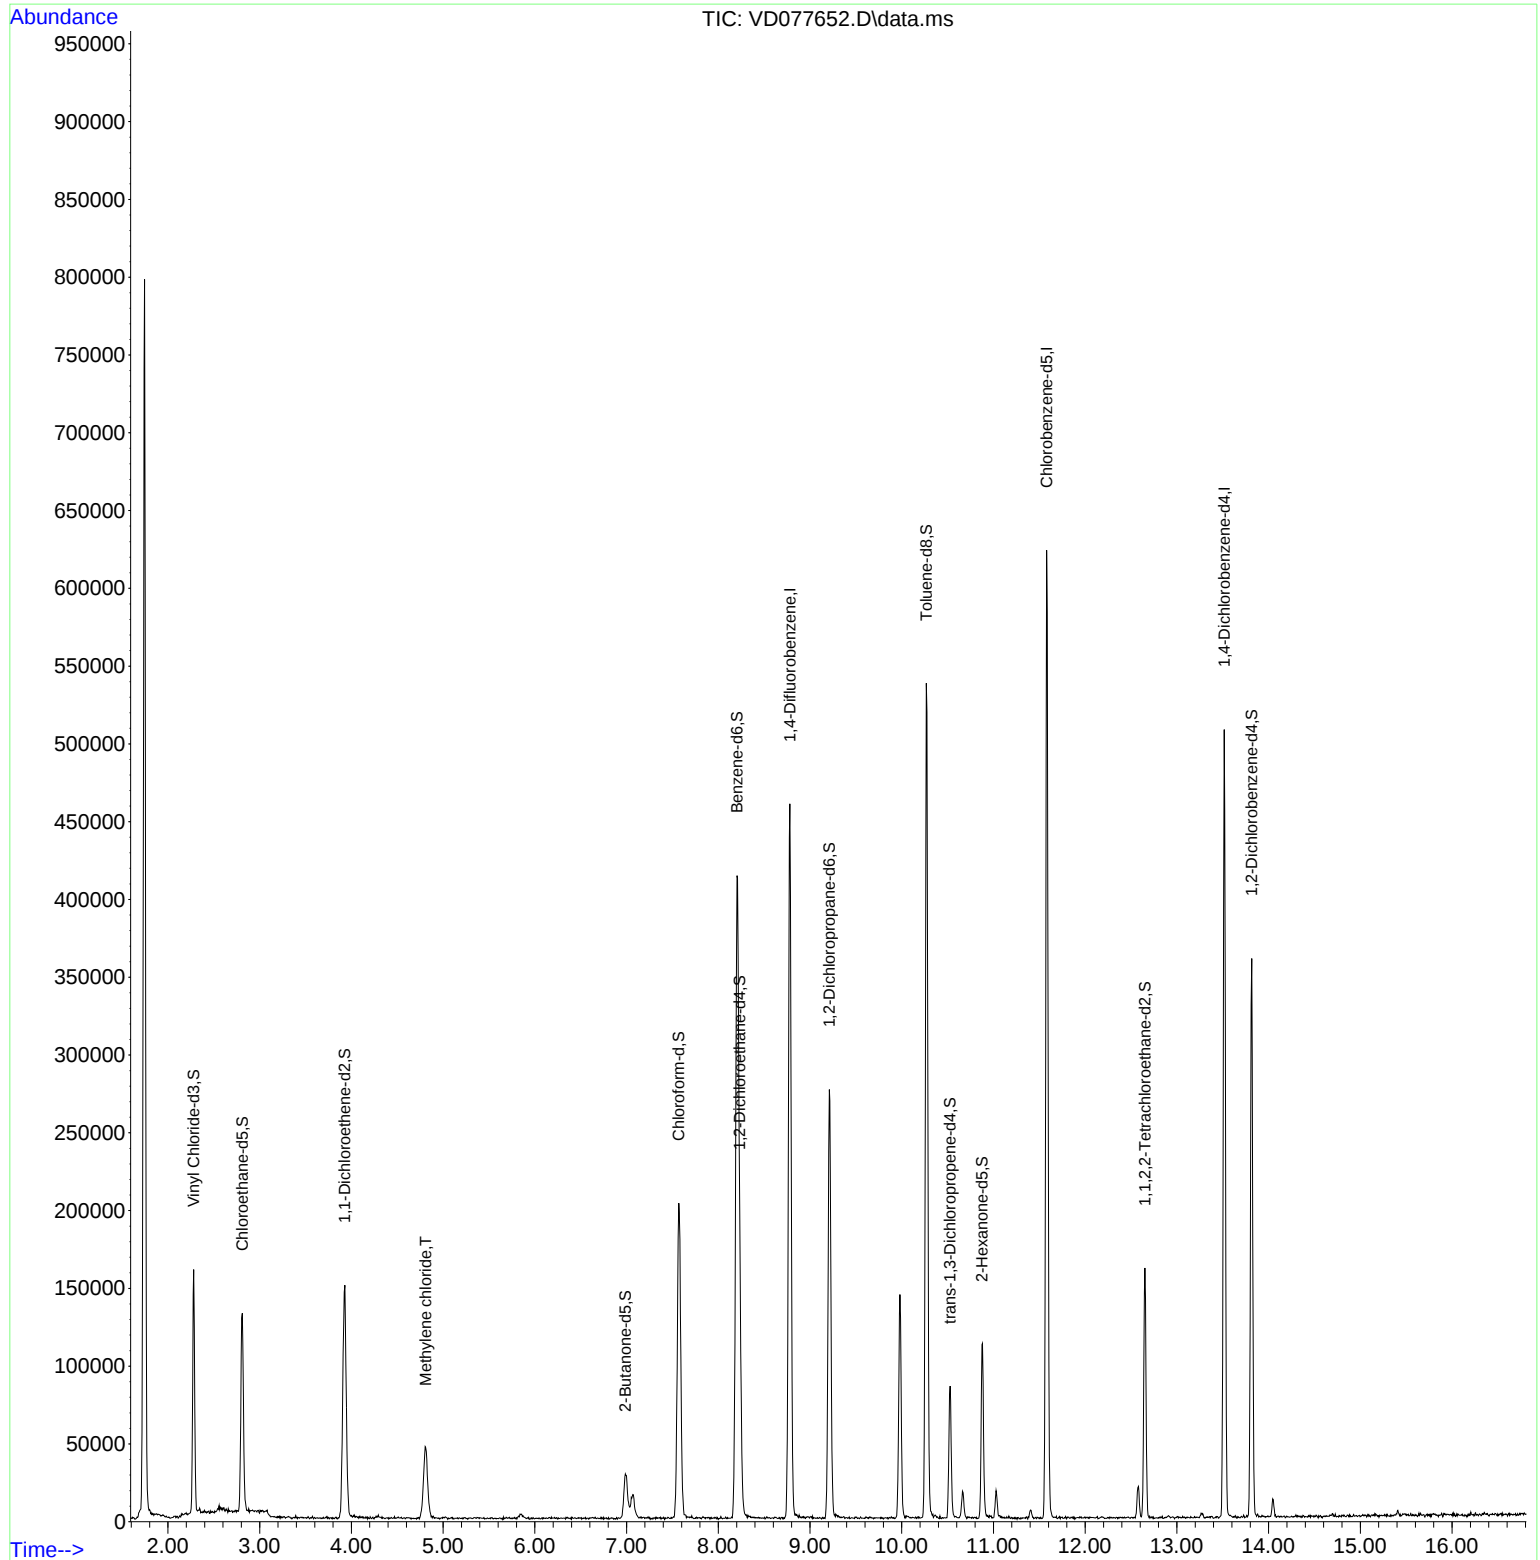

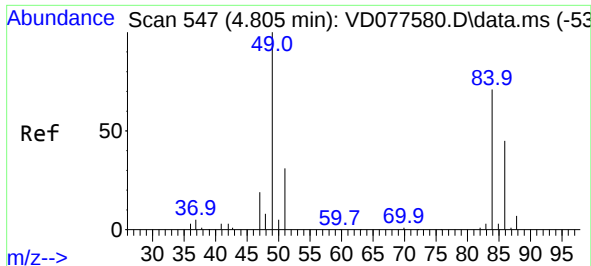

#16
Methylene chloride
Concen: 4.925 ug/L
RT: 4.810 min Scan# 54
Delta R.T. 0.000 min
Lab File: VD077652.D
Acq: 21 Nov 2023 18:21

Instrument :
MSVOA_D
ClientSampleId :
C0AJ4RE

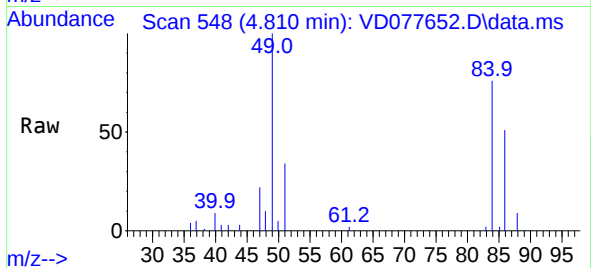

Tgt Ion: 84 Resp: 32300
Ion Ratio Lower Upper
84 100
86 68.1 46.5 86.5
49 132.4 98.3 182.7

