
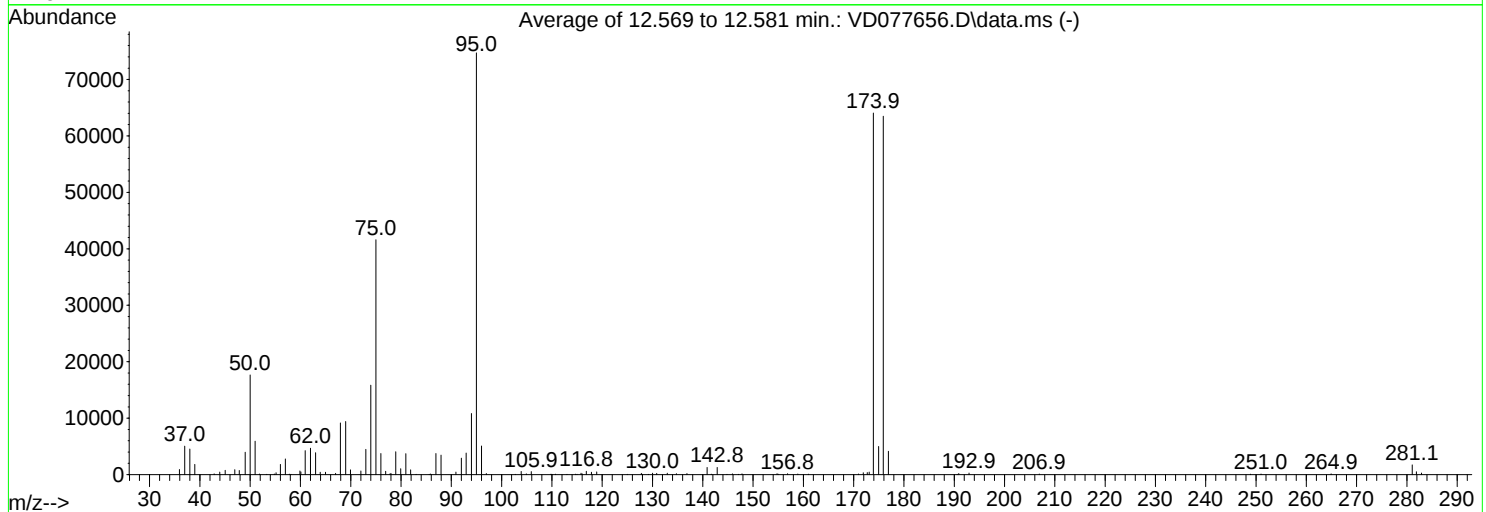


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112223\
Data File : VD077656.D
Acq On : 22 Nov 2023 08:01
Operator : JC/SY
Sample : BFB183
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB183

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM110923SMA.M
Title : SFAM01.0
Last Update : Wed Nov 22 01:40:25 2023

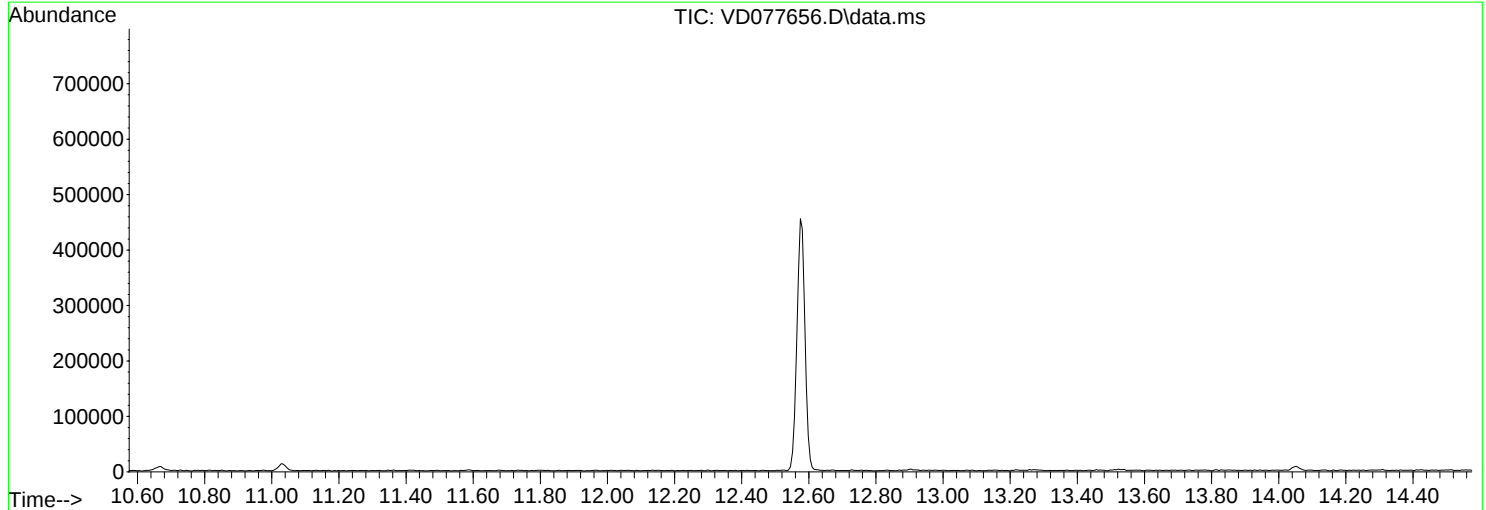

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	17664	PASS
75	95	30	80	55.7	41616	PASS
95	95	100	100	100.0	74715	PASS
96	95	5	9	6.8	5078	PASS
173	174	0.00	2	0.7	471	PASS
174	95	50	120	85.7	64061	PASS
175	174	5	9	7.8	4984	PASS
176	174	95	105	99.1	63477	PASS
177	176	5	10	6.5	4154	PASS

m/z	Abundance
39.90	1741.0
44.00	787.0
51.80	223.0
53.90	184.0
207.00	154.0

Instrument :
MSVOA_D
ClientSampleId :
BFB183

m/z	Abundance
35.90	751.0
37.00	4281.0
38.00	4277.0
39.00	1477.0
40.00	1123.0
43.90	1081.0
45.00	532.0
47.00	1008.0
47.80	543.0
49.00	3470.0
50.00	16336.0
51.00	4490.0
51.90	263.0
53.30	165.0
54.80	356.0
55.10	274.0
56.10	1605.0
57.00	2494.0
59.90	871.0
61.00	3666.0
62.00	4172.0
63.00	3620.0
63.90	463.0
65.00	513.0
67.10	187.0
68.00	7979.0
69.00	8923.0
70.00	784.0
71.90	769.0
73.00	4037.0
74.00	13646.0
75.00	36736.0
76.00	3152.0
77.00	432.0
77.80	397.0
79.00	4048.0
79.90	1065.0
80.90	3321.0
81.90	725.0
85.60	168.0
87.00	2931.0
87.90	2650.0
91.00	504.0
92.00	2077.0
93.00	3322.0
94.00	9486.0
95.00	64536.0
96.00	4611.0
97.00	394.0
103.90	634.0
105.90	602.0
109.80	219.0
113.00	179.0
115.80	302.0
116.80	355.0
117.90	358.0
118.90	519.0
125.00	169.0
127.80	216.0
129.20	185.0
130.90	192.0
136.90	190.0
140.80	1071.0
142.80	1126.0
154.80	229.0
171.00	157.0
171.80	208.0
172.70	1100.0
173.90	53864.0
174.90	4114.0
175.90	52936.0
176.90	3521.0
191.00	262.0
193.00	270.0
207.00	214.0
281.10	981.0
282.00	323.0

Instrument :
MSVOA_D
ClientSampleId :
BFB183

m/z	Abundance
36.00	970.0
37.00	5562.0
38.00	5245.0
39.00	1822.0
39.90	1196.0
42.90	203.0
44.00	1327.0
45.00	945.0
47.00	1059.0
47.90	861.0
49.00	4971.0
50.00	19048.0
51.00	6583.0
51.90	419.0
55.10	433.0
56.00	1994.0
57.00	2847.0
57.80	281.0
59.90	1066.0
60.90	5117.0
62.00	5363.0
63.00	4219.0
64.00	445.0
64.90	411.0
67.00	234.0
68.00	10098.0
69.00	10555.0
70.00	934.0
72.00	617.0
73.00	4712.0
74.00	16496.0
75.00	45224.0
76.00	3829.0
77.10	449.0
78.00	388.0
78.90	4402.0
80.00	939.0
81.00	4164.0
81.90	928.0
85.90	315.0
86.90	4458.0
88.00	3944.0
90.80	565.0
92.00	3944.0
93.00	4051.0
94.00	11951.0
95.00	83096.0
96.00	5258.0
96.90	192.0
104.00	673.0
104.90	225.0
106.00	468.0
110.70	216.0
114.70	226.0
116.00	469.0
116.90	1005.0
117.80	455.0
118.90	578.0
127.80	435.0
130.10	318.0
130.70	232.0
132.90	302.0
134.70	361.0
136.80	191.0
140.90	1104.0
142.80	1321.0
144.80	200.0
146.00	165.0
147.80	202.0
154.70	258.0
156.90	253.0
158.90	188.0
161.00	277.0
171.90	453.0
173.10	1412.0
173.90	68576.0
174.90	5485.0
175.90	68024.0
176.90	4635.0
190.60	174.0
192.90	189.0
206.80	280.0
251.00	157.0
264.90	152.0
281.00	1627.0
281.80	550.0
282.90	526.0

Instrument :
MSVOA_D
ClientSampleId :
BFB183

m/z	Abundance
36.00	1048.0
37.00	5288.0
38.00	4057.0
39.00	2130.0
40.00	1485.0
42.80	201.0
44.00	1338.0
45.10	851.0
46.80	610.0
47.80	803.0
49.00	3508.0
50.00	17608.0
51.00	6731.0
52.00	326.0
55.20	282.0
55.90	1855.0
57.00	3024.0
58.10	203.0
60.10	1426.0
61.00	3958.0
62.00	4457.0
63.00	3812.0
64.00	391.0
65.10	316.0
66.90	308.0
67.90	9431.0
69.00	8741.0
69.90	857.0
72.10	558.0
73.00	4721.0
74.00	17424.0
75.00	42888.0
76.00	4263.0
76.90	897.0
78.00	306.0
78.90	3735.0
79.90	1134.0
80.90	3627.0
81.90	933.0
83.00	157.0
86.90	3805.0
87.90	3803.0
91.00	291.0
92.00	2744.0
92.90	4100.0
94.00	11048.0
95.00	76512.0
96.00	5364.0
102.70	157.0
103.80	366.0
104.90	210.0
105.80	531.0
110.00	171.0
115.00	158.0
115.80	433.0
116.80	470.0
117.80	468.0
118.80	352.0
128.00	175.0
129.90	471.0
130.90	253.0
133.00	475.0
134.80	174.0
136.80	187.0
140.90	1655.0
141.70	223.0
142.90	1411.0
145.80	257.0
147.10	185.0
147.80	215.0
155.00	242.0
156.80	258.0
158.90	159.0
170.90	178.0
172.00	394.0
173.90	69744.0
175.00	5353.0
175.90	69472.0
176.90	4306.0
190.80	363.0
193.00	398.0
206.90	302.0
248.90	252.0
251.00	166.0
265.00	277.0
281.00	2561.0
282.00	663.0
282.90	327.0

Instrument :
MSVOA_D
ClientSampleId :
BFB183