

Data File : VD067773.D
Acq On : 24 Nov 2020 17:37
Operator : VA/SY
Sample : L4858-02
Misc : 5.74G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013

Quant Time: Nov 25 02:05:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112320S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 24 00:51:35 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	45420	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	70489	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	69736	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	31322	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	40528	91.77	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	183.54%#
35) Dibromofluoromethane	7.92	113	28833	64.27	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	128.54%
50) Toluene-d8	10.34	98	75568	46.08	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	92.16%
62) 4-Bromofluorobenzene	12.64	95	27039	48.23	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.46%


Target Compounds			Qvalue			
11) Tert butyl alcohol	5.21	59	124	Below Cal	#	87
16) Acetone	4.16	43	8542	149.722	ug/l #	78
17) Carbon Disulfide	4.41	76	3933	3.647	ug/l #	74
18) Methyl Acetate	4.94	43	718	6.255	ug/l #	38
20) Methylene Chloride	4.98	84	3745	1.675	ug/l #	75
25) 2-Butanone	7.23	43	1137	17.760	ug/l #	37
31) Cyclohexane	8.00	56	4741	8.872	ug/l #	87
36) 1,1-Dichloropropene	7.98	75	2702	4.467	ug/l #	50
37) Ethyl Acetate	7.23	43	1137	6.991	ug/l #	63
38) Carbon Tetrachloride	7.99	117	4750	5.417	ug/l #	12
39) Methylcyclohexane	9.36	83	14779	20.646	ug/l #	89
40) Benzene	8.36	78	2332	1.404	ug/l #	84
43) Isopropyl Acetate	8.47	43	577	1.776	ug/l #	44
48) Methyl methacrylate	9.36	41	6428	39.585	ug/l #	62
55) 1,1,2-Trichloroethane	10.77	97	1655	5.315	ug/l #	18
56) Ethyl methacrylate	10.68	69	858	2.661	ug/l #	1
59) 2-Hexanone	10.96	43	434	4.022	ug/l #	20
68) m/p-Xylenes	11.86	106	2508	2.724	ug/l	88
74) N-amyl acetate	12.27	43	323	1.188	ug/l #	35
75) 1,1,2,2-Tetrachloroethane	12.80	83	321	1.161	ug/l #	25
76) 1,2,3-Trichloropropane	12.64	75	13635	62.460	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.97	105	3036	1.694	ug/l	76
81) trans-1,4-Dichloro-2-buten	12.64	75	13635	146.089	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.27	105	7475	4.175	ug/l	96
90) Hexachloroethane	14.12	117	993	2.662	ug/l #	7
95) Naphthalene	15.40	128	5980	6.068	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VD067773.D
Acq On : 24 Nov 2020 17:37
Operator : VA/SY
Sample : L4858-02
Misc : 5.74G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013

Quant Time: Nov 25 02:05:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112320S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 24 00:51:35 2020
Response via : Initial Calibration

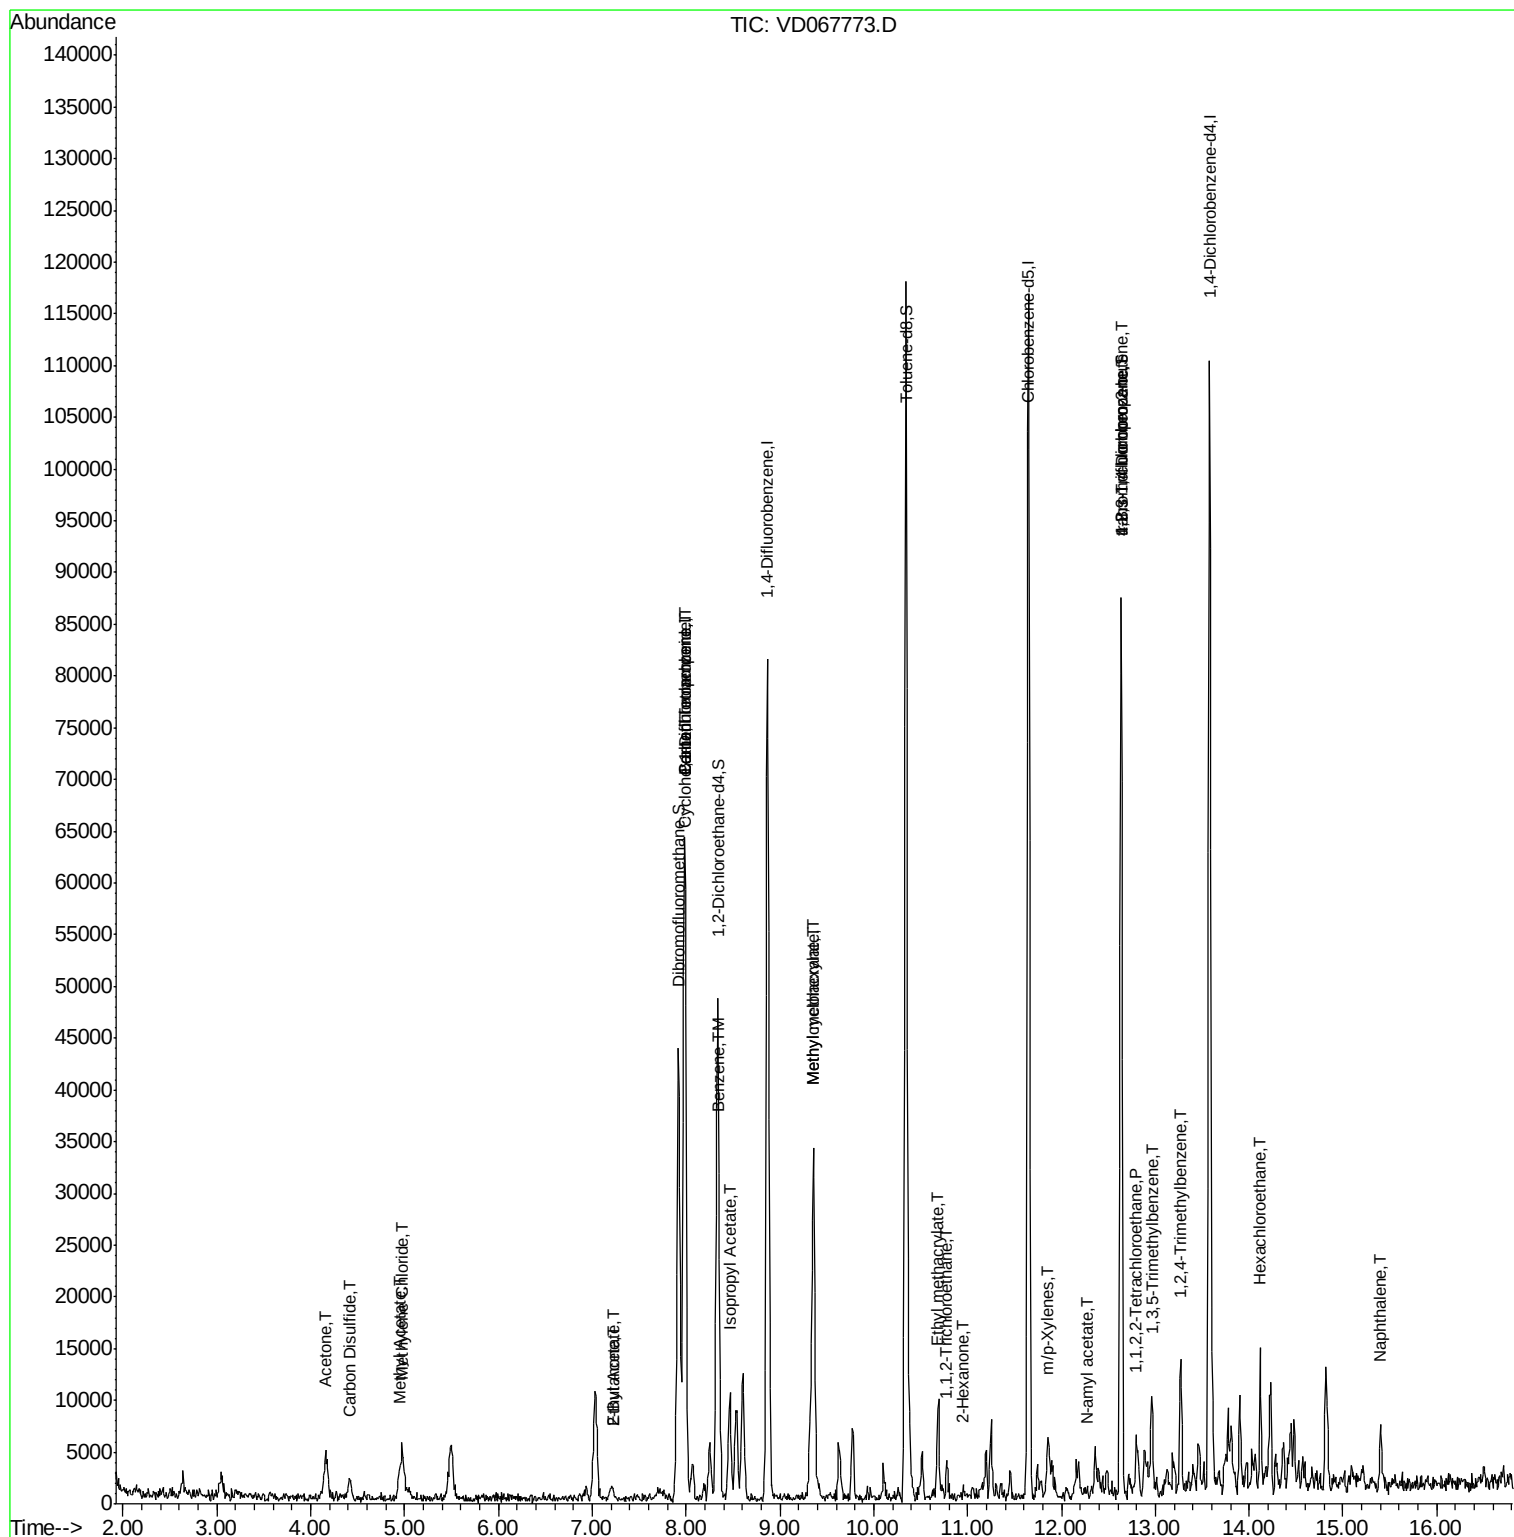



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.01 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :


PHC-340EM-013

Tgt Ion:168 Resp: 45420

Ion Ratio Lower Upper




168 100

99 51.2 43.8 65.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

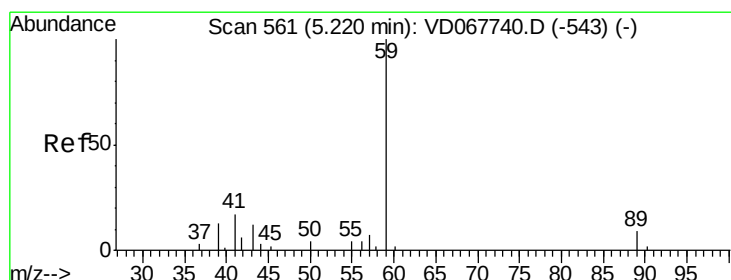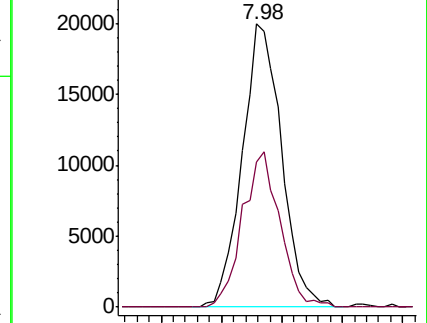

#11

Tert butyl alcohol

Concen: Below Cal

RT: 5.21 min Scan# 560

Delta R.T. -0.01 min

Lab File: VD067773.D


Acq: 24 Nov 2020 17:37

Tgt Ion: 59 Resp: 124

Ion Ratio Lower Upper



59 100


57 0.0 3.4 5.0#



Abundance Ion 59.00 (58.70 to 59.70): VDC

Ion 57.00 (56.70 to 57.70): VDC

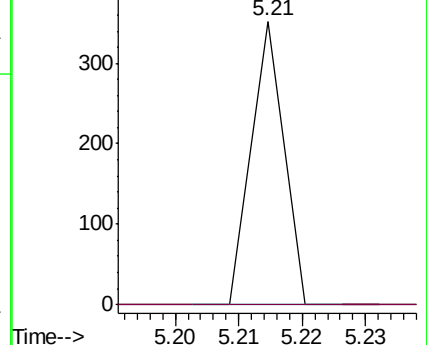

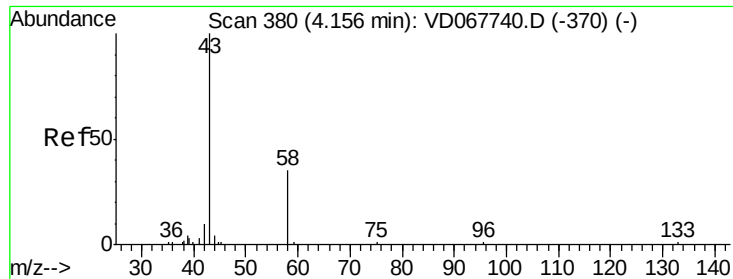

#16

Acetone

Concen: 149.722 ug/l

RT: 4.16 min Scan# 381

Delta R.T. 0.01 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :


PHC-340EM-013

Tgt Ion: 43 Resp: 8542

Ion Ratio Lower Upper




43 100

58 21.8 27.6 41.4#

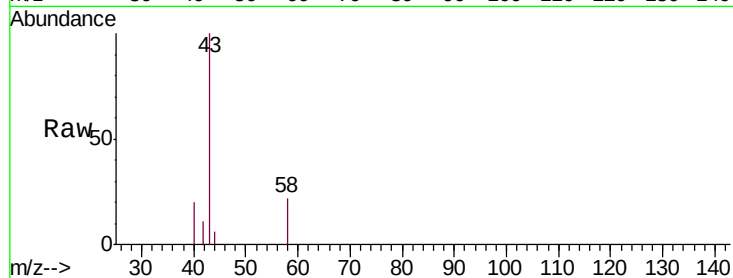

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC

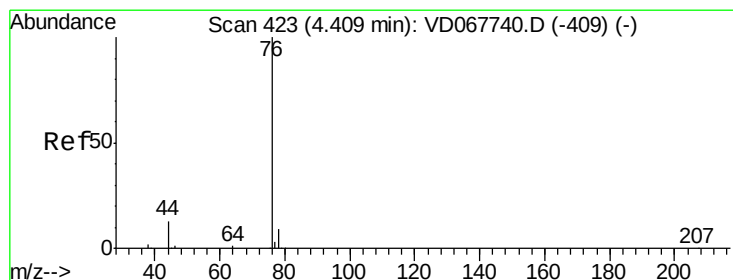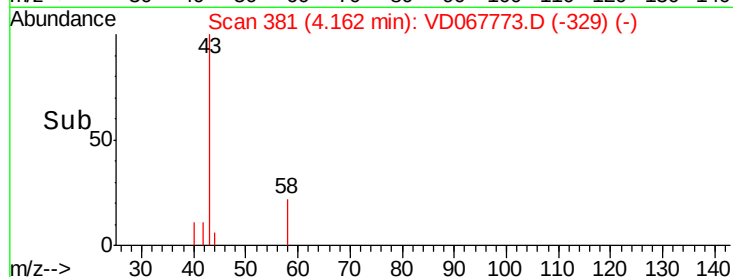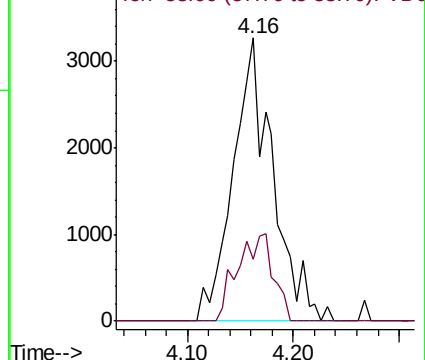

#17

Carbon Disulfide

Concen: 3.647 ug/l

RT: 4.41 min Scan# 423

Delta R.T. 0.00 min

Lab File: VD067773.D


Acq: 24 Nov 2020 17:37

Tgt Ion: 76 Resp: 3933

Ion Ratio Lower Upper



76 100


78 0.0 7.5 11.3#

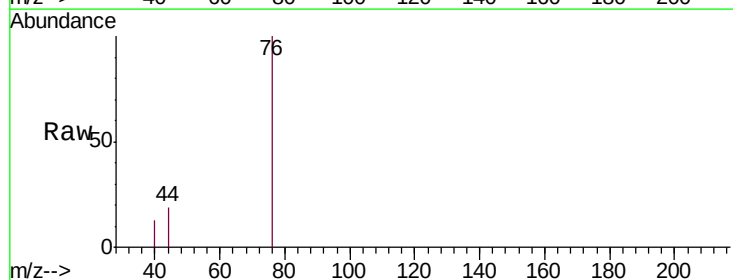

Abundance Ion 75.90 (75.60 to 76.60): VDC

Ion 77.90 (77.60 to 78.60): VDC

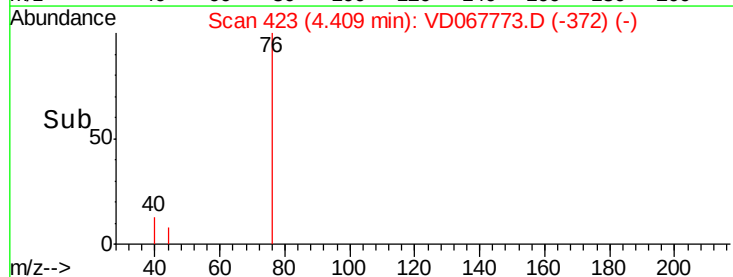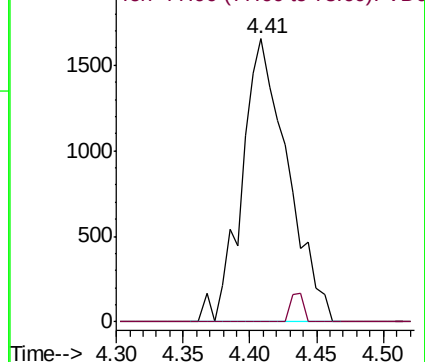

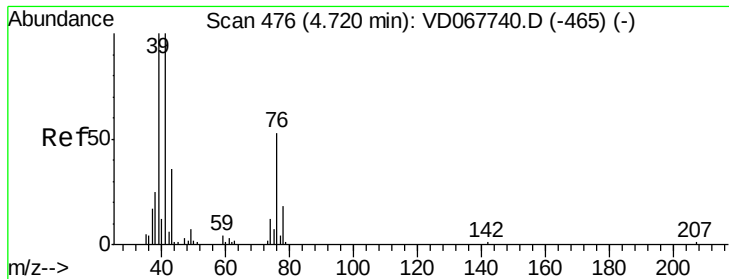

#18

Methyl Acetate

Concen: 6.255 ug/l

RT: 4.94 min Scan# 514

Delta R.T. 0.22 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :


PHC-340EM-013

Tgt Ion: 43 Resp: 718

Ion Ratio Lower Upper

43 100

74 0.0 29.7 44.5#

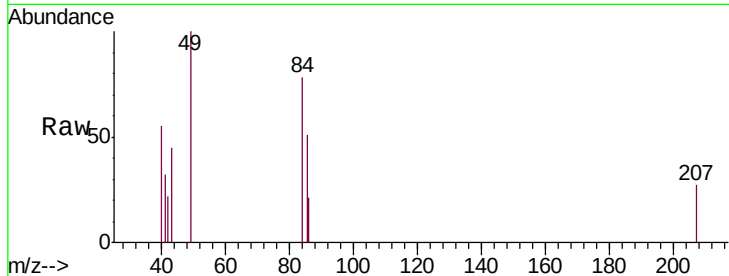

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 74.00 (73.70 to 74.70): VDC

4.94



300

200

100

0

Time-->

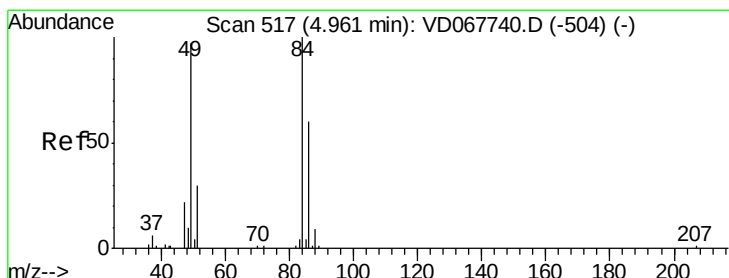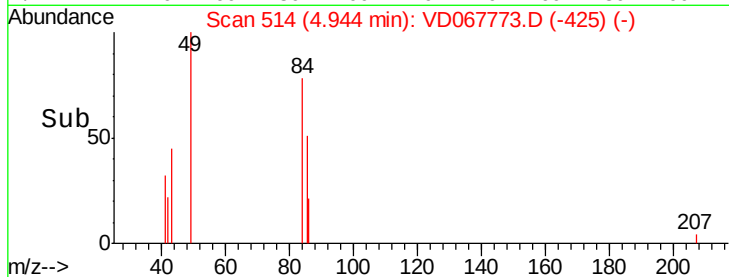

#20

Methylene Chloride

Concen: 1.675 ug/l

RT: 4.98 min Scan# 520

Delta R.T. 0.02 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Tgt Ion: 84 Resp: 3745


Ion Ratio Lower Upper

84 100

49 118.0 77.4 116.2#

51 20.8 24.1 36.1#

86 35.2 48.2 72.2#

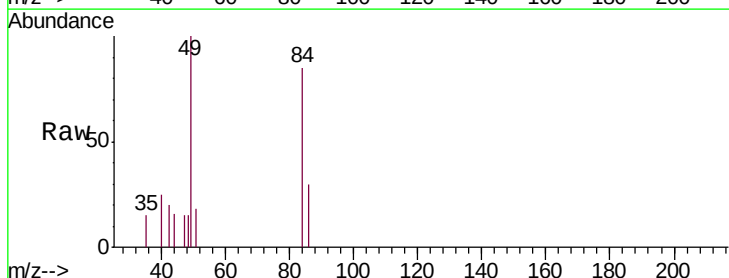

Abundance Ion 83.90 (83.60 to 84.60): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC

2000


1500

1000

500

0

Time-->

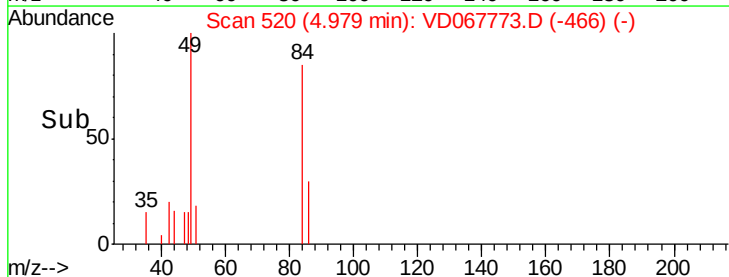


4.98

4.90

4.95

5.00





5.05



#25
2-Butanone
Concen: 17.760 ug/l
RT: 7.23 min Scan# 902
Delta R.T. 0.01 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37




Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013


Tgt Ion: 43 Resp: 1137
Ion Ratio Lower Upper
43 100
72 0.0 30.8 46.2#

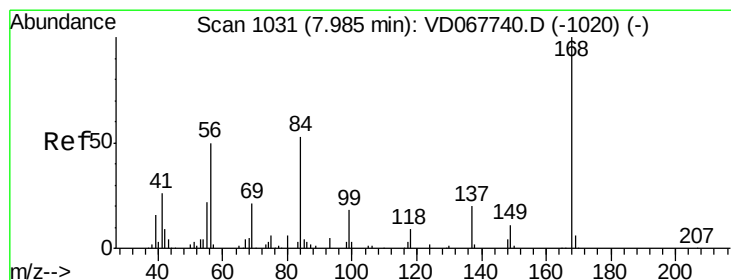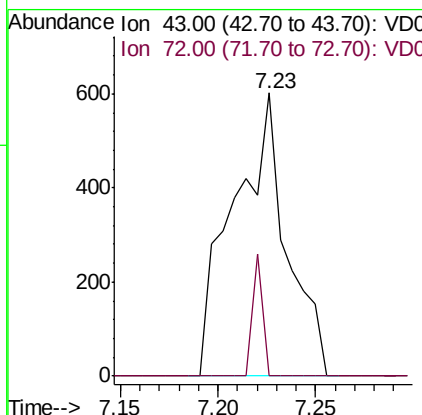

#31
Cyclohexane
Concen: 8.872 ug/l
RT: 8.00 min Scan# 1033
Delta R.T. 0.01 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion: 56 Resp: 4741
Ion Ratio Lower Upper
56 100
69 57.0 33.2 49.8#
84 97.8 84.8 127.2



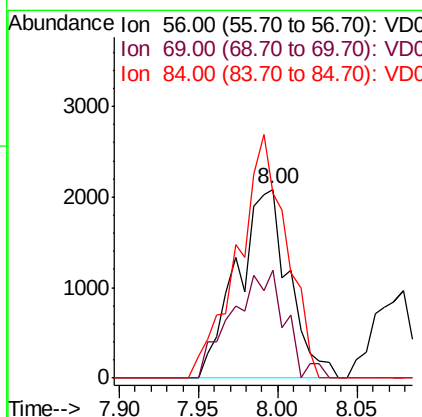





#33
 1,2-Dichloroethane-d4
 Concen: 91.770 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. -0.01 min
 Lab File: VD067773.D
 Acq: 24 Nov 2020 17:37




Instrument :
 MSVOA_D
 ClientSampleId :
 PHC-340EM-013


Tgt Ion: 65 Resp: 40528
 Ion Ratio Lower Upper
 65 100
 67 47.2 0.0 101.0

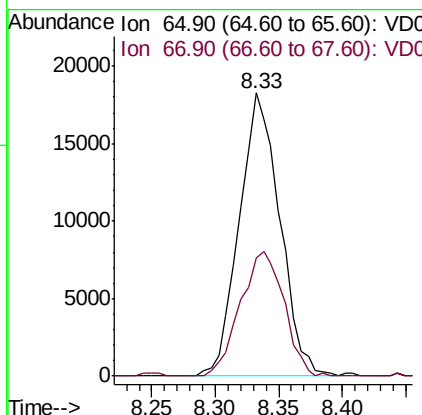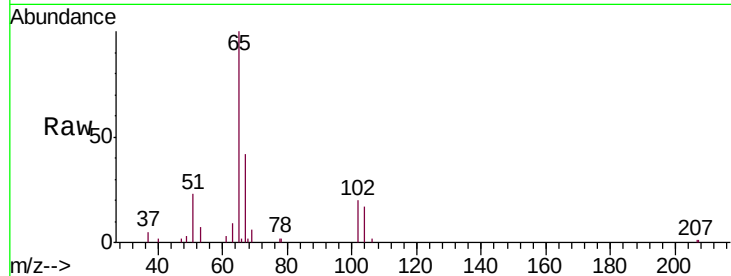

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD067773.D
 Acq: 24 Nov 2020 17:37

Tgt Ion: 114 Resp: 70489
 Ion Ratio Lower Upper
 114 100
 63 15.5 0.0 34.8
 88 16.0 0.0 34.4

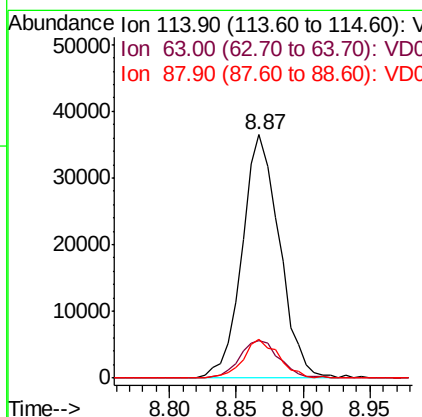



#35

Dibromofluoromethane

Concen: 64.275 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. 0.01 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :

PHC-340EM-013


Tgt Ion:113 Resp: 28833

Ion Ratio Lower Upper

113 100

111 98.4 81.4 122.0




192 23.2 17.0 25.4



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

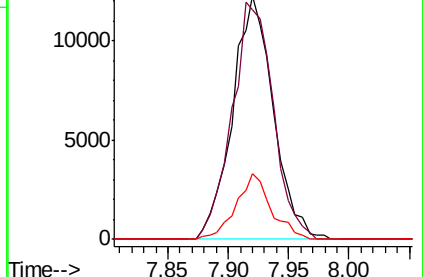

#36

1,1-Dichloropropene

Concen: 4.467 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. -0.13 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37


Tgt Ion: 75 Resp: 2702

Ion Ratio Lower Upper

75 100

110 11.9 20.1 60.2#



77 0.0 24.8 37.2#




Abundance Ion 74.90 (74.60 to 75.60): V

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): V

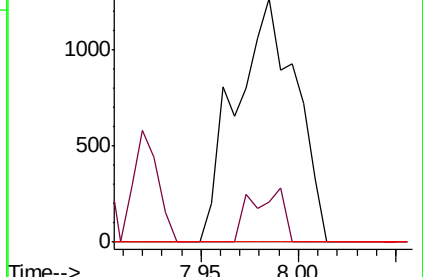







#37
Ethyl Acetate
Concen: 6.991 ug/l
RT: 7.23 min Scan# 902
Delta R.T. -0.08 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013

Tgt Ion: 43 Resp: 1137
Ion Ratio Lower Upper
43 100
61 0.0 12.9 19.3#
70 0.0 12.2 18.2#

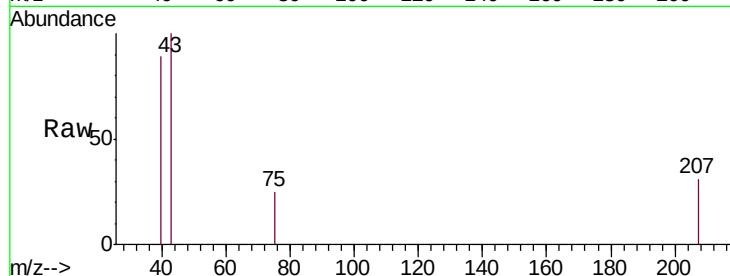


Abundance Ion 43.00 (42.70 to 43.70): VDC
Ion 60.90 (60.60 to 61.60): VDC
Ion 70.00 (69.70 to 70.70): VDC


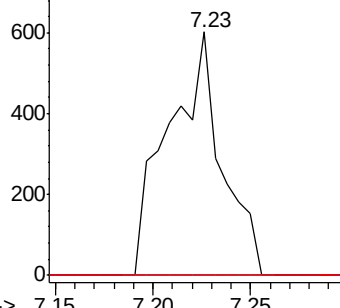



#38
Carbon Tetrachloride
Concen: 5.417 ug/l
RT: 7.99 min Scan# 1032
Delta R.T. -0.11 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion: 117 Resp: 4750
Ion Ratio Lower Upper
117 100
119 0.0 76.6 115.0#
121 0.0 24.5 36.7#



Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V




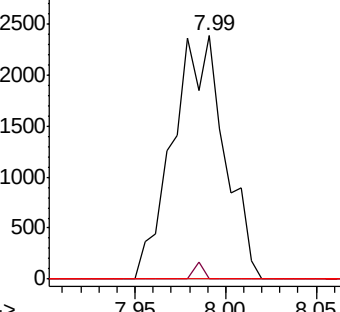




#39
Methylcyclohexane
Concen: 20.646 ug/l
RT: 9.36 min Scan# 1264
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37




Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013


Tgt Ion: 83 Resp: 14779
Ion Ratio Lower Upper
83 100
55 77.2 51.0 76.4#
98 52.6 40.4 60.6

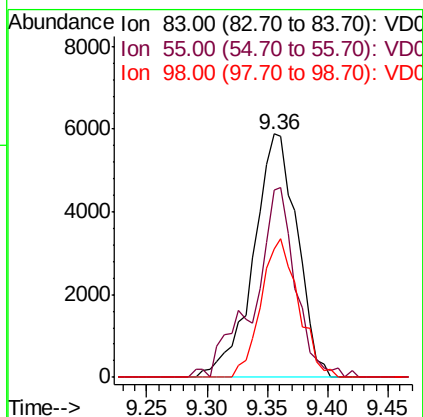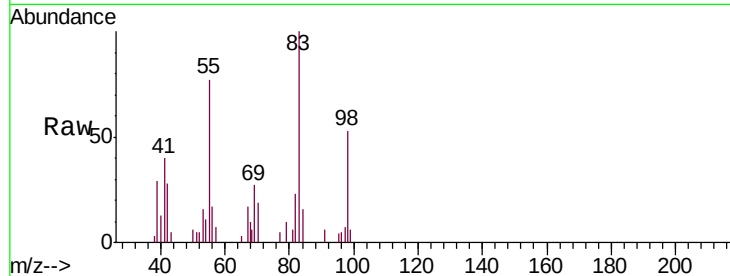

#40
Benzene
Concen: 1.404 ug/l
RT: 8.36 min Scan# 1094
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion: 78 Resp: 2332
Ion Ratio Lower Upper
78 100
77 29.7 17.8 26.6#

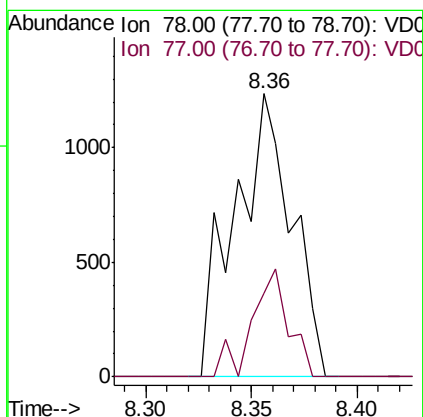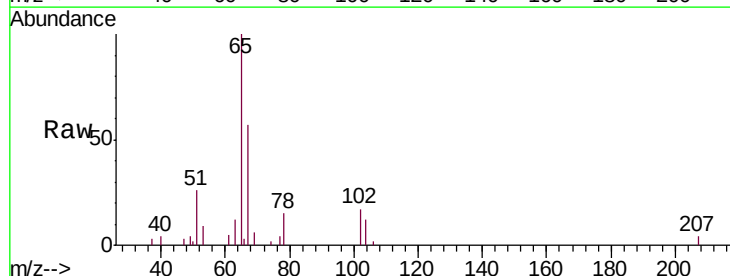



#43

Isopropyl Acetate

Concen: 1.776 ug/l

RT: 8.47 min Scan# 1113

Delta R.T. 0.01 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :

PHC-340EM-013


Tgt Ion: 43 Resp: 577

Ion Ratio Lower Upper




43 100

61 0.0 30.2 45.4#

87 0.0 14.2 21.4#

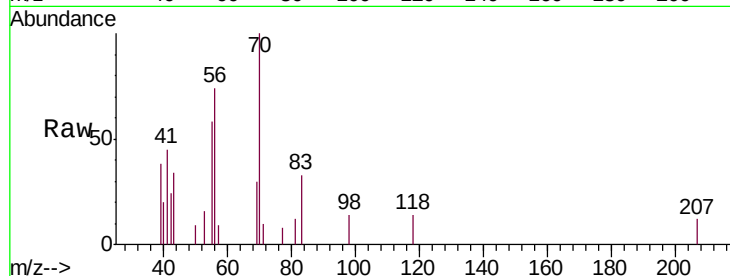

Abundance Ion 43.00 (42.70 to 43.70): VDC
Ion 61.00 (60.70 to 61.70): VDC
Ion 87.00 (86.70 to 87.70): VDC

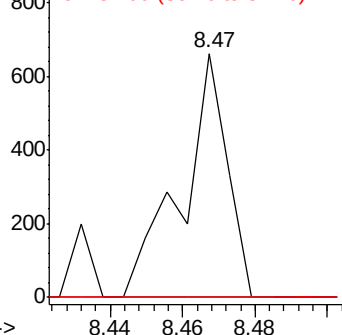

#48

Methyl methacrylate

Concen: 39.585 ug/l

RT: 9.36 min Scan# 1264

Delta R.T. -0.11 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37


Tgt Ion: 41 Resp: 6428

Ion Ratio Lower Upper



41 100


69 46.1 87.8 131.6#

39 71.0 60.5 90.7



Abundance Ion 41.00 (40.70 to 41.70): VDC
Ion 69.00 (68.70 to 69.70): VDC
Ion 39.00 (38.70 to 39.70): VDC




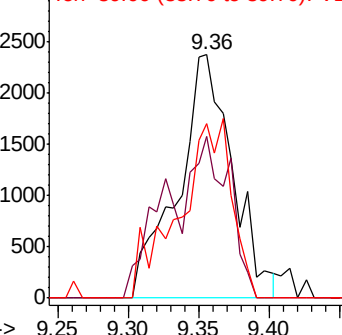




#50
Toluene-d8
Concen: 46.076 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37




Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013


Tgt Ion: 98 Resp: 75568
Ion Ratio Lower Upper
98 100
100 68.2 53.1 79.7

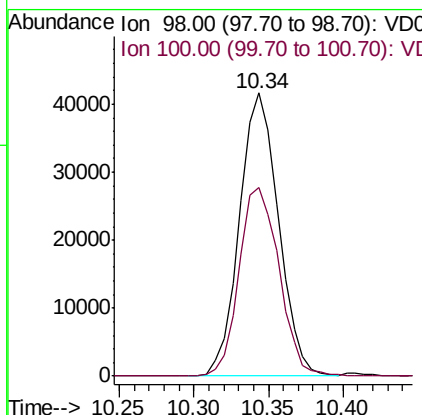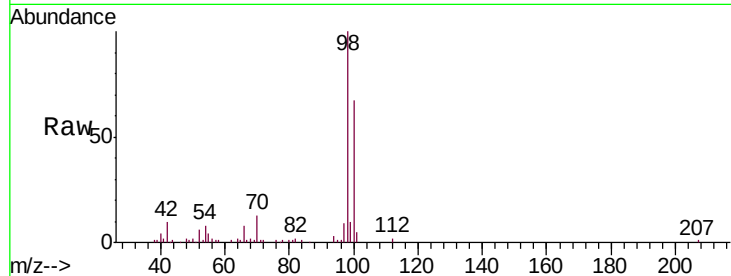

#55
1,1,2-Trichloroethane
Concen: 5.315 ug/l
RT: 10.77 min Scan# 1505
Delta R.T. -0.03 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion: 97 Resp: 1655
Ion Ratio Lower Upper
97 100
83 0.0 60.2 90.4#
85 0.0 40.5 60.7#
99 0.0 50.6 76.0#



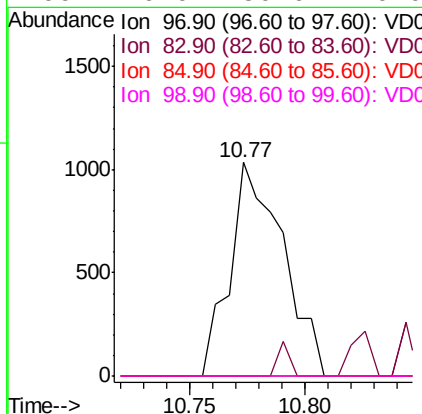





#56
Ethyl methacrylate
Concen: 2.661 ug/l
RT: 10.68 min Scan# 1489
Delta R.T. 0.01 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37




Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013


Tgt Ion: 69 Resp: 858
Ion Ratio Lower Upper
69 100
41 172.4 43.4 65.0#
39 92.8 29.6 44.4#

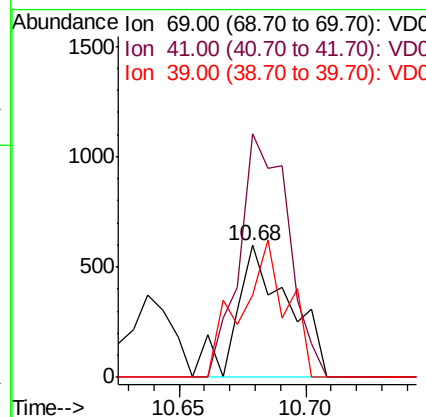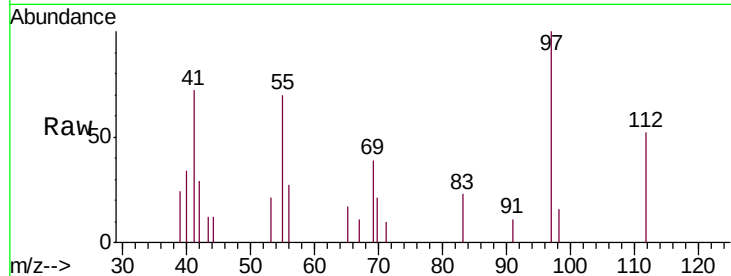

#59
2-Hexanone
Concen: 4.022 ug/l
RT: 10.96 min Scan# 1536
Delta R.T. -0.04 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion: 43 Resp: 434
Ion Ratio Lower Upper
43 100
58 0.0 30.5 91.5#



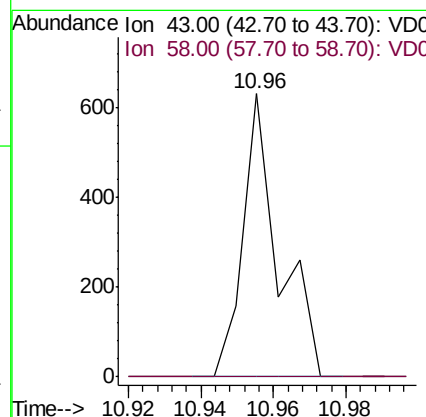
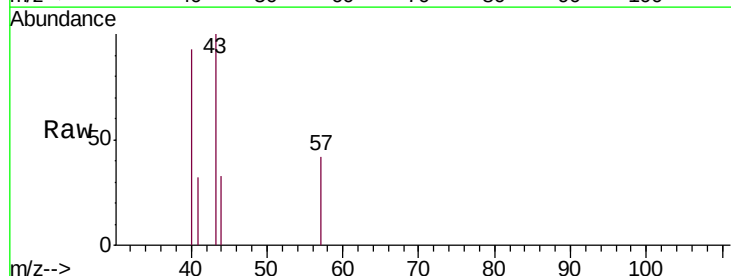




#62
4-Bromofluorobenzene
Concen: 48.233 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37




Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013


Tgt Ion: 95 Resp: 27039
Ion Ratio Lower Upper
95 100
174 96.1 0.0 182.4
176 90.0 0.0 178.2

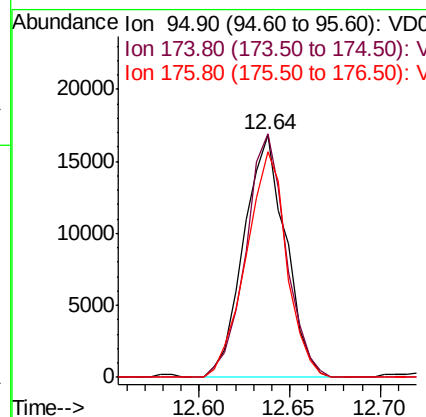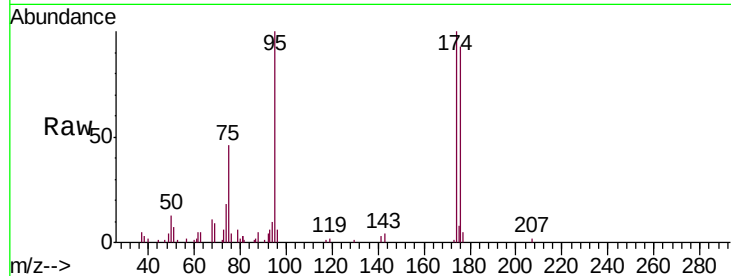

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion: 117 Resp: 69736
Ion Ratio Lower Upper
117 100
82 52.7 40.2 60.4
119 32.1 26.5 39.7



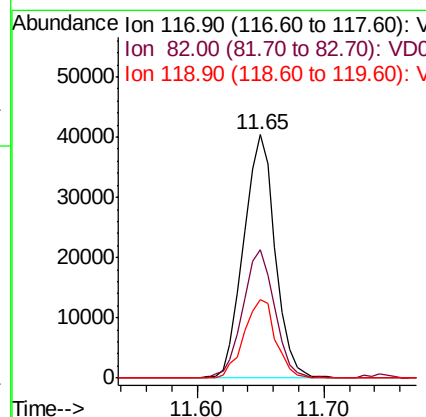





#68
m/p-Xylenes
Concen: 2.724 ug/l
RT: 11.86 min Scan# 1690
Delta R.T. 0.01 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37




Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013


Tgt Ion:106 Resp: 2508
Ion Ratio Lower Upper
106 100
91 186.1 163.0 244.6

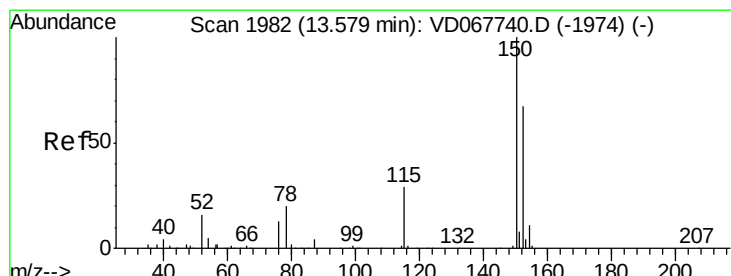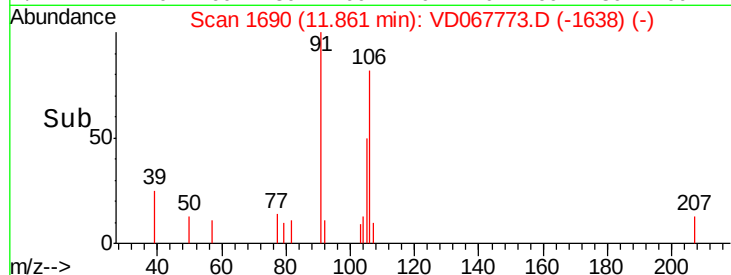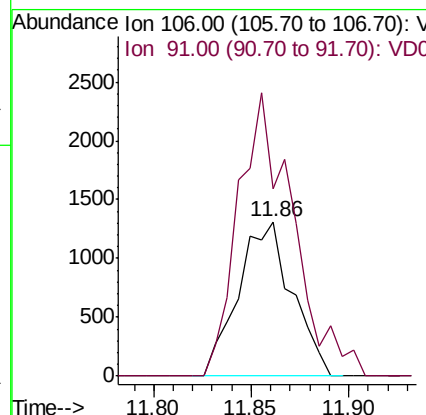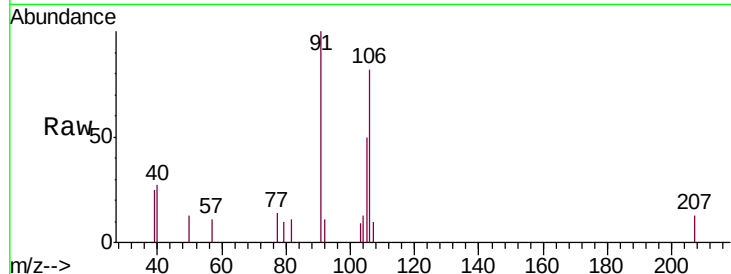

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion:152 Resp: 31322
Ion Ratio Lower Upper
152 100
115 60.2 29.4 88.3
150 151.0 0.0 340.6

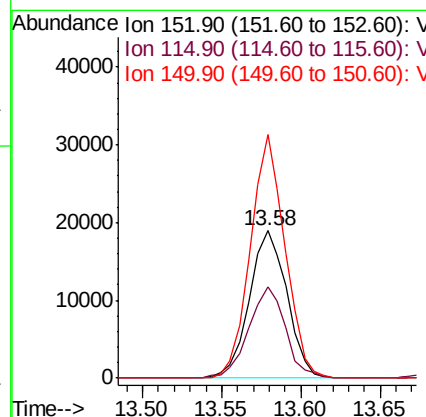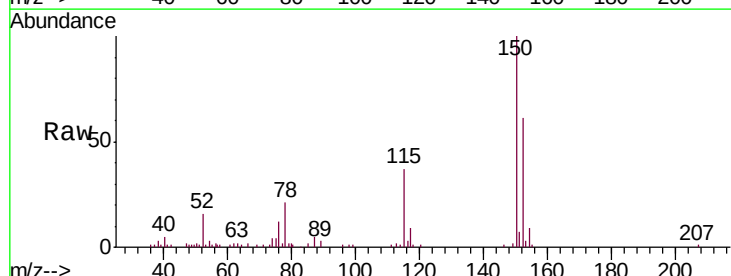



#74

N-ethyl acetate

Concen: 1.188 ug/l

RT: 12.27 min Scan# 1759

Delta R.T. -0.02 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :

PHC-340EM-013

Tgt Ion: 43 Resp: 323


Ion Ratio Lower Upper

43 100

70 0.0 44.6 66.8#

55 0.0 24.2 36.2#

61 0.0 22.0 33.0#

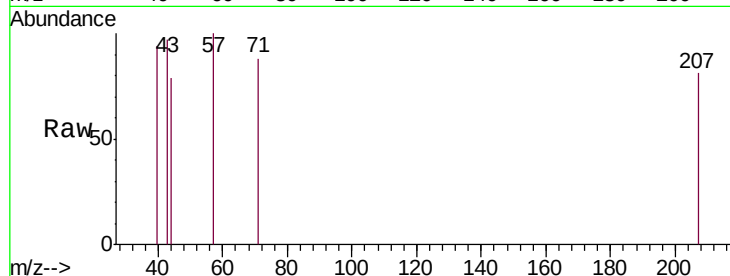




Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 70.00 (69.70 to 70.70): VDC

Ion 55.00 (54.70 to 55.70): VDC

Ion 61.00 (60.70 to 61.70): VDC

Time-->

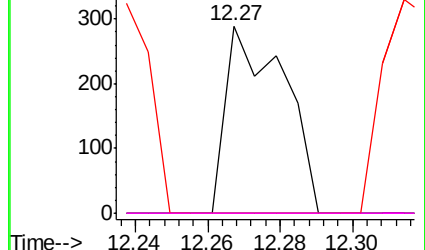

#75

1,1,2,2-Tetrachloroethane

Concen: 1.161 ug/l

RT: 12.80 min Scan# 1850

Delta R.T. 0.06 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37


Tgt Ion: 83 Resp: 321

Ion Ratio Lower Upper

83 100

131 0.0 8.1 24.1#

85 0.0 33.9 101.7#






Abundance Ion 82.90 (82.60 to 83.60): VDC

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VDC

Time-->



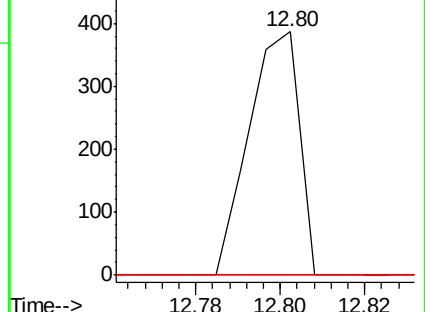



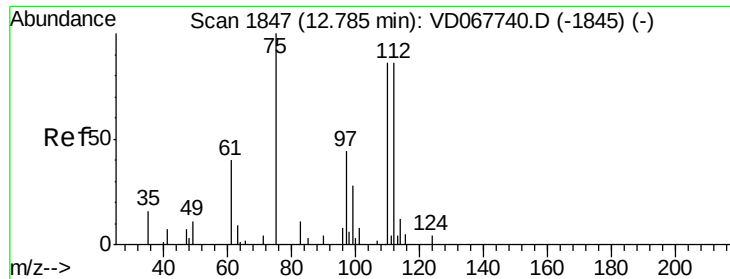

#76
 1,2,3-Trichloropropane
 Concen: 62.460 ug/l
 RT: 12.64 min Scan# 1822
 Delta R.T. -0.15 min
 Lab File: VD067773.D
 Acq: 24 Nov 2020 17:37




Instrument :
 MSVOA_D
 ClientSampleId :
 PHC-340EM-013


Tgt Ion: 75 Resp: 13635
 Ion Ratio Lower Upper
 75 100
 77 0.0 0.0 0.0

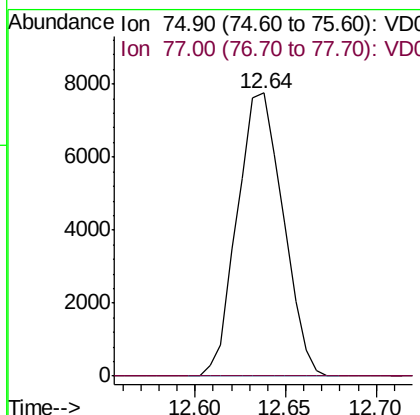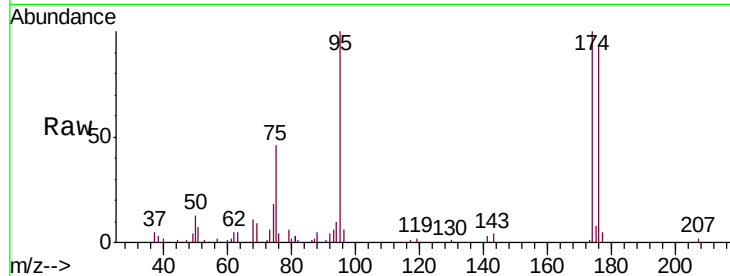

#80
 1,3,5-Trimethylbenzene
 Concen: 1.694 ug/l
 RT: 12.97 min Scan# 1878
 Delta R.T. 0.01 min
 Lab File: VD067773.D
 Acq: 24 Nov 2020 17:37

Tgt Ion: 105 Resp: 3036
 Ion Ratio Lower Upper
 105 100
 120 63.8 23.9 71.7

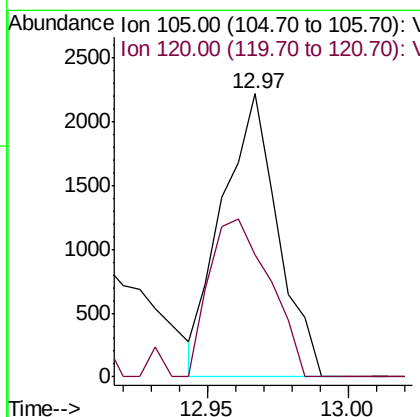

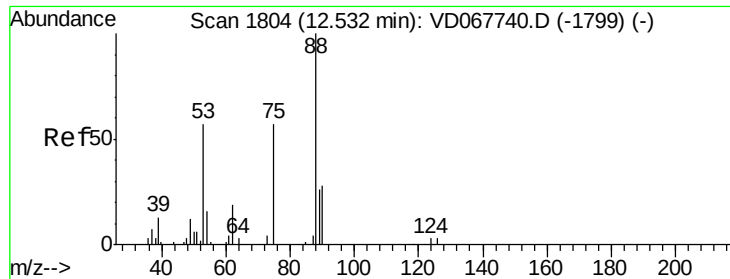

#81

trans-1,4-Dichloro-2-butene

Concen: 146.089 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.11 min

Lab File: VD067773.D

Acq: 24 Nov 2020 17:37

Instrument :

MSVOA_D

ClientSampleId :

PHC-340EM-013


Tgt Ion: 75 Resp: 13635

Ion Ratio Lower Upper

75 100

53 0.5 76.0 114.0#




89 0.0 40.2 60.4#

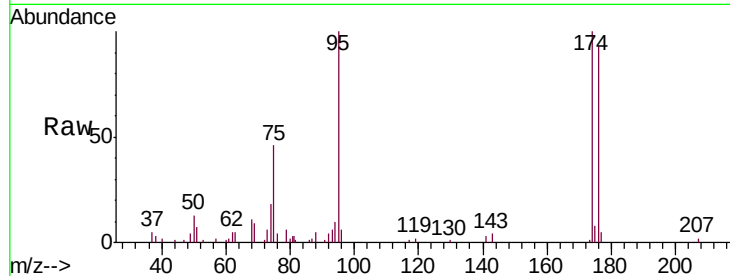

Abundance Ion 74.90 (74.60 to 75.60): VDC

Ion 53.00 (52.70 to 53.70): VDC

Ion 88.90 (88.60 to 89.60): VDC

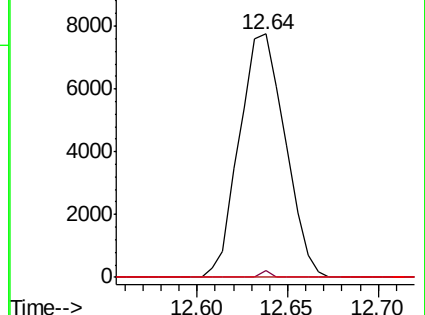

#84

1,2,4-Trimethylbenzene

Concen: 4.175 ug/l

RT: 13.27 min Scan# 1930

Delta R.T. 0.00 min

Lab File: VD067773.D


Acq: 24 Nov 2020 17:37

Tgt Ion: 105 Resp: 7475

Ion Ratio Lower Upper



105 100


120 48.0 22.6 67.7



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V



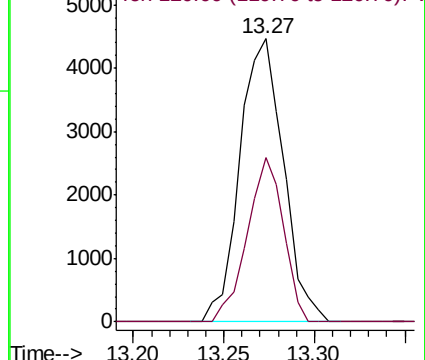





#90
Hexachloroethane
Concen: 2.662 ug/l
RT: 14.12 min Scan# 2074
Delta R.T. 0.01 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Instrument :
MSVOA_D
ClientSampleId :
PHC-340EM-013

Tgt Ion:117 Resp: 993
Ion Ratio Lower Upper
117 100
201 0.0 42.2 126.6#

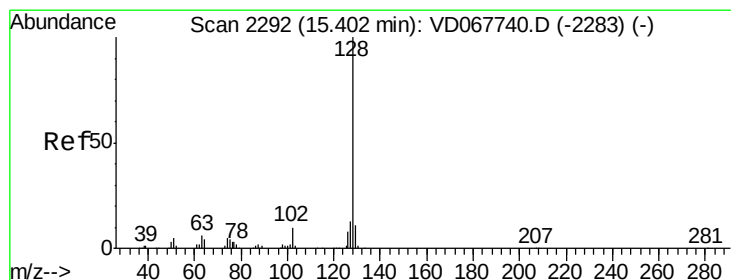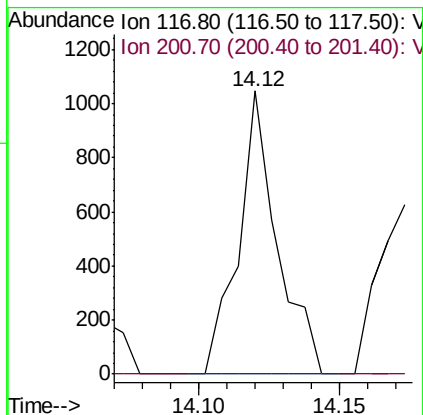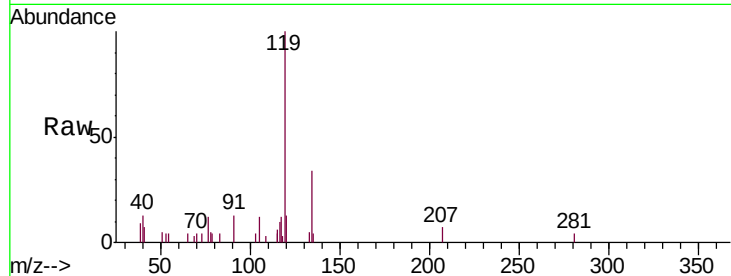

#95
Naphthalene
Concen: 6.068 ug/l
RT: 15.40 min Scan# 2292
Delta R.T. 0.00 min
Lab File: VD067773.D
Acq: 24 Nov 2020 17:37

Tgt Ion:128 Resp: 5980
Ion Ratio Lower Upper
128 100
127 13.8 10.7 16.1
129 12.1 8.6 12.8

