


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD112618\
 Data File : VD060447.D
 Acq On : 26 Nov 2018 10:04
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Title : SW846 8260
 Last Update : Mon Nov 19 16:31:59 2018

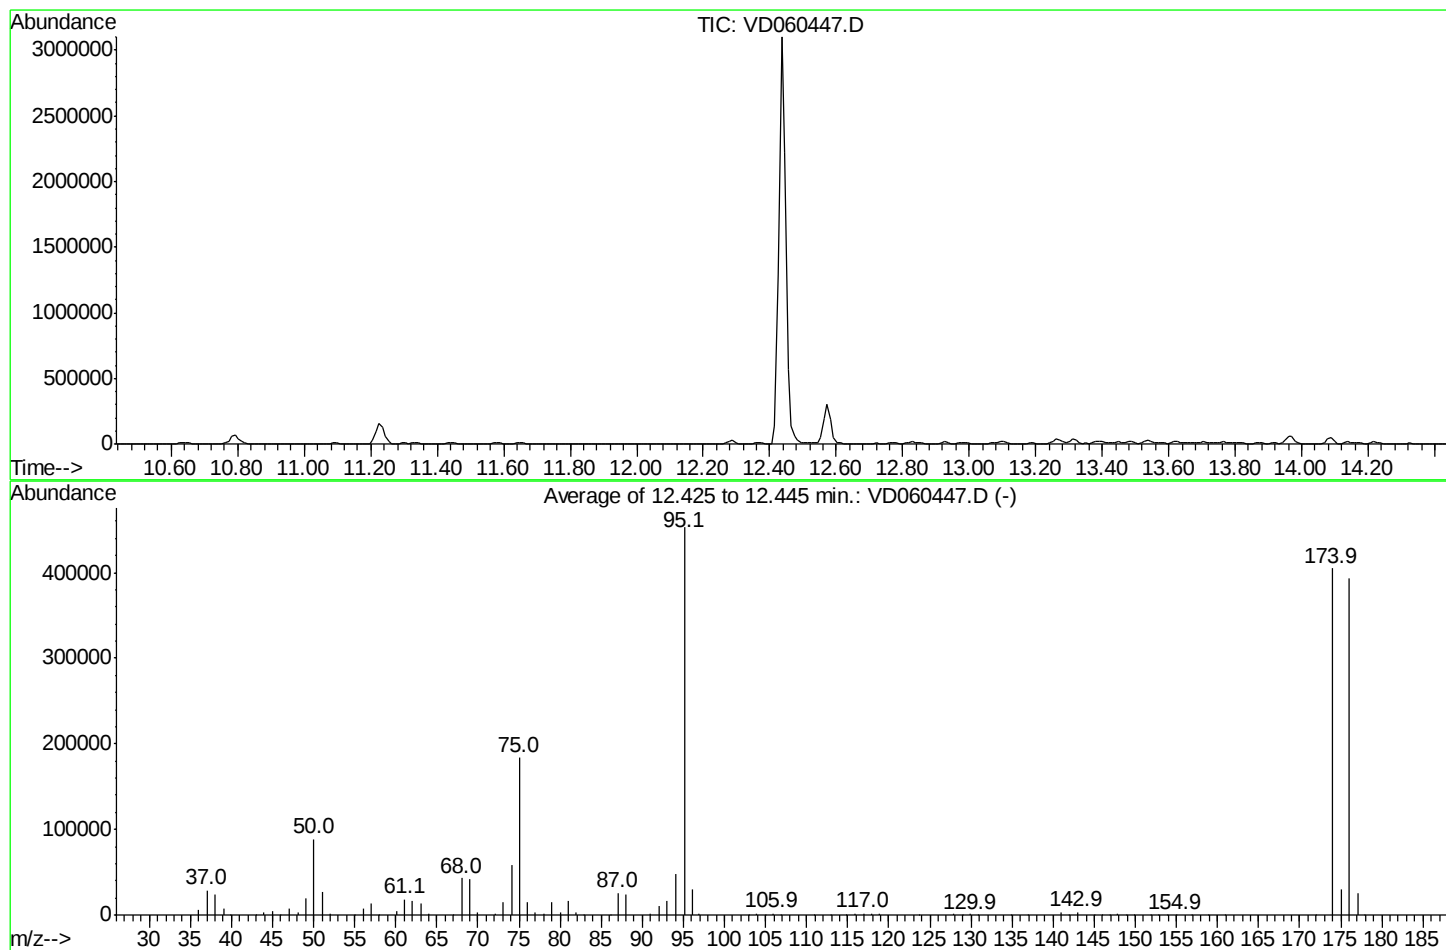

AutoFind: Scans 1108, 1109, 1110; Background Corrected with Scan 1103

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	88624	PASS
75	95	30	60	40.5	183298	PASS
95	95	100	100	100.0	452949	PASS
96	95	5	9	6.7	30349	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.5	405184	PASS
175	174	5	9	7.3	29389	PASS
176	174	95	101	96.9	392746	PASS
177	176	5	9	6.7	26142	PASS