

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD112619\
 Data File : VD064389.D
 Acq On : 26 Nov 2019 17:40
 Operator : VA/SY
 Sample : K6024-06
 Misc : 7.92G/5.00ml/MSVOA D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 B-6-(0.5-1.0)

Quant Time: Nov 27 06:36:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 12 02:43:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.99	168	737393	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	1071231	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	935682	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	423889	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	293262	48.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.72%	
35) Dibromofluoromethane	7.92	113	314729	51.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.36%	
50) Toluene-d8	10.34	98	1257323	54.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.40%	
62) 4-Bromofluorobenzene	12.64	95	383401	47.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.46%	
Target Compounds						
44) Trichloroethene	9.11	130	100368	12.376	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD112619\
Data File : VD064389.D
Acq On : 26 Nov 2019 17:40
Operator : VA/SY
Sample : K6024-06
Misc : 7.92G/5.00ml/MSVOA D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
B-6-(0.5-1.0)

Quant Time: Nov 27 06:36:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110819S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 12 02:43:24 2019
Response via : Initial Calibration

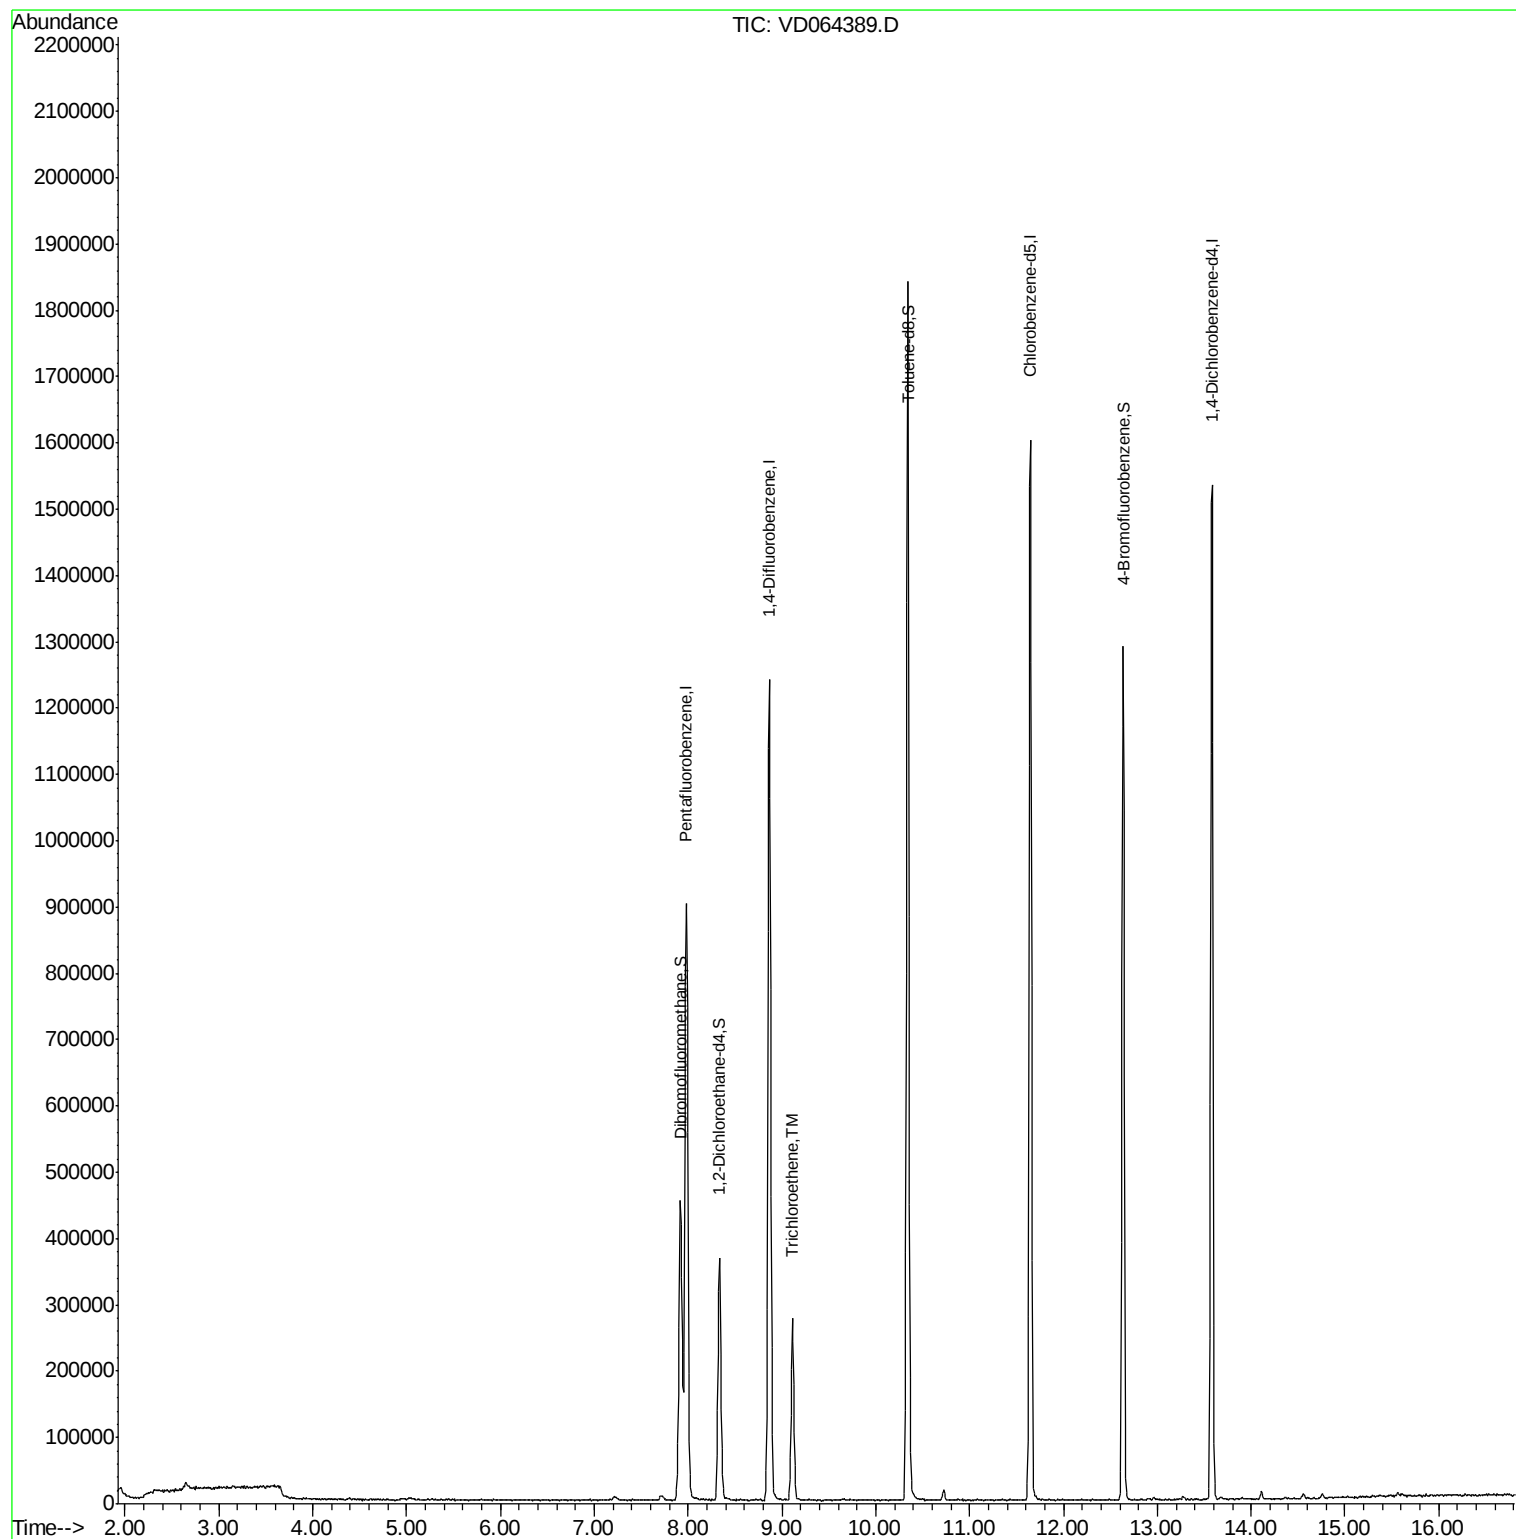

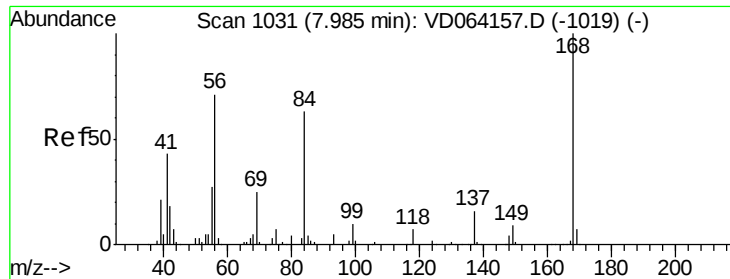

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.99 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD064389.D

Acq: 26 Nov 2019 17:40

Instrument :

MSVOA_D

ClientSampleId :


B-6-(0.5-1.0)

Tot Ion:168 Resp: 737393

Ion Ratio Lower Upper




168 100

99 50.6 41.6 62.4

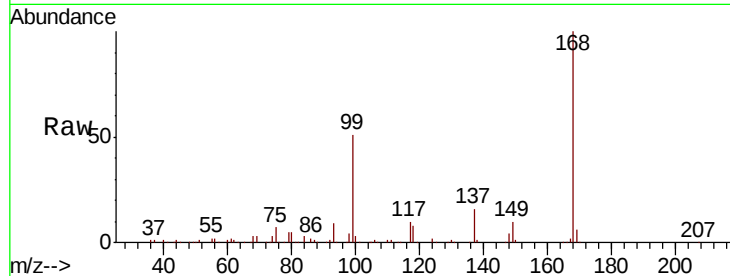

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

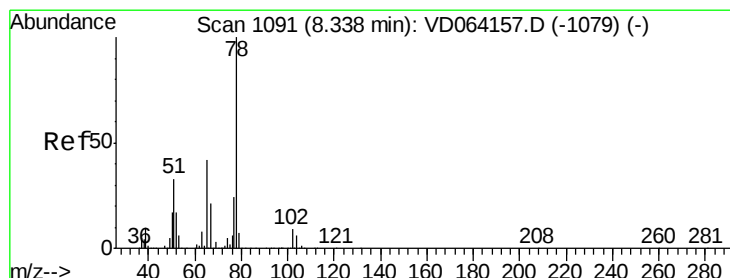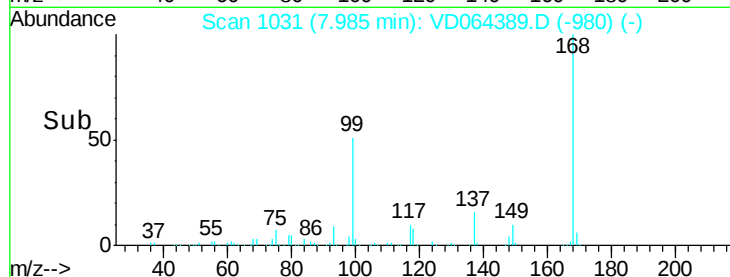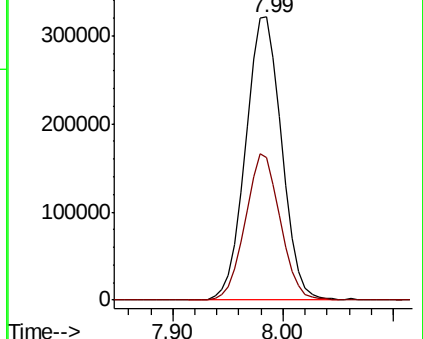

#33

1,2-Dichloroethane-d4

Concen: 48.356 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD064389.D


Acq: 26 Nov 2019 17:40

Tgt Ion: 65 Resp: 293262

Ion Ratio Lower Upper



65 100


67 51.5 0.0 104.4

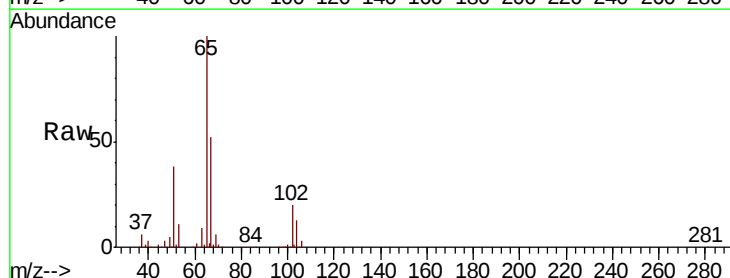

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

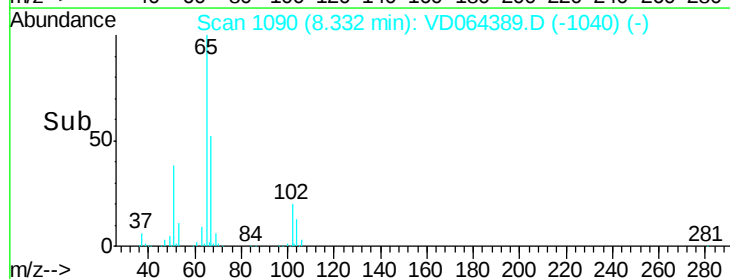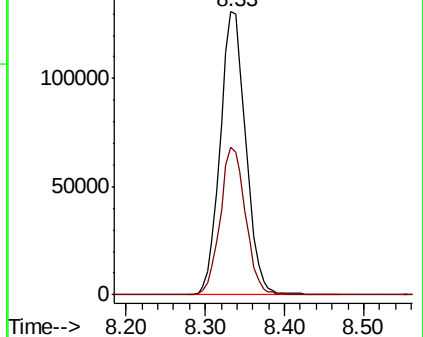


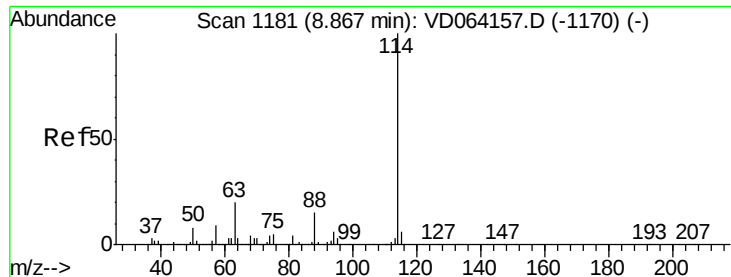




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD064389.D
 Acq: 26 Nov 2019 17:40

Instrument :
 MSVOA_D
 ClientSampleId :
 B-6-(0.5-1.0)

Tot Ion:114 Resp: 1071231
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 40.0
 88 14.8 0.0 30.2

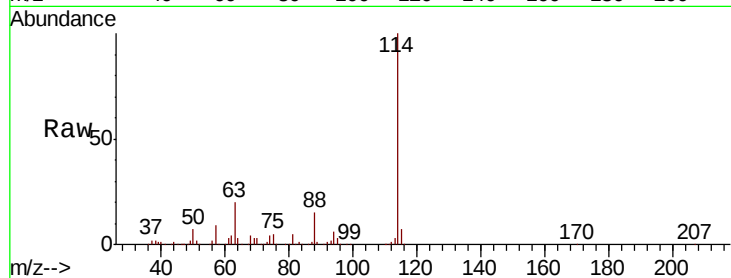


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VDC
 Ion 87.90 (87.60 to 88.60): VDC

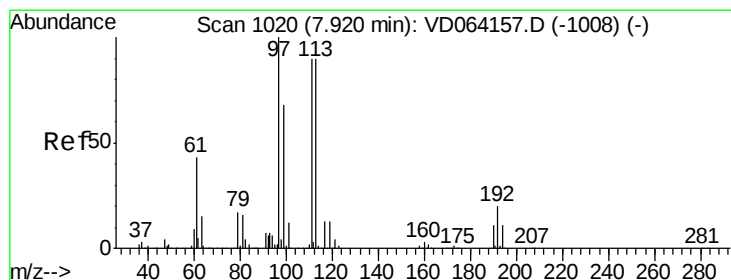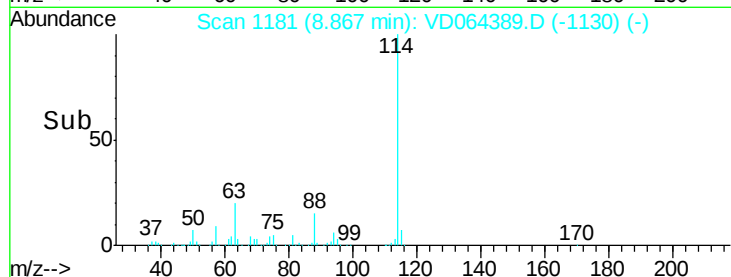
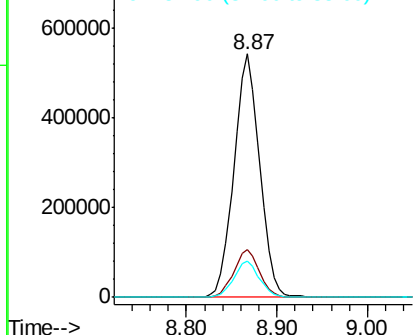



#35
 Dibromofluoromethane
 Concen: 51.183 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD064389.D
 Acq: 26 Nov 2019 17:40

Tgt Ion:113 Resp: 314729
 Ion Ratio Lower Upper
 113 100
 111 103.7 81.5 122.3
 192 22.8 18.8 28.2

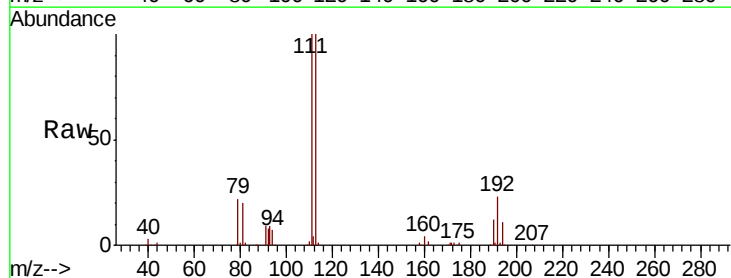

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

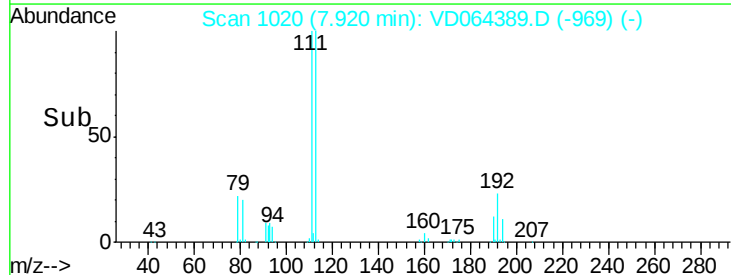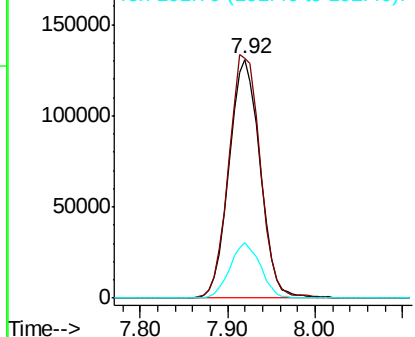

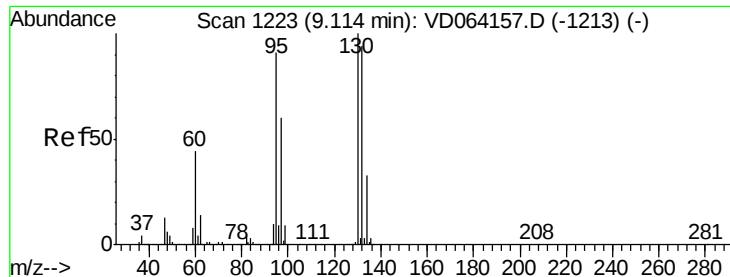

#44

Trichloroethene

Concen: 12.376 ug/l

RT: 9.11 min Scan# 1223

Delta R.T. 0.00 min

Lab File: VD064389.D

Acq: 26 Nov 2019 17:40

Instrument :

MSVOA_D

ClientSampleId :


B-6-(0.5-1.0)

Tot Ion:130 Resp: 100368

Ion Ratio Lower Upper

130 100

95 86.7 0.0 181.6

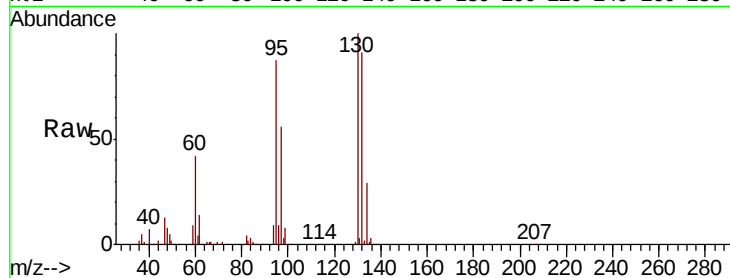

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VDC

9.11

60000

50000

40000

30000



20000

10000

0

Time-->

9.05 9.10 9.15 9.20

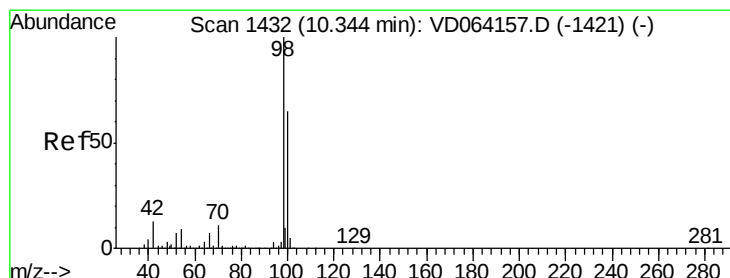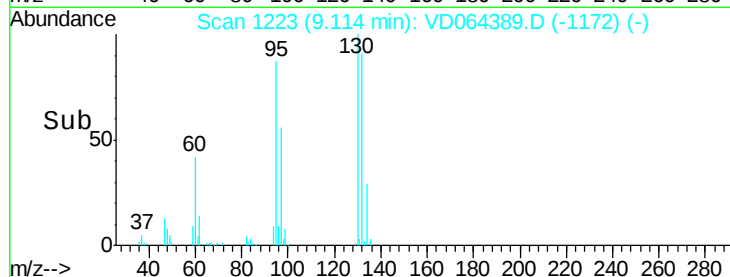

#50

Toluene-d8

Concen: 54.202 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD064389.D


Acq: 26 Nov 2019 17:40

Tgt Ion: 98 Resp: 1257323

Ion Ratio Lower Upper

98 100

100 65.5 52.6 78.8

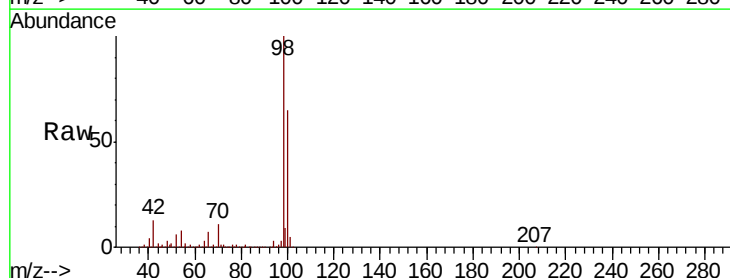

Abundance Ion 98.00 (97.70 to 98.70): VDC

Ion 100.00 (99.70 to 100.70): VD

10.34

800000

600000


400000


200000

0

Time-->

10.20 10.30 10.40 10.50

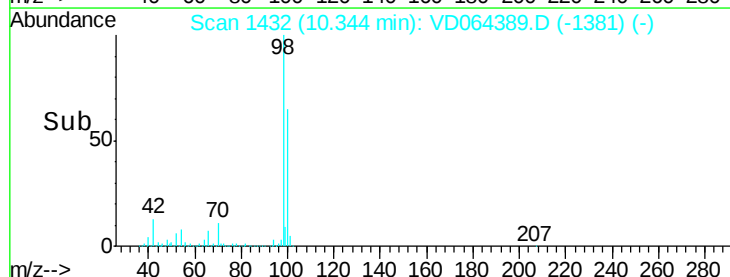

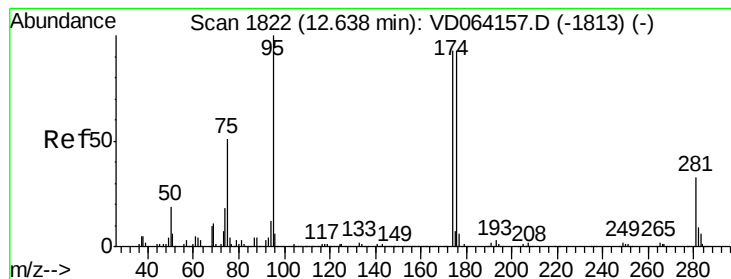

#62

4-Bromofluorobenzene

Concen: 47.727 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD064389.D

Acq: 26 Nov 2019 17:40

Instrument :

MSVOA_D

ClientSampleId :

B-6-(0.5-1.0)


Tot Ion: 95 Resp: 383401

Ion Ratio Lower Upper

95 100

174 97.3 0.0 183.6




176 94.1 0.0 180.2

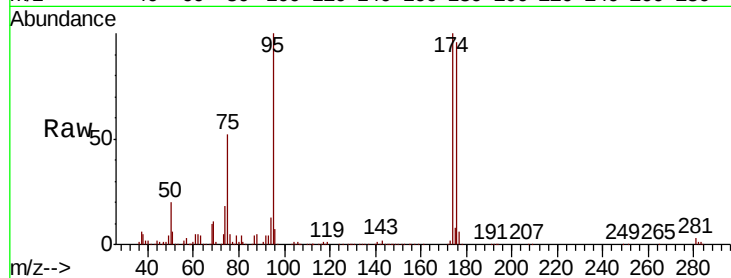

Abundance Ion 94.90 (94.60 to 95.60): V

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

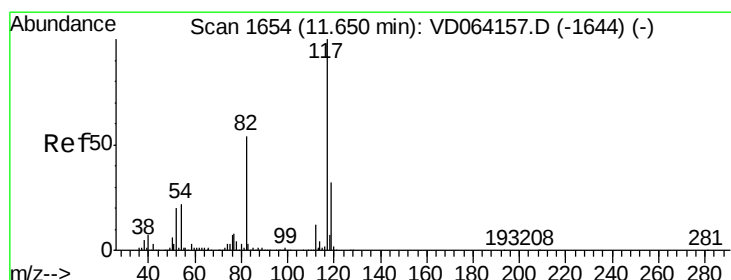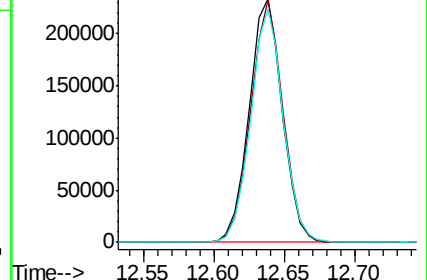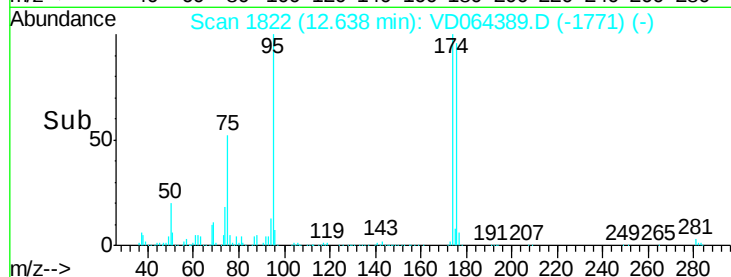

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.65 min Scan# 1654

Delta R.T. 0.00 min

Lab File: VD064389.D

Acq: 26 Nov 2019 17:40


Tgt Ion: 117 Resp: 935682

Ion Ratio Lower Upper

117 100

82 51.0 42.8 64.2



119 32.6 25.6 38.4

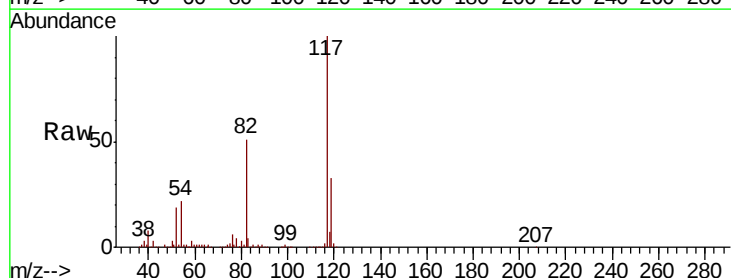


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

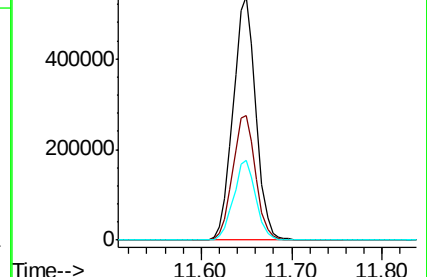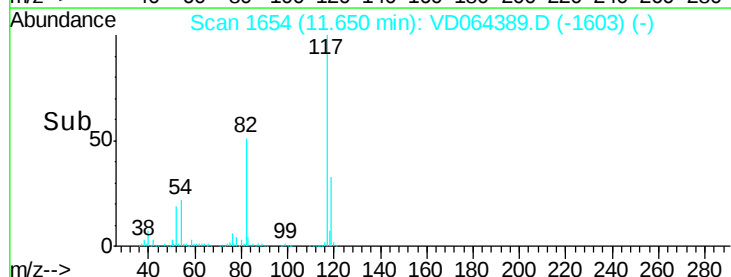

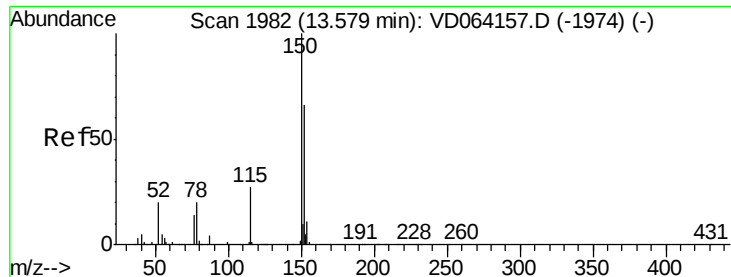

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.01 min

Lab File: VD064389.D

Acq: 26 Nov 2019 17:40

Instrument :

MSVOA_D

ClientSampleId :

B-6-(0.5-1.0)


Tot Ion:152 Resp: 423889

Ion Ratio Lower Upper

152 100

115 55.0 27.4 82.2

150 159.3 0.0 351.6

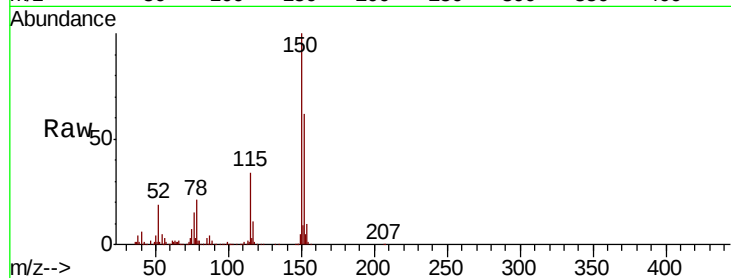

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

