


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD112619\  
Data File : VD064374.D  
Acq On : 26 Nov 2019 09:26  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D110819S.M  
Title : SW846 8260  
Last Update : Tue Nov 12 02:43:24 2019

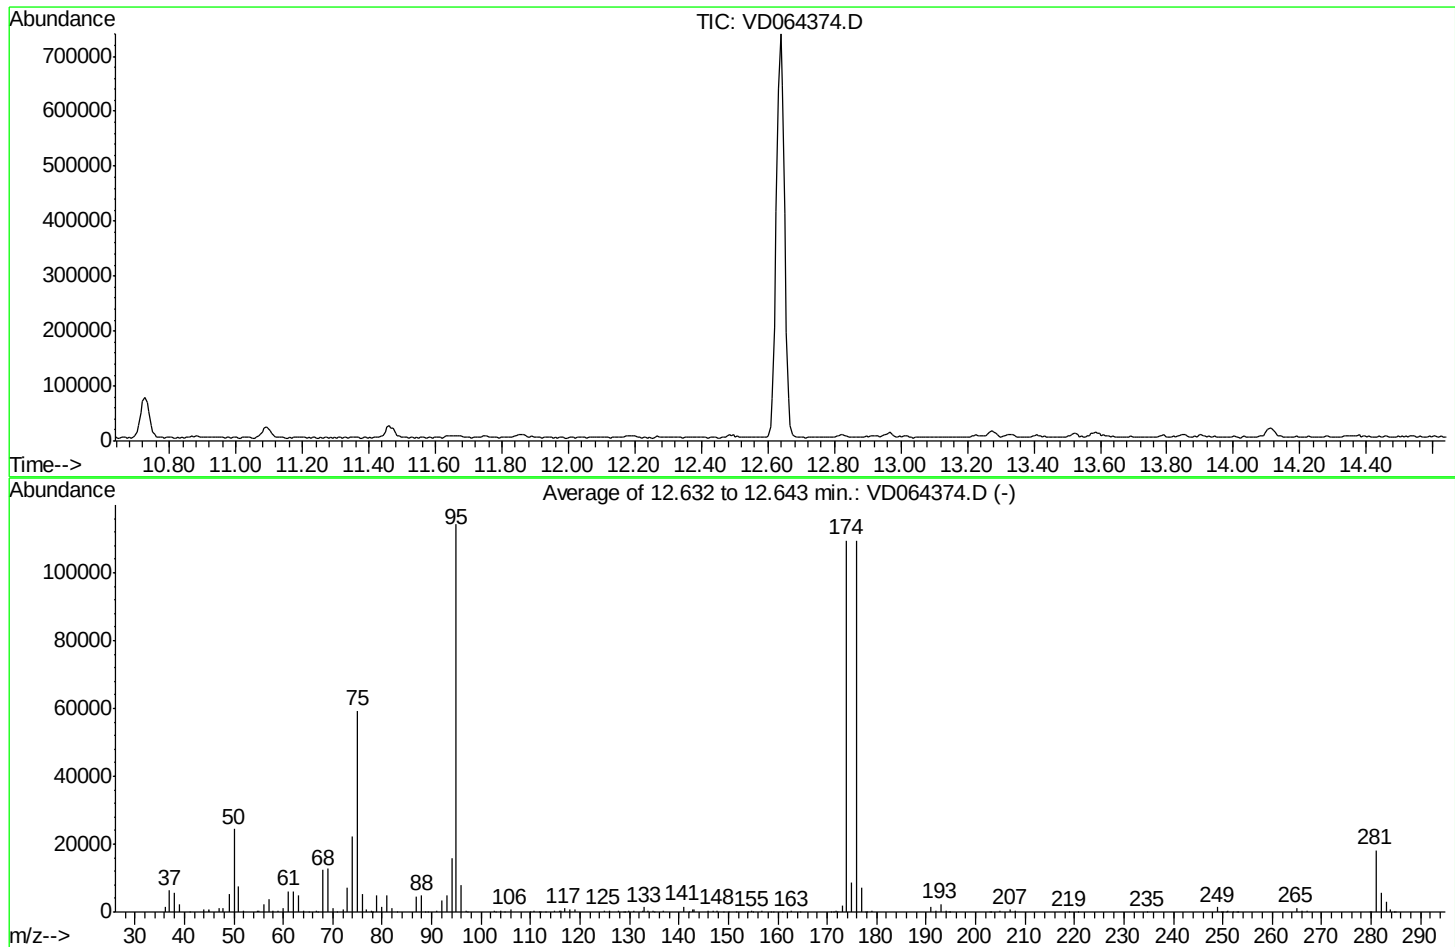

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 21.4      | 24474   | PASS             |
| 75          | 95           | 30           | 60           | 52.0      | 59416   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 114288  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 7931    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.8       | 1955    | PASS             |
| 174         | 95           | 50           | 100          | 95.8      | 109509  | PASS             |
| 175         | 174          | 5            | 9            | 7.8       | 8569    | PASS             |
| 176         | 174          | 95           | 101          | 99.9      | 109445  | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 7369    | PASS             |